

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024903.D
 Acq On : 23 Oct 2021 18:12
 Operator : JC/MD
 Sample : M4303-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P014-TW001-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	31	34	39	rVB3	2573	2690	1.07%	0.123%
2	1.367	42	46	52	rBV	19943	22574	8.94%	1.028%
3	1.672	92	96	101	rVB	17007	20004	7.93%	0.911%
4	2.312	194	201	208	rBV	50499	82099	32.53%	3.739%
5	4.477	547	556	574	rBV2	24101	85556	33.90%	3.897%
6	4.739	589	599	608	rBV4	3775	11712	4.64%	0.533%
7	5.068	641	653	667	rVB2	40693	125220	49.62%	5.703%
8	5.982	788	803	814	rBV2	86726	252370	100.00%	11.494%
9	6.769	922	932	946	rVB	86127	207250	82.12%	9.439%
10	7.317	1013	1022	1034	rBV	54369	122519	48.55%	5.580%
11	8.329	1181	1188	1199	rBV	27718	47423	18.79%	2.160%
12	8.653	1233	1241	1248	rBV	137284	215297	85.31%	9.806%
13	8.726	1248	1253	1258	rVB4	2599	4177	1.66%	0.190%
14	8.951	1285	1290	1299	rBV3	17559	30089	11.92%	1.370%
15	9.390	1354	1362	1376	rBV	151609	224371	88.91%	10.219%
16	10.055	1466	1471	1479	rBV	173738	241154	95.56%	10.983%
17	11.195	1653	1658	1664	rBV2	57783	73423	29.09%	3.344%
18	11.317	1675	1678	1682	rBV2	2472	3066	1.21%	0.140%
19	12.024	1788	1794	1800	rBV	188538	234673	92.99%	10.688%
20	12.323	1836	1843	1850	rVB	145045	189990	75.28%	8.653%


Sum of corrected areas: 2195657

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024903.D
Acq On : 23 Oct 2021 18:12
Operator : JC/MD
Sample : M4303-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P014-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

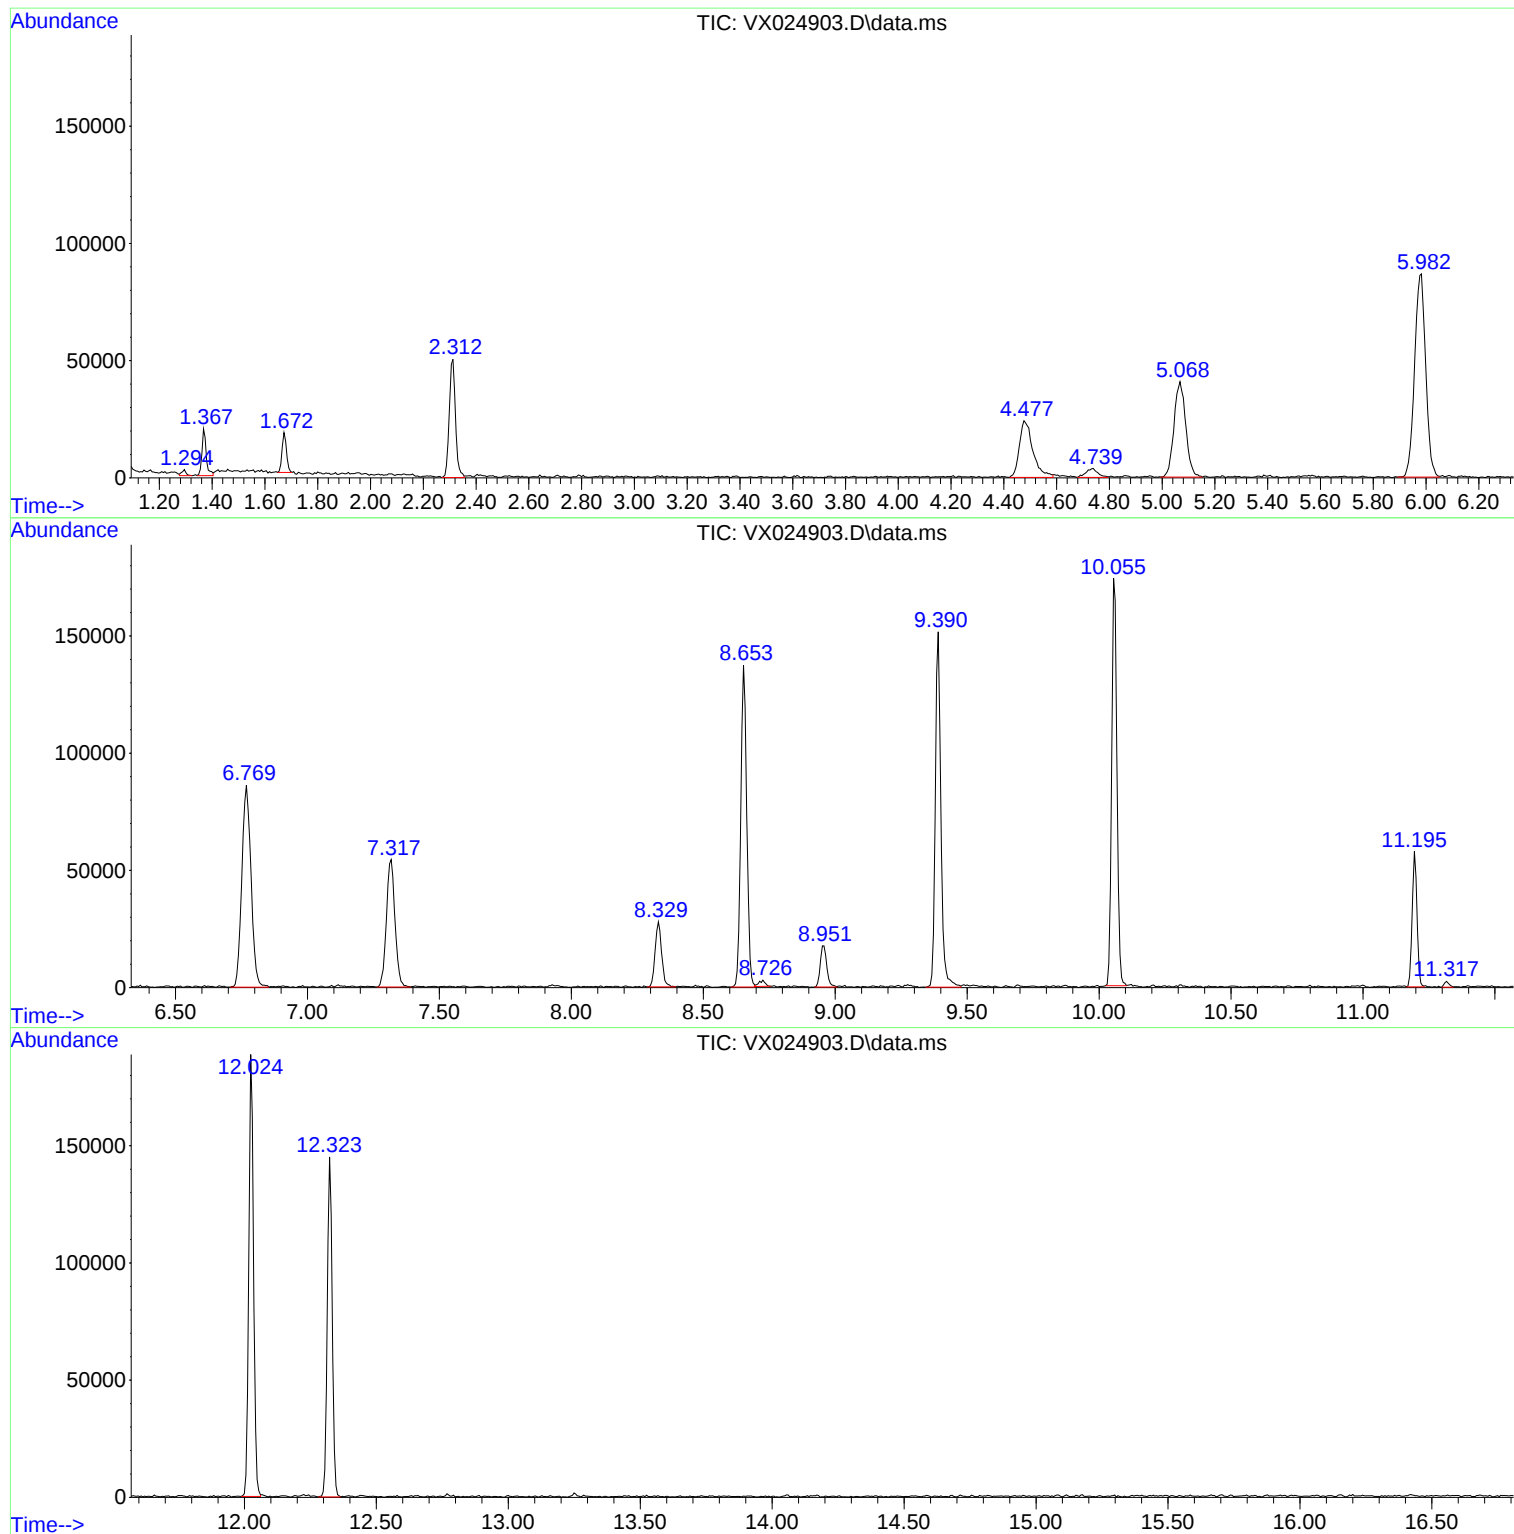

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024903.D
Acq On : 23 Oct 2021 18:12
Operator : JC/MD
Sample : M4303-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P014-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024903.D
Acq On : 23 Oct 2021 18:12
Operator : JC/MD
Sample : M4303-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P014-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
