

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024904.D
 Acq On : 23 Oct 2021 18:36
 Operator : JC/MD
 Sample : M4303-12
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P015-TW001-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	31	34	36	rVB	4984	4894	2.06%	0.241%
2	1.368	41	46	51	rBV	19771	20521	8.63%	1.010%
3	1.672	92	96	101	rBV	16689	20862	8.77%	1.027%
4	2.306	192	200	212	rBV	44847	74467	31.30%	3.664%
5	4.483	547	557	573	rBV	22091	77213	32.46%	3.799%
6	5.068	642	653	666	rBV2	37747	118195	49.68%	5.816%
7	5.983	783	803	816	rBV3	79403	237903	100.00%	11.706%
8	6.769	923	932	952	rVB	84537	200695	84.36%	9.875%
9	7.312	1012	1021	1033	rBV3	50273	112902	47.46%	5.555%
10	8.330	1181	1188	1197	rBV2	25226	42041	17.67%	2.069%
11	8.653	1234	1241	1249	rBV	121156	190031	79.88%	9.351%
12	8.726	1249	1253	1259	rVB3	2574	4663	1.96%	0.229%
13	8.958	1285	1291	1299	rVB	17133	26029	10.94%	1.281%
14	9.281	1335	1344	1347	rBV4	2496	3813	1.60%	0.188%
15	9.391	1354	1362	1374	rBV	138700	205851	86.53%	10.129%
16	10.055	1464	1471	1480	rBV	165677	230472	96.88%	11.340%
17	11.195	1652	1658	1665	rVB	52763	67368	28.32%	3.315%
18	11.323	1673	1679	1682	rVB	2107	2619	1.10%	0.129%
19	12.024	1788	1794	1806	rVB	174732	221111	92.94%	10.880%
20	12.323	1837	1843	1851	rBV	132766	170658	71.73%	8.397%


Sum of corrected areas: 2032308

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024904.D
Acq On : 23 Oct 2021 18:36
Operator : JC/MD
Sample : M4303-12
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P015-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

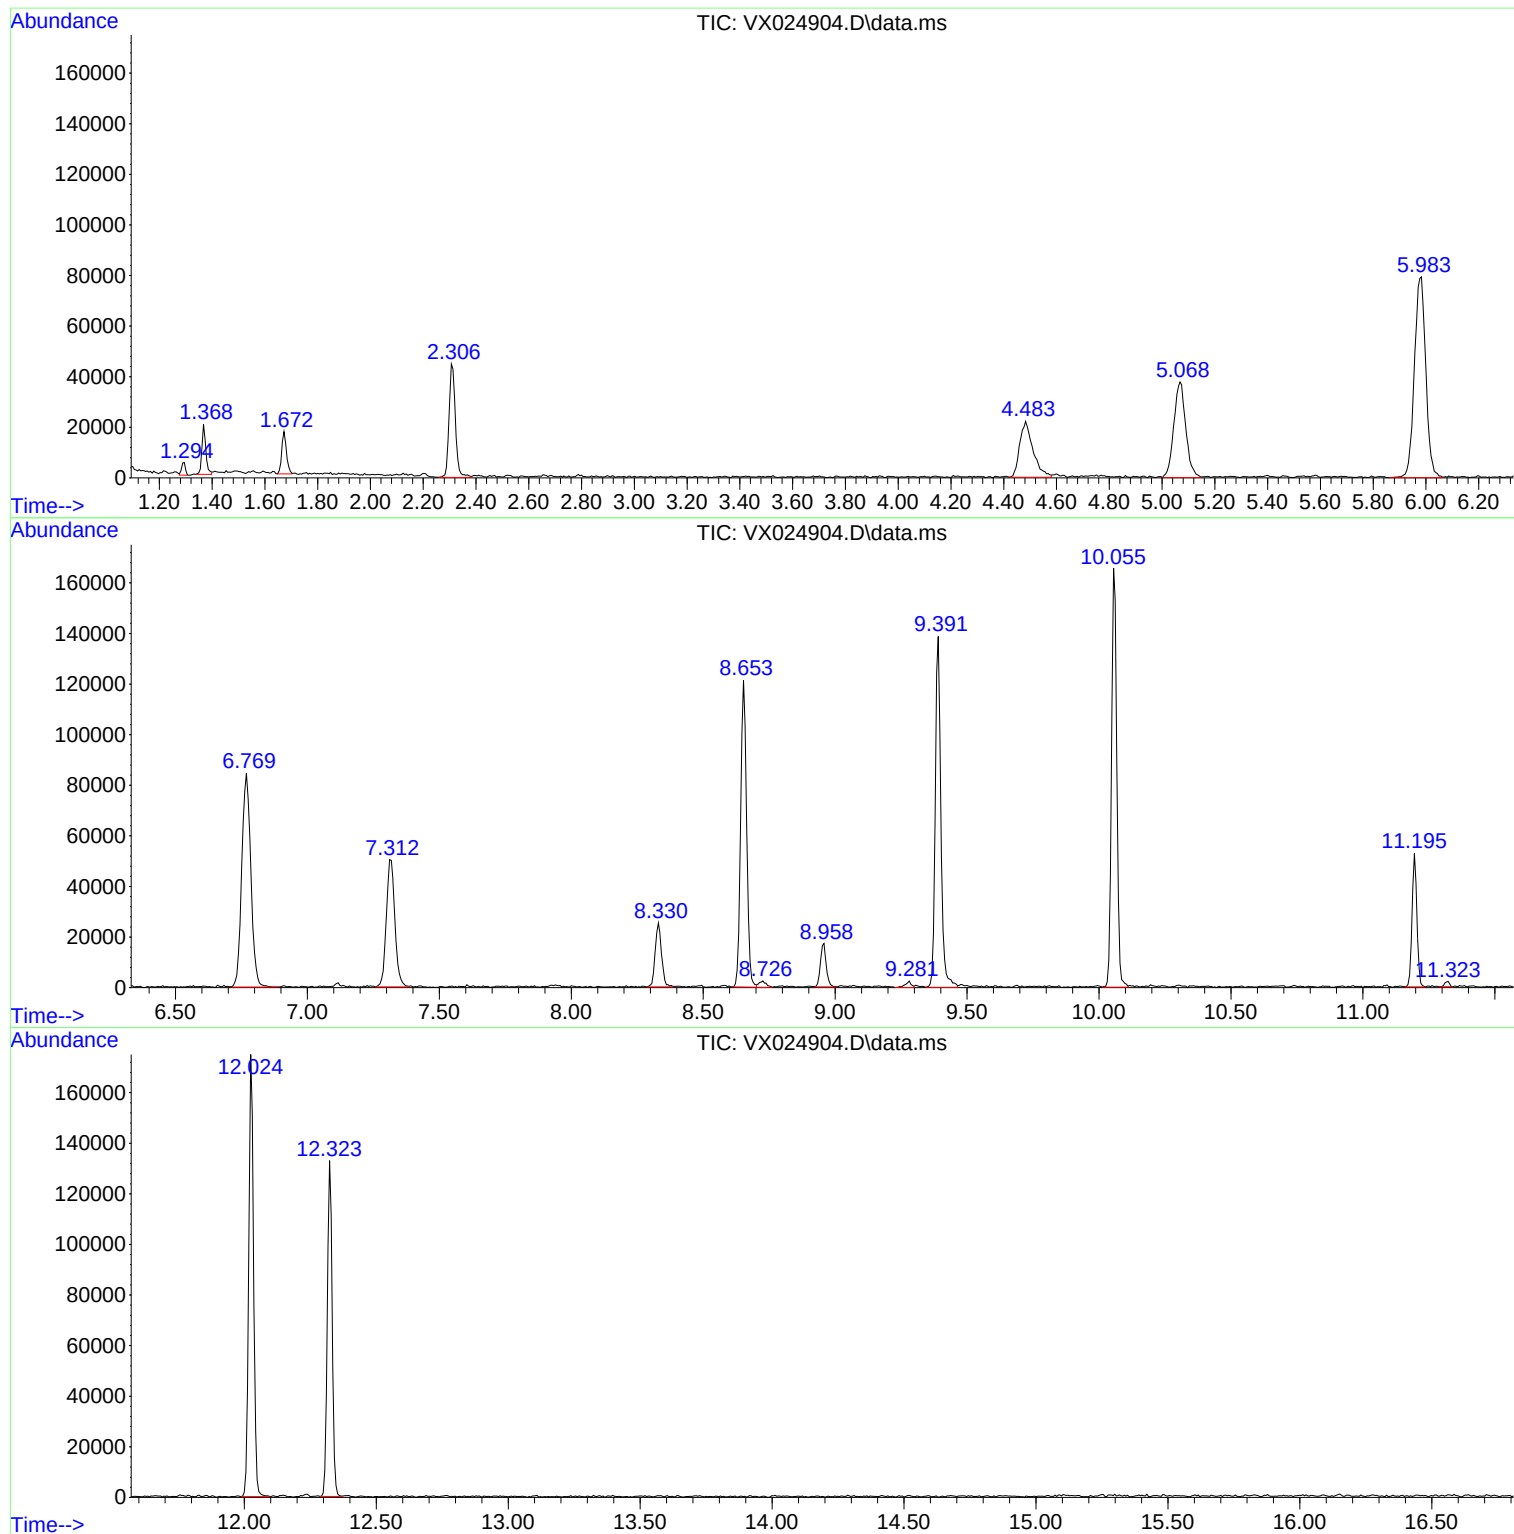

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024904.D
Acq On : 23 Oct 2021 18:36
Operator : JC/MD
Sample : M4303-12
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P015-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024904.D
Acq On : 23 Oct 2021 18:36
Operator : JC/MD
Sample : M4303-12
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P015-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
