

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024907.D
 Acq On : 23 Oct 2021 19:47
 Operator : JC/MD
 Sample : M4303-15
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P021-TW001-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	50	rBV	19015	18423	7.60%	0.898%
2	1.673	92	96	102	rBV	16210	20552	8.48%	1.002%
3	2.313	195	201	208	rBV	44559	73633	30.38%	3.591%
4	4.483	547	557	572	rBV	22087	76773	31.68%	3.744%
5	4.733	592	598	599	rBV2	2290	3307	1.36%	0.161%
6	5.068	639	653	668	rBV2	36556	116390	48.03%	5.676%
7	5.977	788	802	813	rBV4	76208	228135	94.14%	11.126%
8	6.769	921	932	944	rBV2	84226	206536	85.23%	10.072%
9	7.318	1013	1022	1030	rBV2	50620	110646	45.66%	5.396%
10	8.330	1183	1188	1194	rVB	24345	41328	17.05%	2.015%
11	8.653	1233	1241	1249	rBV	123854	192315	79.36%	9.379%
12	8.726	1249	1253	1259	rVB2	3834	6231	2.57%	0.304%
13	8.958	1286	1291	1298	rBV2	16640	24951	10.30%	1.217%
14	9.281	1338	1344	1348	rBV3	1670	2983	1.23%	0.145%
15	9.391	1356	1362	1382	rBV	132796	202221	83.45%	9.862%
16	10.055	1466	1471	1481	rBV	175707	242340	100.00%	11.818%
17	10.305	1508	1512	1517	rBV2	1970	2958	1.22%	0.144%
18	11.195	1650	1658	1663	rBV2	50856	68213	28.15%	3.327%
19	11.317	1673	1678	1682	rVB2	2614	3526	1.45%	0.172%
20	12.024	1787	1794	1802	rBV	189443	237372	97.95%	11.576%
21	12.323	1837	1843	1849	rBV	136976	171683	70.84%	8.373%


Sum of corrected areas: 2050516

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024907.D
Acq On : 23 Oct 2021 19:47
Operator : JC/MD
Sample : M4303-15
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P021-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

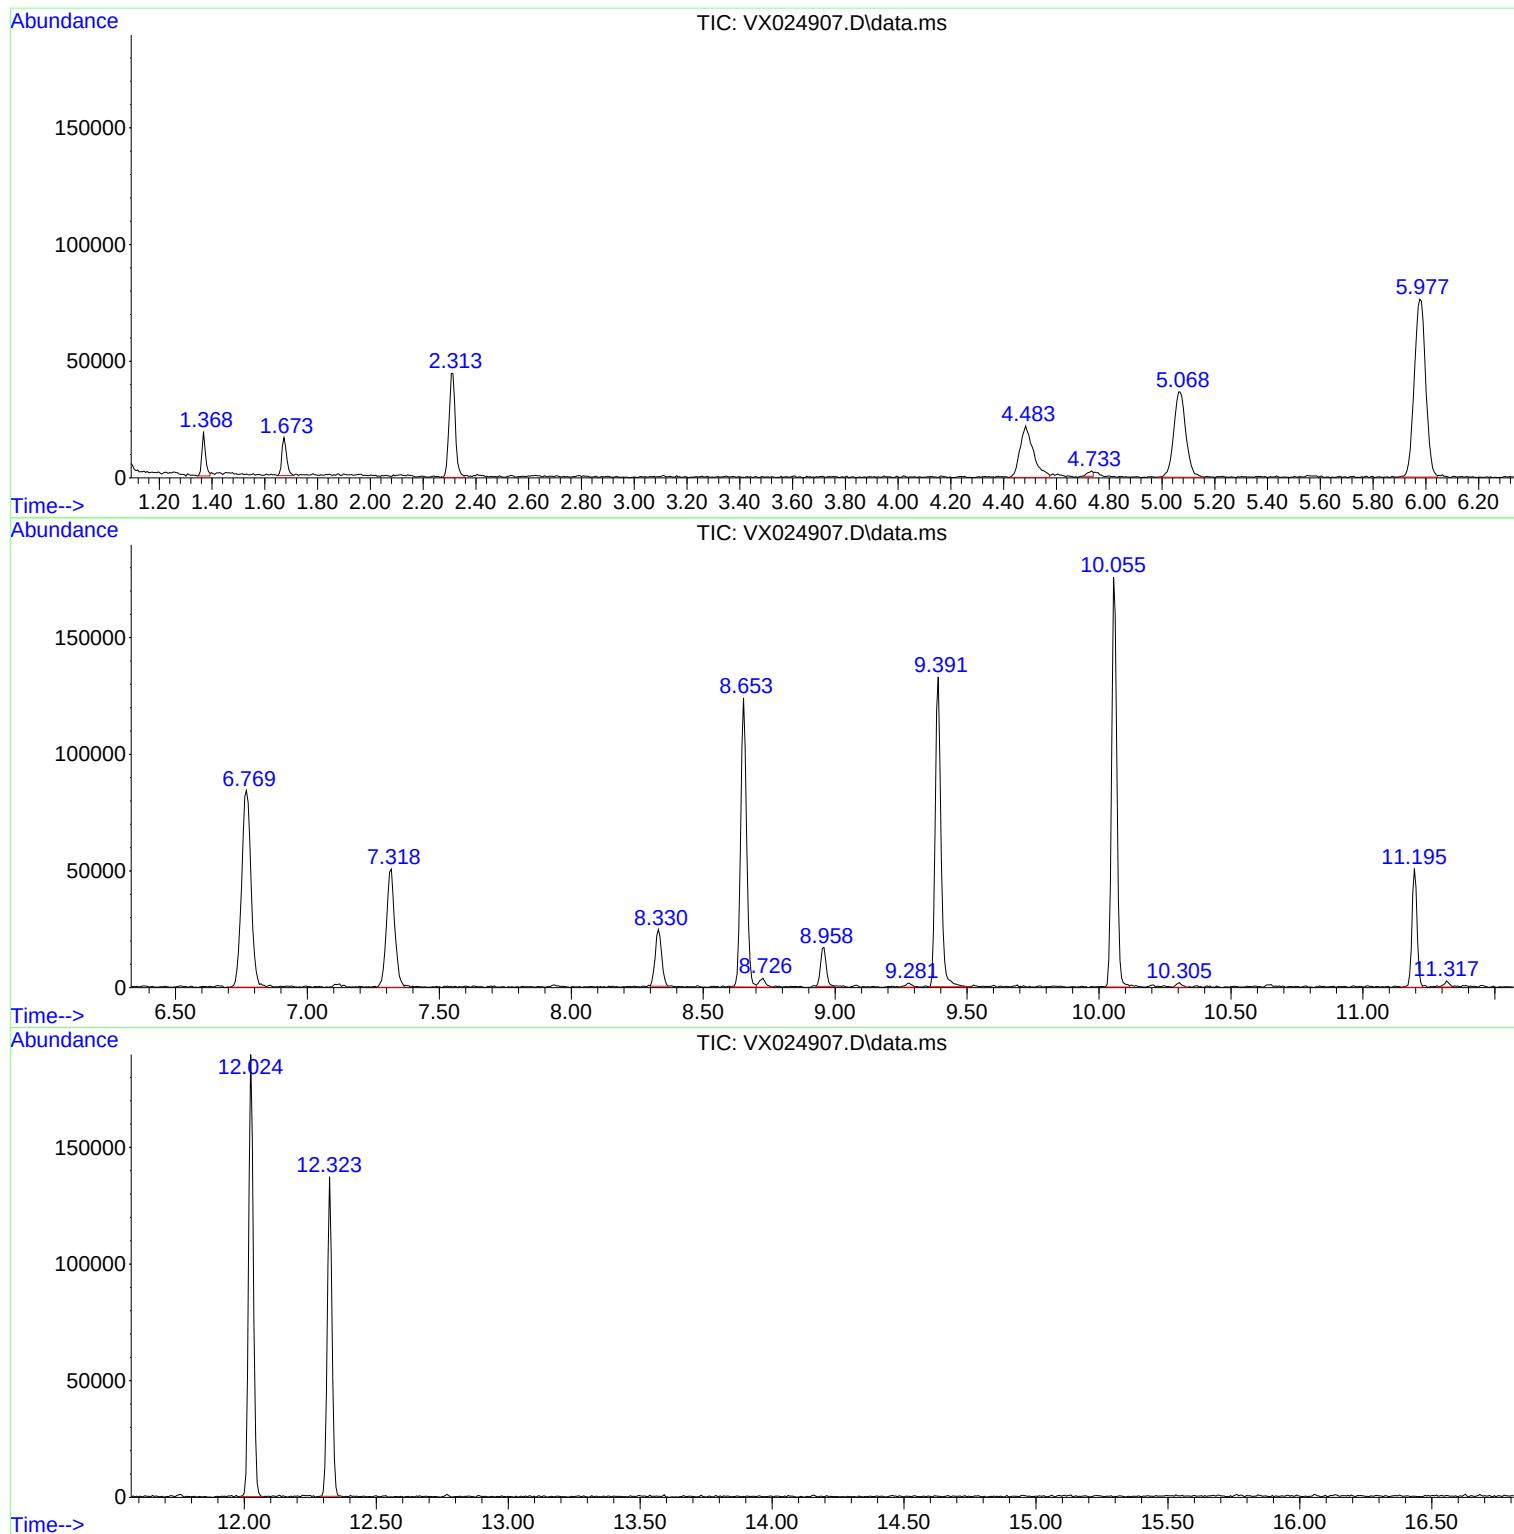

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024907.D
Acq On : 23 Oct 2021 19:47
Operator : JC/MD
Sample : M4303-15
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P021-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024907.D
Acq On : 23 Oct 2021 19:47
Operator : JC/MD
Sample : M4303-15
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P021-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
