

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024908.D
 Acq On : 23 Oct 2021 20:11
 Operator : JC/MD
 Sample : M4303-16
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P027-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.148	7	10	18	rVB4	1462	3139	1.28%	0.150%
2	1.368	39	46	51	rBV	20948	28196	11.54%	1.351%
3	1.672	92	96	101	rVB	18043	20804	8.52%	0.997%
4	2.313	193	201	208	rBV	47396	75960	31.09%	3.639%
5	4.477	544	556	571	rBV2	23224	85006	34.80%	4.072%
6	4.739	592	599	607	rBV2	1348	3838	1.57%	0.184%
7	5.068	639	653	665	rBV	40489	125372	51.32%	6.006%
8	5.977	791	802	816	rBV2	81605	244292	100.00%	11.702%
9	6.769	923	932	943	rVB2	78139	190172	77.85%	9.110%
10	7.111	983	988	994	rVB4	1725	3308	1.35%	0.158%
11	7.318	1013	1022	1034	rVB2	51809	117005	47.90%	5.605%
12	8.330	1181	1188	1195	rBV2	26631	44838	18.35%	2.148%
13	8.653	1234	1241	1248	rBV	133074	207145	84.79%	9.923%
14	8.726	1248	1253	1257	rVB4	2843	5289	2.17%	0.253%
15	8.958	1285	1291	1297	rBV	18532	27809	11.38%	1.332%
16	9.391	1356	1362	1372	rBV	141409	208419	85.32%	9.984%
17	10.055	1466	1471	1481	rBV	159210	223546	91.51%	10.708%
18	11.195	1653	1658	1664	rVB	56340	71095	29.10%	3.406%
19	12.024	1789	1794	1802	rBV	172695	218858	89.59%	10.484%
20	12.323	1837	1843	1850	rVB	144508	183513	75.12%	8.791%




Sum of corrected areas: 2087604

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024908.D
Acq On : 23 Oct 2021 20:11
Operator : JC/MD
Sample : M4303-16
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P027-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

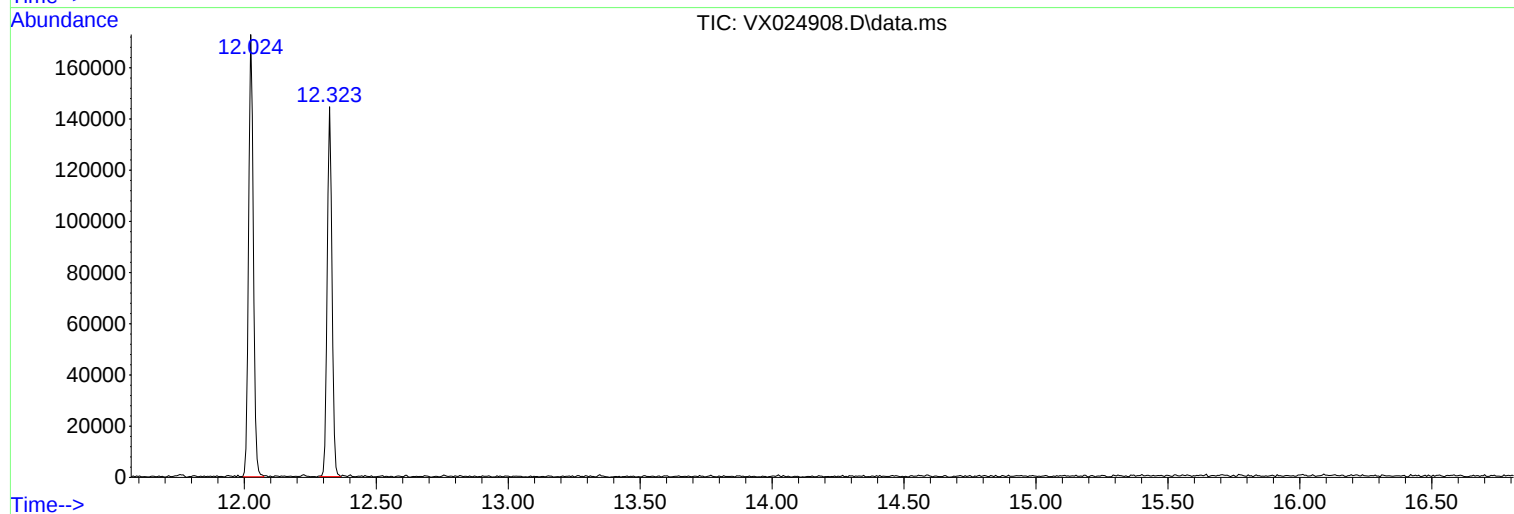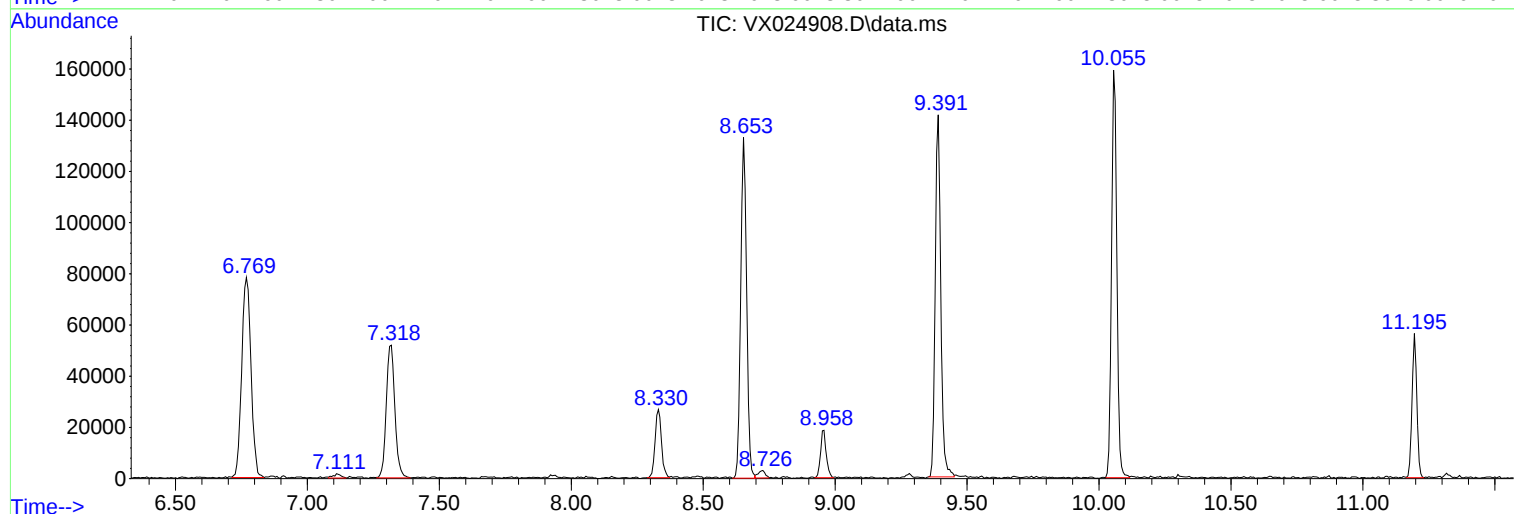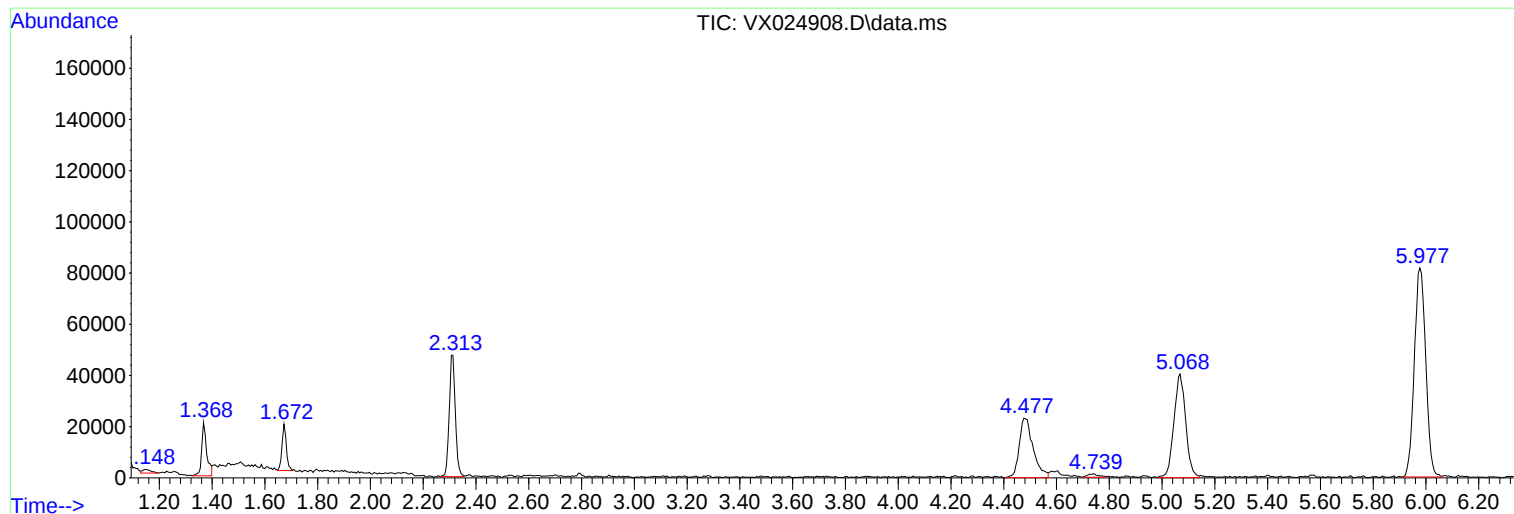

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024908.D
Acq On : 23 Oct 2021 20:11
Operator : JC/MD
Sample : M4303-16
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P027-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024908.D
Acq On : 23 Oct 2021 20:11
Operator : JC/MD
Sample : M4303-16
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P027-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
