

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024909.D
 Acq On : 23 Oct 2021 20:35
 Operator : JC/MD
 Sample : M4303-17
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P032-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	51	rBV	18511	19344	7.62%	0.854%
2	1.672	92	96	101	rBV	17955	21015	8.27%	0.928%
3	2.306	193	200	210	rVB	47560	77557	30.54%	3.426%
4	4.483	546	557	567	rBV	22127	79828	31.43%	3.526%
5	4.580	572	573	585	rVB4	2119	4330	1.70%	0.191%
6	4.733	592	598	610	rBV3	4061	11925	4.70%	0.527%
7	5.068	641	653	666	rBV2	41137	122987	48.43%	5.433%
8	5.977	790	802	816	rBV3	85165	249871	98.39%	11.038%
9	6.769	923	932	942	rBV	91834	218080	85.87%	9.633%
10	7.129	981	991	1001	rBV3	35417	81448	32.07%	3.598%
11	7.312	1014	1021	1030	rBV	53072	117258	46.17%	5.180%
12	8.330	1182	1188	1196	rBV2	28655	46476	18.30%	2.053%
13	8.653	1234	1241	1249	rBV	135677	207420	81.67%	9.163%
14	8.726	1249	1253	1259	rVB5	2251	4094	1.61%	0.181%
15	8.958	1286	1291	1297	rVB2	18529	27139	10.69%	1.199%
16	9.391	1356	1362	1376	rBV	148068	217661	85.70%	9.615%
17	10.055	1462	1471	1478	rBV	181522	253970	100.00%	11.219%
18	11.195	1653	1658	1666	rBV	57215	73850	29.08%	3.262%
19	12.024	1787	1794	1801	rBV	198700	244699	96.35%	10.809%
20	12.323	1838	1843	1850	rBV	143257	184831	72.78%	8.165%


Sum of corrected areas: 2263783

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024909.D
Acq On : 23 Oct 2021 20:35
Operator : JC/MD
Sample : M4303-17
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P032-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

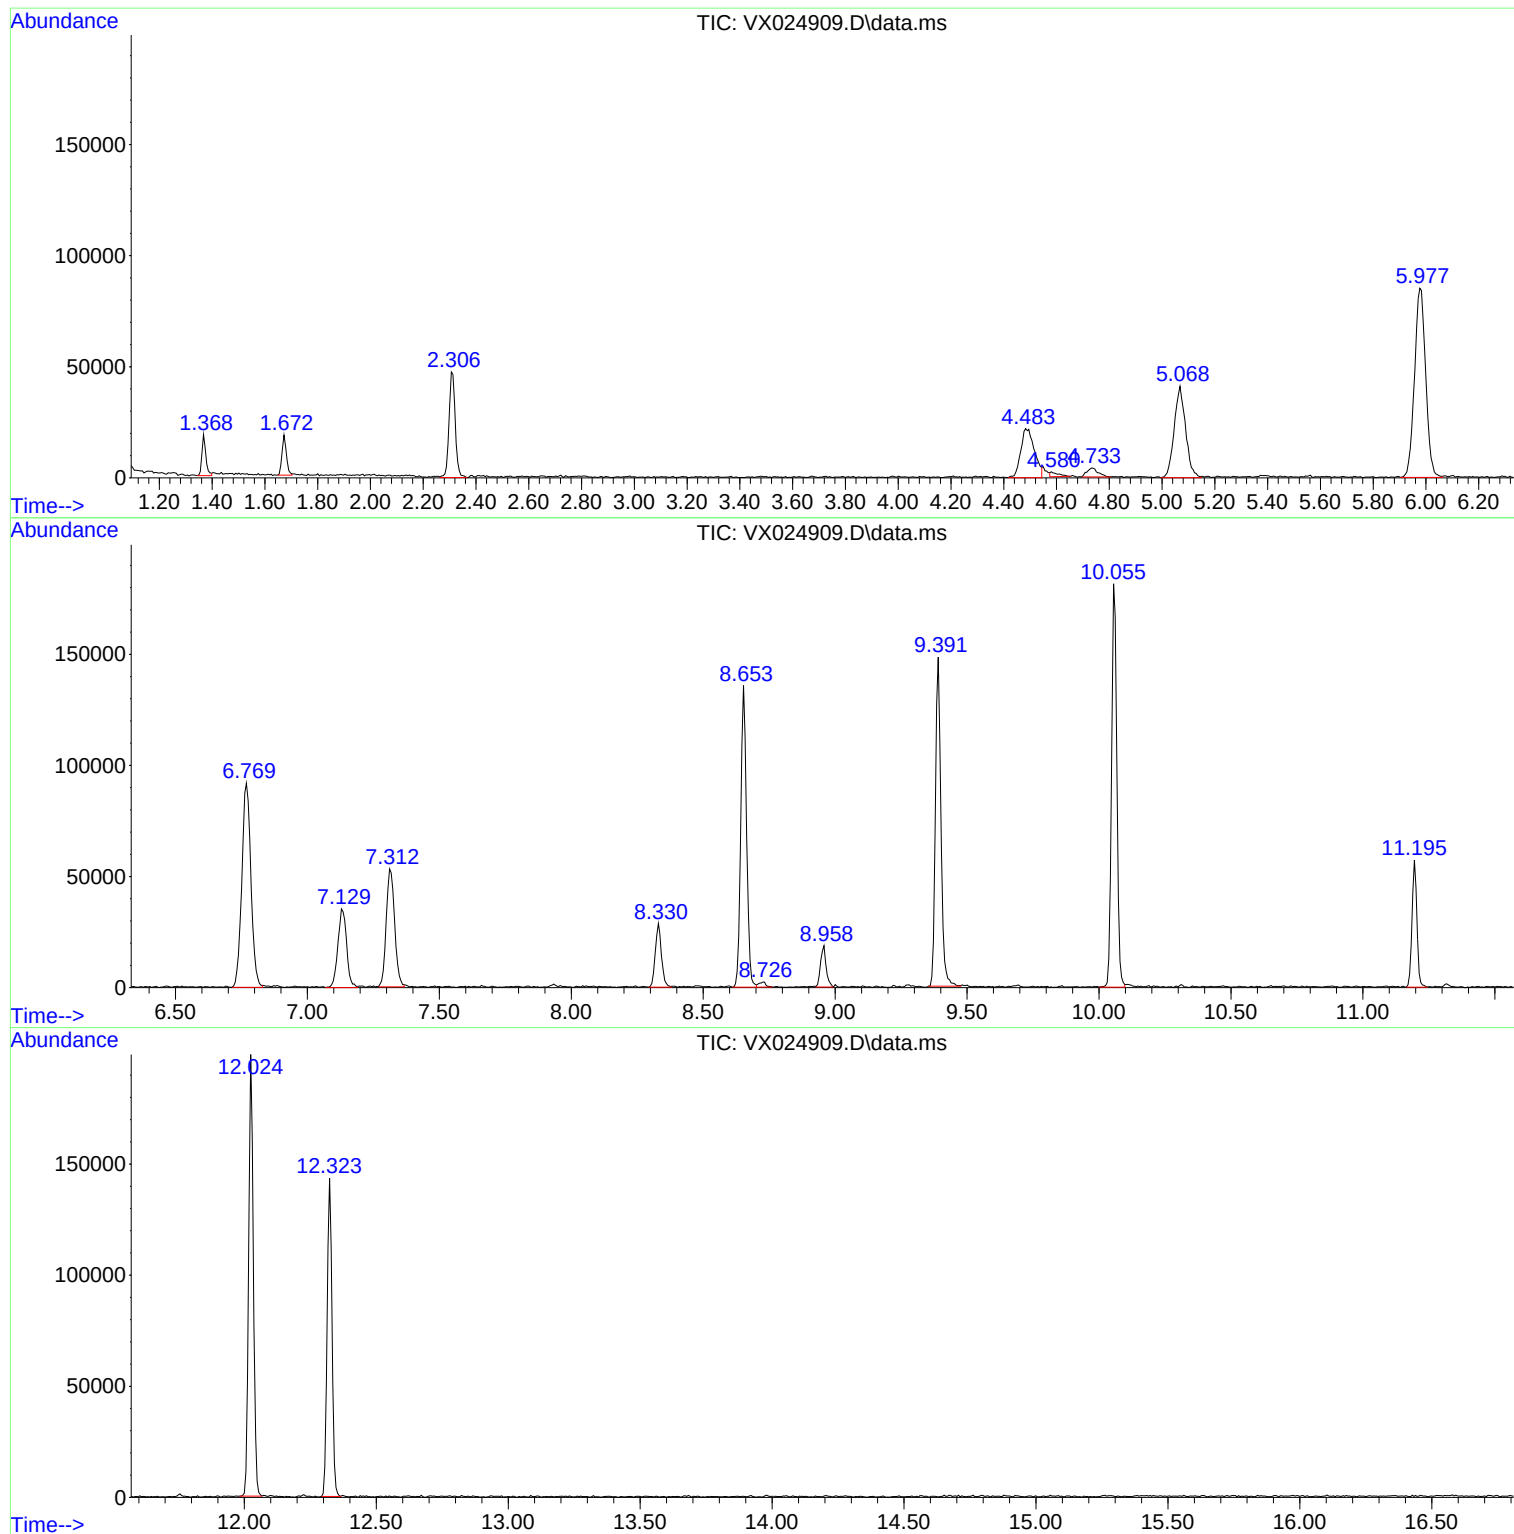

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024909.D
Acq On : 23 Oct 2021 20:35
Operator : JC/MD
Sample : M4303-17
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P032-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024909.D
Acq On : 23 Oct 2021 20:35
Operator : JC/MD
Sample : M4303-17
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P032-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
