
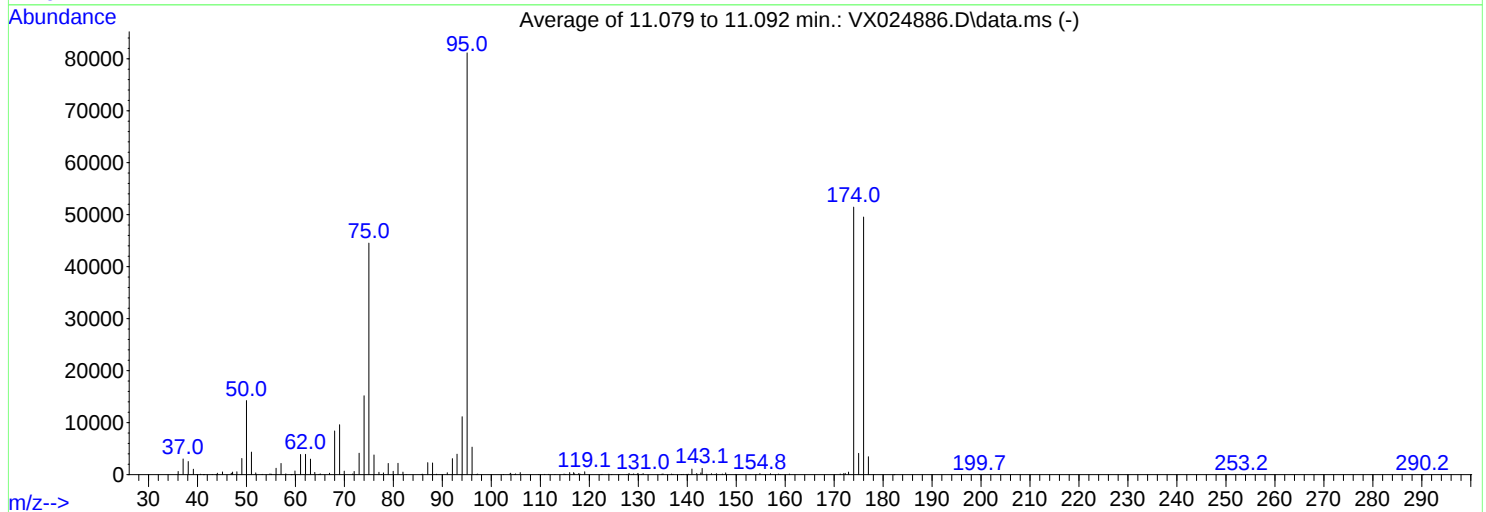


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024886.D
 Acq On : 23 Oct 2021 10:37
 Operator : JC/MD
 Sample : BFB608
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB608

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Oct 27 02:59:04 2021

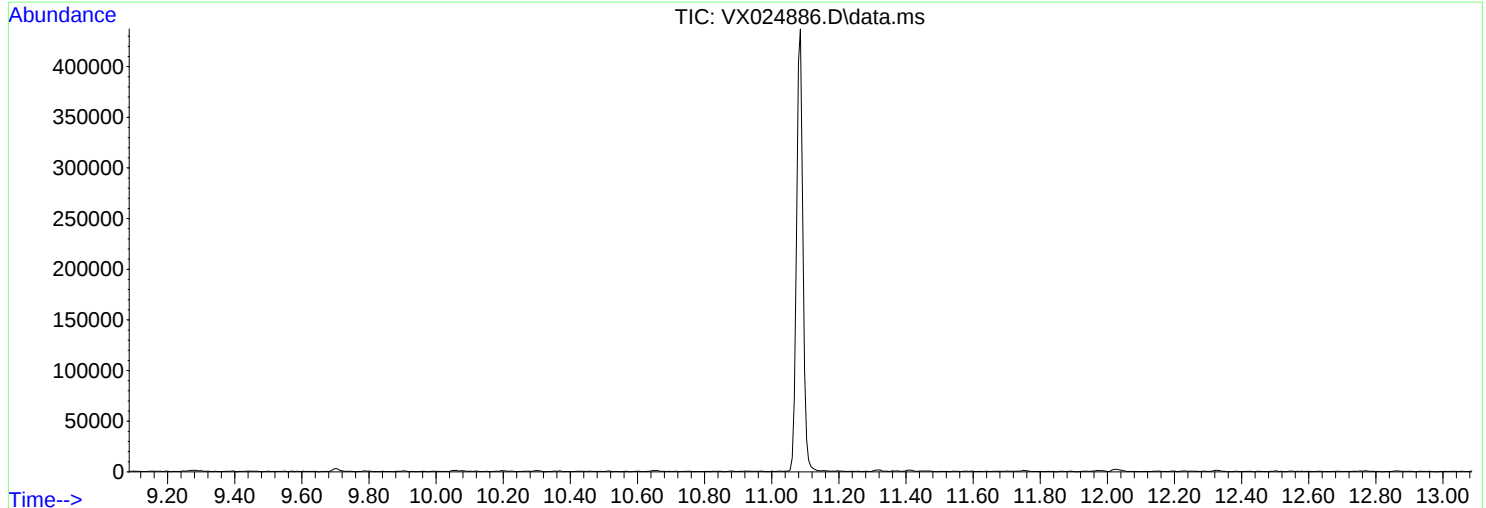

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	14244	PASS
75	95	30	80	54.9	44525	PASS
95	95	100	100	100.0	81131	PASS
96	95	5	9	6.5	5299	PASS
173	174	0.00	2	0.9	486	PASS
174	95	50	120	63.4	51472	PASS
175	174	5	9	8.0	4093	PASS
176	174	95	105	96.3	49563	PASS
177	176	5	10	7.0	3457	PASS

m/z	Abundance
35.90	510.0
37.00	1842.0
38.10	1545.0
39.10	1097.0
39.90	76.0
40.60	98.0
43.80	373.0
45.00	302.0
47.10	559.0
48.00	421.0
48.90	1858.0
50.10	9728.0
51.00	2660.0
52.00	224.0
56.10	591.0
57.00	1432.0
58.00	154.0
60.00	509.0
61.00	2447.0
62.00	2224.0
63.00	1901.0
63.90	193.0
64.80	164.0
66.90	175.0
68.00	5911.0
69.00	5555.0
69.90	463.0
71.70	357.0
72.10	363.0
73.00	2563.0
74.00	11055.0
75.10	30488.0
76.00	2209.0
76.90	181.0
77.60	123.0
78.90	1431.0
79.90	542.0
80.90	1471.0
81.90	368.0
85.90	166.0
87.00	1694.0
87.90	1627.0
88.80	268.0
91.00	249.0
92.10	2078.0
93.00	2806.0
94.10	8914.0
95.10	57384.0
96.00	4102.0
97.20	144.0
102.50	64.0
103.90	321.0
104.70	119.0
105.90	292.0
111.70	85.0
114.90	94.0
116.10	322.0
117.00	423.0
118.10	360.0
119.00	468.0
122.60	116.0
124.00	70.0
126.10	76.0
128.10	275.0
129.00	181.0
129.90	368.0
131.10	180.0
135.00	210.0
136.70	87.0
139.90	144.0
140.90	1004.0
141.90	256.0
143.00	1122.0
143.80	64.0
144.80	172.0
146.00	117.0
147.20	110.0
147.90	222.0
154.80	230.0
157.10	178.0
158.60	126.0
160.80	100.0
171.20	156.0
172.00	266.0
172.80	400.0
174.00	43720.0
175.00	2883.0
176.00	41168.0
176.90	2532.0
178.10	84.0
253.20	78.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608

Scan 1631 (11.031 min): VX024886.D\data.ms
BFB608

m/z	Abundance
36.50	120.0
39.90	69.0
43.90	106.0
44.20	115.0
166.10	73.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608

m/z	Abundance
36.10	733.0
37.10	3555.0
38.10	3248.0
39.10	1167.0
39.90	121.0
40.70	76.0
43.10	74.0
44.10	688.0
45.10	642.0
47.20	912.0
48.10	641.0
49.10	3849.0
50.00	15924.0
51.00	4849.0
52.00	322.0
53.20	60.0
54.80	244.0
55.10	282.0
56.00	1342.0
57.00	2728.0
58.00	201.0
59.10	54.0
59.90	848.0
61.00	4531.0
62.10	5107.0
63.00	3512.0
63.90	516.0
65.10	307.0
67.00	394.0
68.00	9977.0
69.00	10981.0
69.90	952.0
72.00	748.0
73.00	5168.0
74.00	17416.0
75.00	52264.0
76.00	4679.0
77.10	327.0
77.90	499.0
78.90	2522.0
79.90	639.0
81.00	2468.0
82.00	511.0
85.80	120.0
86.00	106.0
87.00	2452.0
88.00	2364.0
91.10	377.0
92.00	4188.0
93.00	4812.0
94.00	12389.0
95.00	89728.0
96.10	6218.0
96.90	168.0
103.80	476.0
105.00	192.0
105.90	408.0
109.70	78.0
110.90	84.0
113.00	61.0
114.80	148.0
116.00	340.0
116.90	310.0
117.80	274.0
119.00	631.0
122.40	111.0
124.60	64.0
128.10	253.0
129.00	182.0
129.80	356.0
130.60	148.0
131.00	221.0
135.10	213.0
136.90	59.0
138.80	61.0
139.10	61.0
140.20	147.0
141.10	1198.0
142.00	244.0
142.80	1028.0
143.10	1128.0
144.00	138.0
145.00	187.0
146.00	352.0
147.10	117.0
147.80	269.0
149.90	104.0
152.80	64.0
154.10	68.0
154.90	208.0
156.90	212.0
159.00	102.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608

160.90	149.0
170.10	111.0
171.30	108.0
171.90	380.0
172.40	283.0
173.00	425.0
174.00	49096.0
175.00	4237.0
176.00	46904.0
177.00	3270.0
182.20	51.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608

m/z	Abundance
36.10	589.0
37.00	3678.0
38.10	2789.0
39.20	850.0
39.90	131.0
40.60	65.0
41.20	55.0
42.90	51.0
44.00	476.0
45.20	609.0
46.90	820.0
48.10	597.0
49.10	3587.0
50.00	17080.0
51.00	5524.0
51.80	490.0
53.20	125.0
54.80	242.0
56.10	1785.0
57.10	2313.0
58.10	129.0
59.90	816.0
61.10	4640.0
62.00	4446.0
63.10	3563.0
64.00	557.0
64.90	178.0
66.90	242.0
68.00	9301.0
69.00	12246.0
70.00	628.0
71.90	725.0
73.00	4626.0
74.00	17024.0
75.00	50824.0
76.10	4448.0
76.90	454.0
77.20	456.0
78.00	547.0
79.00	2546.0
80.00	720.0
80.90	2655.0
81.90	630.0
82.60	137.0
85.80	60.0
87.00	2827.0
88.10	2787.0
88.80	58.0
90.90	455.0
92.10	2961.0
93.00	4210.0
94.00	12121.0
95.10	96280.0
96.00	5578.0
97.20	195.0
104.00	482.0
104.90	276.0
105.90	544.0
110.90	73.0
111.70	128.0
114.80	116.0
115.20	179.0
115.90	565.0
116.80	948.0
117.90	348.0
119.10	564.0
122.60	82.0
124.00	170.0
126.00	61.0
127.70	227.0
128.10	219.0
128.70	196.0
129.10	123.0
130.00	366.0
130.90	291.0
134.80	308.0
136.80	225.0
137.10	217.0
139.20	145.0
140.20	142.0
140.90	1058.0
141.90	190.0
143.00	1365.0
143.80	81.0
145.00	188.0
145.70	146.0
146.10	116.0
147.10	163.0
147.90	570.0
150.00	64.0
152.80	53.0
154.90	256.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608

155.90	65.0
157.00	202.0
158.70	266.0
160.90	101.0
171.20	143.0
172.20	487.0
173.00	634.0
174.00	61600.0
175.00	5158.0
176.00	60616.0
177.00	4568.0
199.70	68.0
290.20	56.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608