

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
 Data File : VX038424.D
 Acq On : 23 Oct 2023 11:59
 Operator : JC/MD
 Sample : 04991-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1027

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Title : SW846 8260

Signal : TIC: VX038424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.374	205	211	225	rVV	144175	231742	27.24%	4.247%
2	4.227	505	515	532	rBV	80462	215555	25.34%	3.950%
3	4.556	560	569	585	rBV	43401	125200	14.72%	2.294%
4	5.385	693	705	720	rBV2	98598	290906	34.20%	5.331%
5	5.550	721	732	748	rBV	150156	435125	51.15%	7.973%
6	5.952	788	798	816	rBV	107509	282553	33.22%	5.178%
7	6.763	921	931	948	rBV	247795	599877	70.52%	10.992%
8	7.586	1059	1066	1072	rBV2	5435	11629	1.37%	0.213%
9	8.647	1233	1240	1249	rBV	529258	829305	97.49%	15.196%
10	8.714	1249	1251	1260	rVB3	5581	10219	1.20%	0.187%
11	9.519	1379	1383	1393	rBV	19368	30044	3.53%	0.551%
12	10.055	1465	1471	1487	rBV	556896	785232	92.31%	14.389%
13	10.506	1540	1545	1554	rBV	30459	41434	4.87%	0.759%
14	10.756	1582	1586	1595	rBV3	10364	22205	2.61%	0.407%
15	11.079	1634	1639	1645	rBV	483023	617147	72.55%	11.309%
16	11.134	1645	1648	1656	rVB	22590	30528	3.59%	0.559%
17	11.573	1715	1720	1723	rBV2	9469	12998	1.53%	0.238%
18	11.604	1723	1725	1735	rVB2	8403	12320	1.45%	0.226%
19	11.969	1776	1785	1788	rBV3	5597	9234	1.09%	0.169%
20	12.018	1788	1793	1802	rVB	646055	850658	100.00%	15.588%
21	13.676	2059	2065	2070	rBV3	8656	13329	1.57%	0.244%




Sum of corrected areas: 5457240

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038424.D
Acq On : 23 Oct 2023 11:59
Operator : JC/MD
Sample : 04991-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1027

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

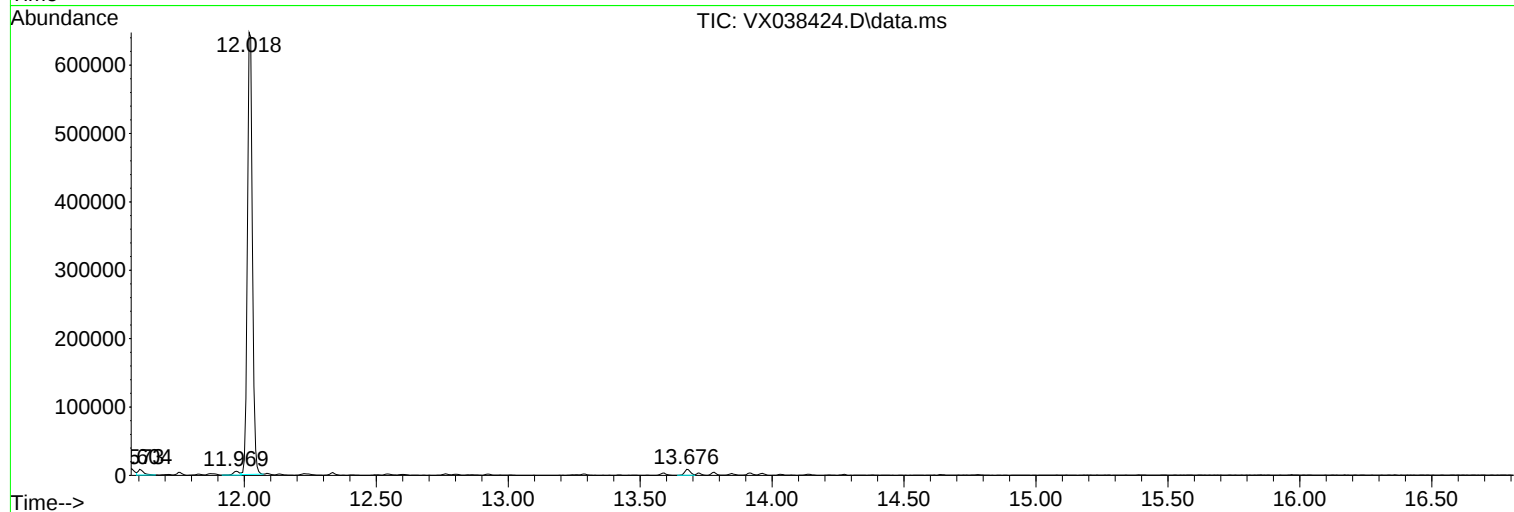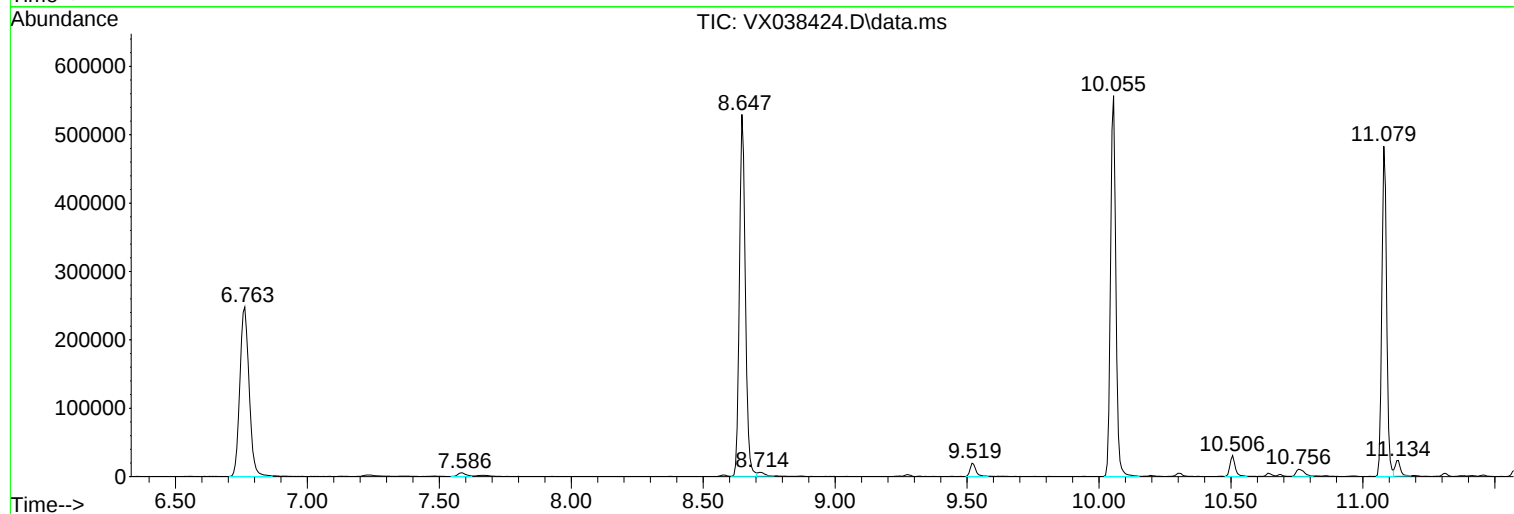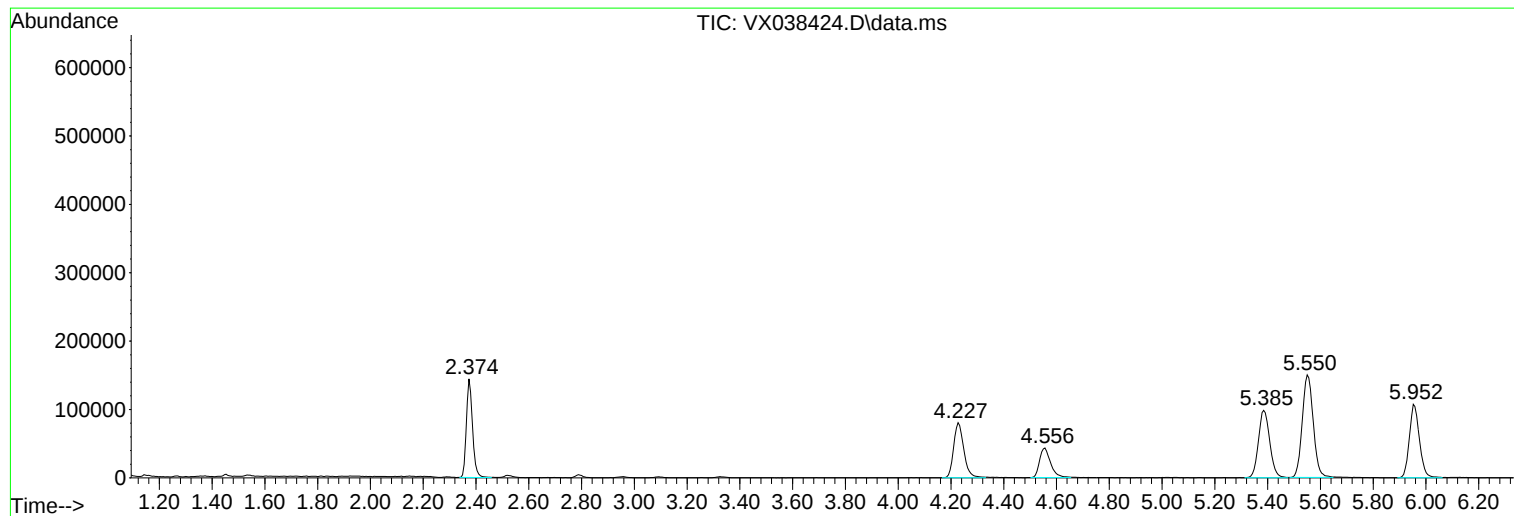

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038424.D
Acq On : 23 Oct 2023 11:59
Operator : JC/MD
Sample : 04991-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1027










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butanal Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.227	24.77 ug/l	215555	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butanal	72	C4H8O	000123-72-8	94
2			Propanal, 2-methyl-	72	C4H8O	000078-84-2	46
3			2-Propanone, hydrazone	72	C3H8N2	005281-20-9	35
4			Propane	44	C3H8	000074-98-6	35
5			1-Propene, 3-methoxy-	72	C4H8O	000627-40-7	32

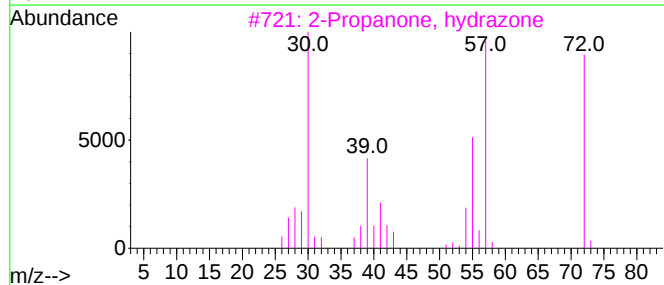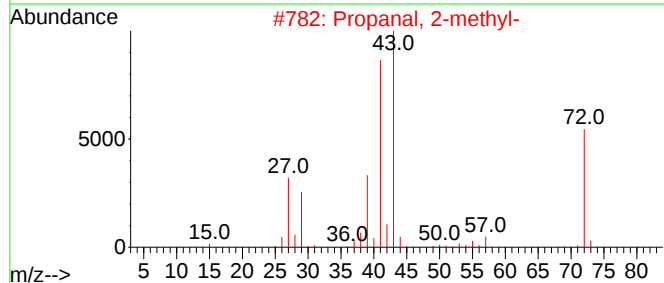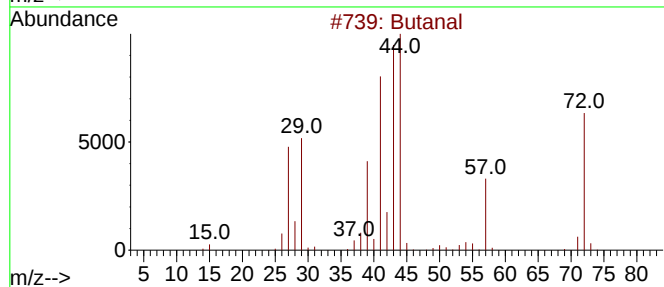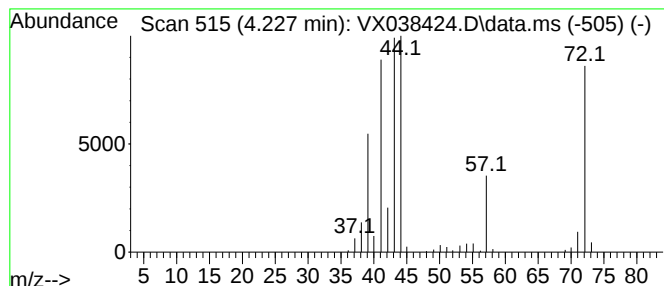

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038424.D
Acq On : 23 Oct 2023 11:59
Operator : JC/MD
Sample : 04991-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1027

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butanal	4.227	24.8	ug/l	215555	1	5.550	435125	50.0