

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
 Data File : VX038436.D
 Acq On : 23 Oct 2023 16:37
 Operator : JC/MD
 Sample : 05007-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.098	648	658	669	rBV3	10796	31411	4.22%	0.695%
2	5.385	694	705	720	rBV	84477	249801	33.60%	5.524%
3	5.549	722	732	748	rBV	125556	366453	49.29%	8.104%
4	5.952	788	798	813	rBV	91120	245034	32.96%	5.419%
5	6.763	922	931	949	rBV	209960	513839	69.11%	11.363%
6	8.646	1234	1240	1259	rBV	439302	719099	96.71%	15.902%
7	10.055	1465	1471	1486	rBV	492764	688013	92.53%	15.215%
8	11.079	1634	1639	1656	rBV	407293	541301	72.80%	11.970%
9	12.024	1788	1794	1802	rBV	584566	743525	100.00%	16.442%
10	13.585	2044	2050	2062	rBV	202119	269474	36.24%	5.959%
11	13.963	2107	2112	2121	rVB	52415	70611	9.50%	1.561%
12	15.249	2316	2323	2331	rBV	56238	83515	11.23%	1.847%




Sum of corrected areas: 4522076

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038436.D
Acq On : 23 Oct 2023 16:37
Operator : JC/MD
Sample : 05007-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

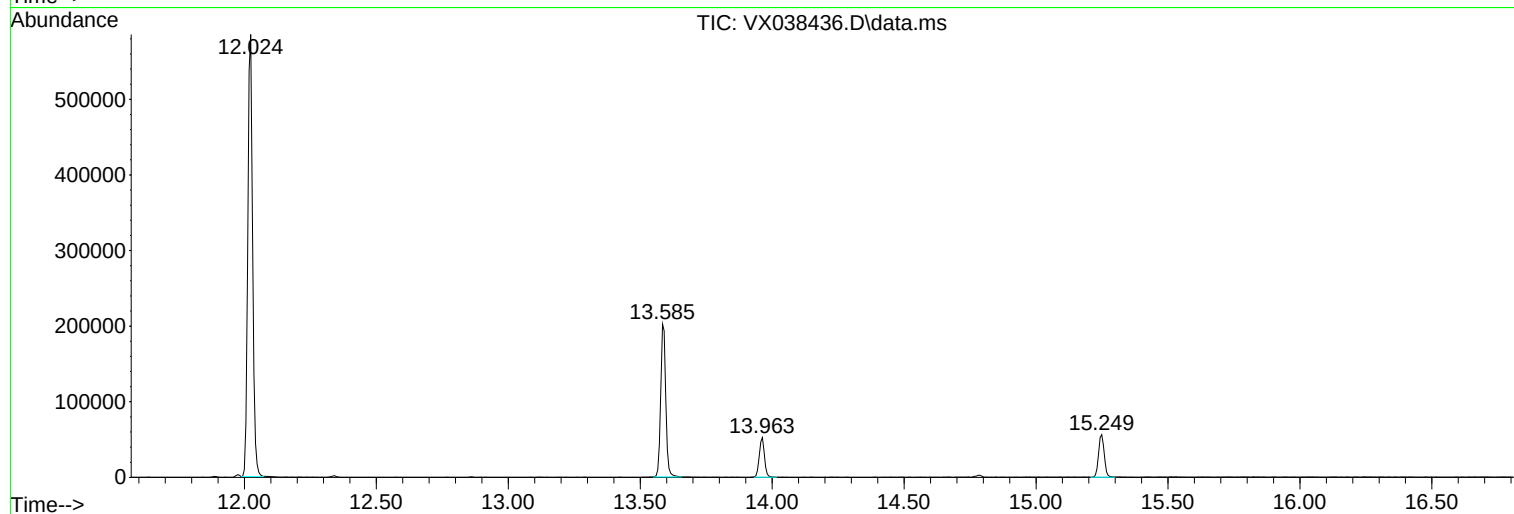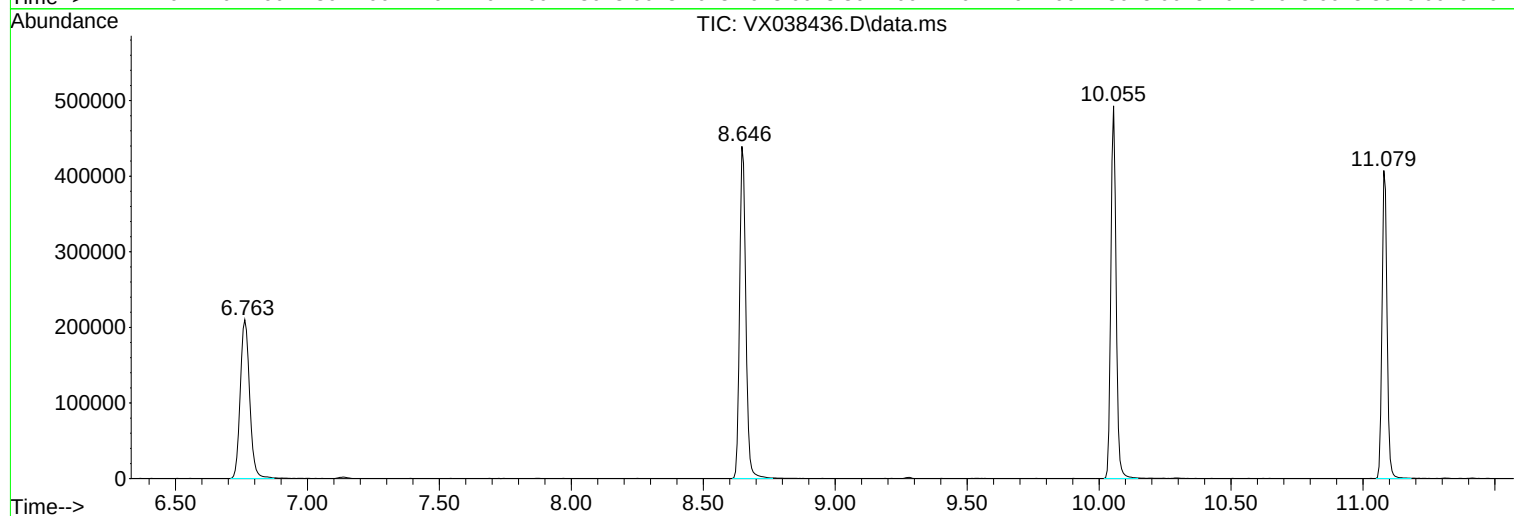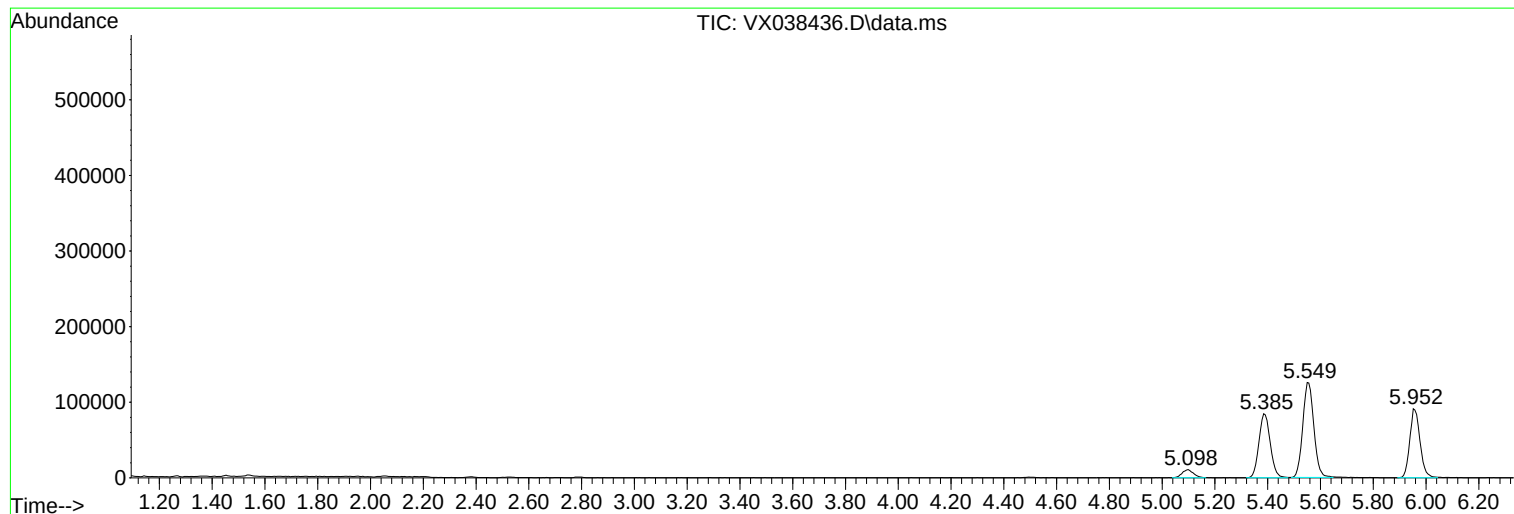

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038436.D
Acq On : 23 Oct 2023 16:37
Operator : JC/MD
Sample : 05007-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,2,3,4-tetrachloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.249	5.62 ug/l	83515	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,2,3,4-tetrachloro-	214	C6H2Cl4	000634-66-2	99
2			Benzene, 1,2,3,5-tetrachloro-	214	C6H2Cl4	000634-90-2	98
3			Benzene, 1,2,4,5-tetrachloro-	214	C6H2Cl4	000095-94-3	98
4			Imidazole, 4-bromo-2-trifluorome...	214	C4H2BrF3N2	219534-98-2	46
5			3-Bromo-5-(trifluoromethyl)-2H-p...	214	C4H2BrF3N2	093608-11-8	43

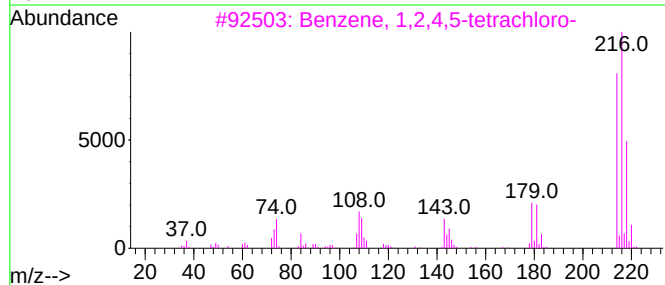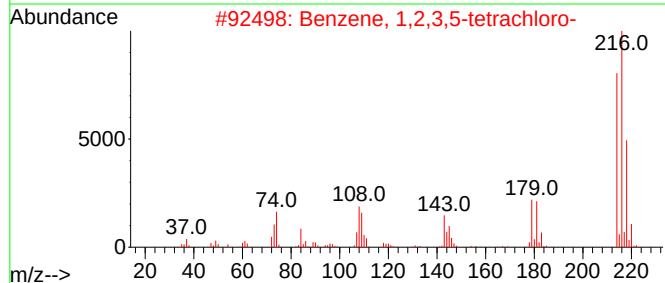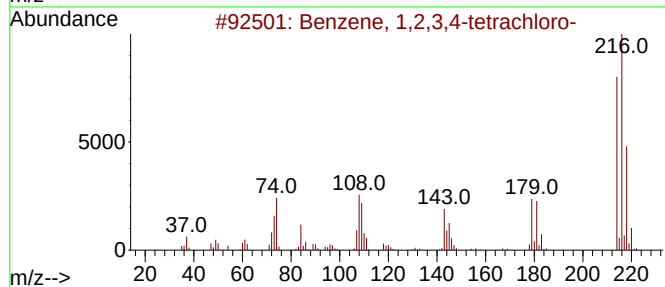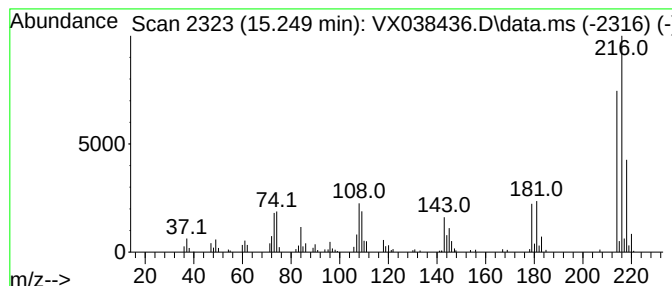

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038436.D
Acq On : 23 Oct 2023 16:37
Operator : JC/MD
Sample : 05007-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,2,3,...	15.249	5.6	ug/l	83515	4	12.024	743525	50.0