

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
 Data File : VX038437.D
 Acq On : 23 Oct 2023 17:01
 Operator : JC/MD
 Sample : 05007-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	694	705	719	rBV	87490	255888	33.65%	5.955%
2	5.550	722	732	753	rVB	130423	378543	49.78%	8.809%
3	5.958	788	799	819	rBV	94371	248743	32.71%	5.789%
4	6.763	921	931	948	rBV	220799	526811	69.28%	12.259%
5	8.647	1234	1240	1261	rBV	446206	736920	96.92%	17.149%
6	10.055	1465	1471	1489	rBV	521113	705681	92.81%	16.422%
7	11.079	1634	1639	1652	rBV	420120	548954	72.20%	12.775%
8	12.024	1788	1794	1806	rBV	588084	760359	100.00%	17.694%
9	13.585	2044	2050	2062	rBV	72654	96992	12.76%	2.257%
10	13.957	2106	2111	2122	rBV2	14100	20845	2.74%	0.485%
11	15.249	2318	2323	2330	rBV	13099	17441	2.29%	0.406%




Sum of corrected areas: 4297177

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038437.D
Acq On : 23 Oct 2023 17:01
Operator : JC/MD
Sample : 05007-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

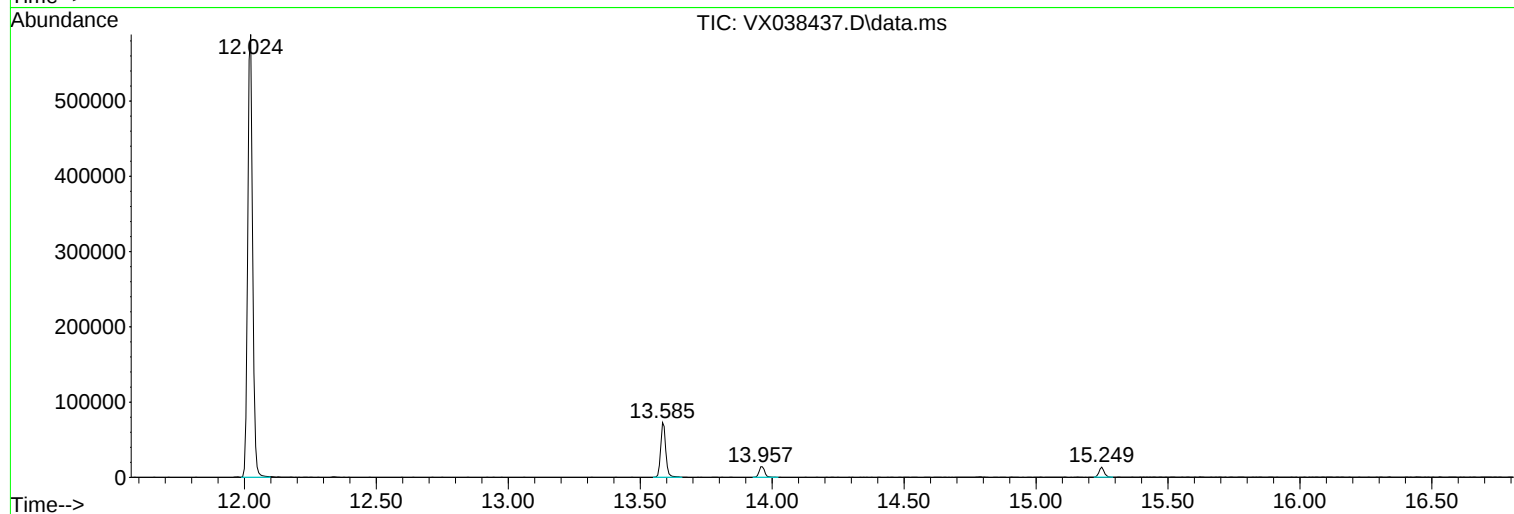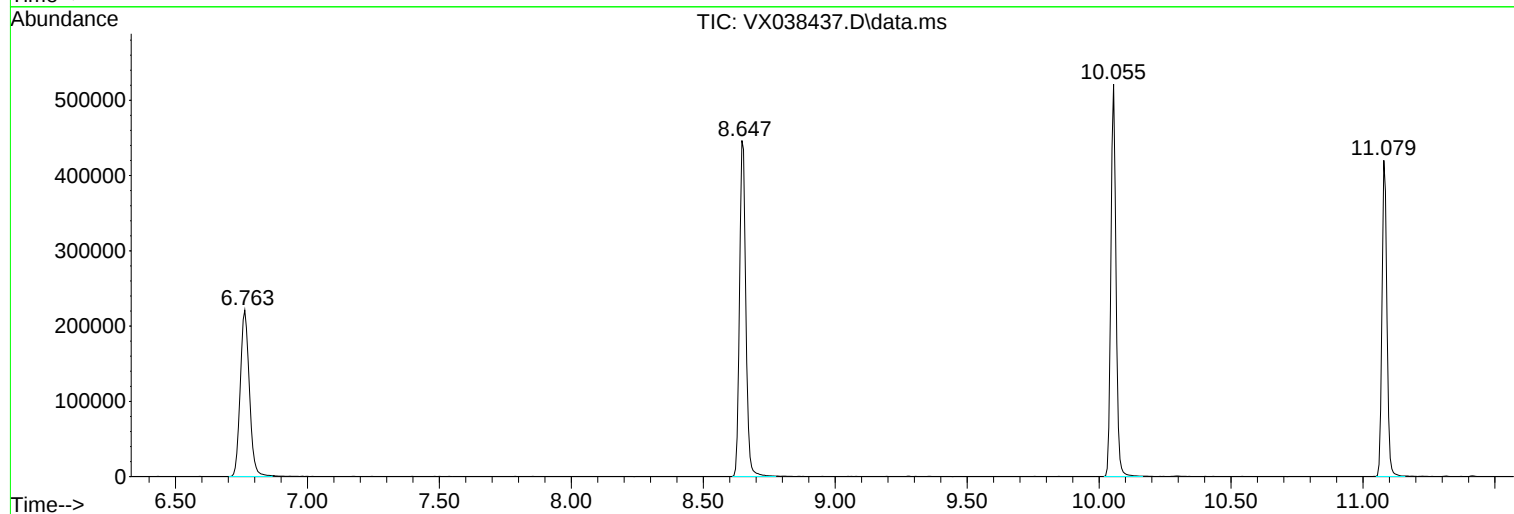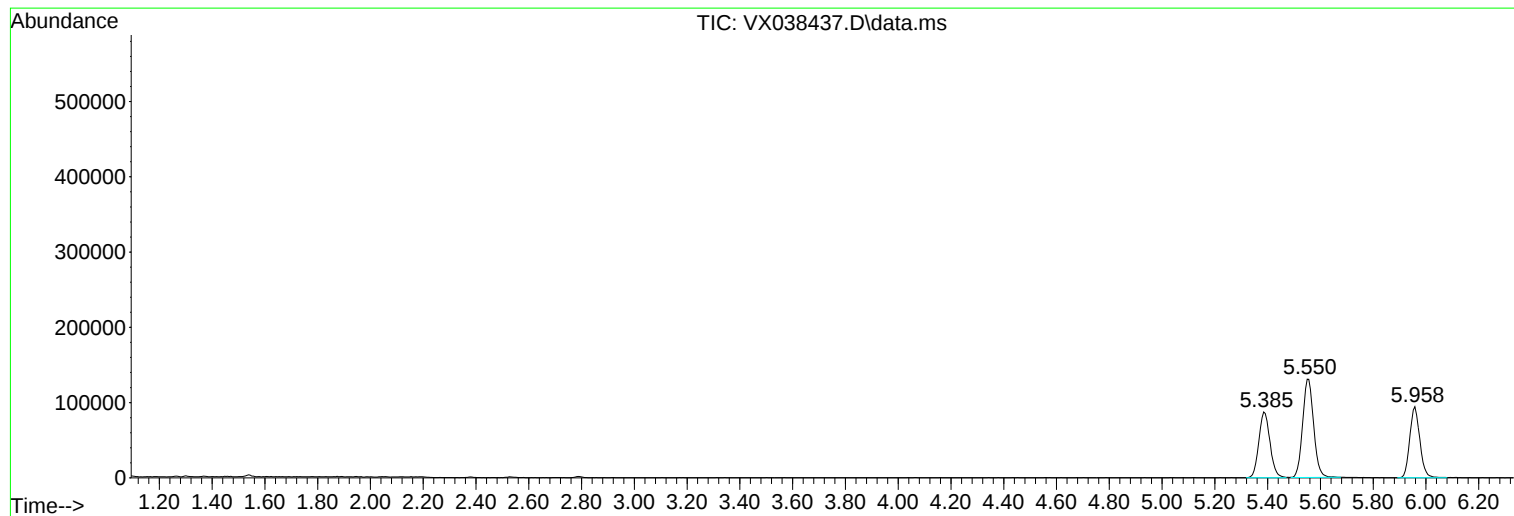

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038437.D
Acq On : 23 Oct 2023 17:01
Operator : JC/MD
Sample : 05007-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038437.D
Acq On : 23 Oct 2023 17:01
Operator : JC/MD
Sample : 05007-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------