

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
 Data File : VX038438.D
 Acq On : 23 Oct 2023 17:24
 Operator : JC/MD
 Sample : 05007-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GW-25-10-13

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	695	705	721	rBV2	88229	257202	33.84%	6.064%
2	5.550	721	732	746	rBV	130256	378081	49.74%	8.913%
3	5.958	788	799	815	rBV2	94823	250384	32.94%	5.903%
4	6.763	919	931	953	rBV	216427	527038	69.34%	12.425%
5	8.647	1234	1240	1260	rBV	452913	738990	97.23%	17.422%
6	10.055	1465	1471	1489	rBV	508064	704612	92.70%	16.612%
7	11.079	1634	1639	1652	rBV	417083	553273	72.79%	13.044%
8	12.024	1788	1794	1806	rBV	578805	760068	100.00%	17.919%
9	13.585	2046	2050	2061	rVB	39687	53685	7.06%	1.266%
10	13.963	2106	2112	2117	rVB2	7540	10416	1.37%	0.246%
11	15.249	2318	2323	2329	rBV2	5555	7946	1.05%	0.187%




Sum of corrected areas: 4241695

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038438.D
Acq On : 23 Oct 2023 17:24
Operator : JC/MD
Sample : 05007-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-25-10-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

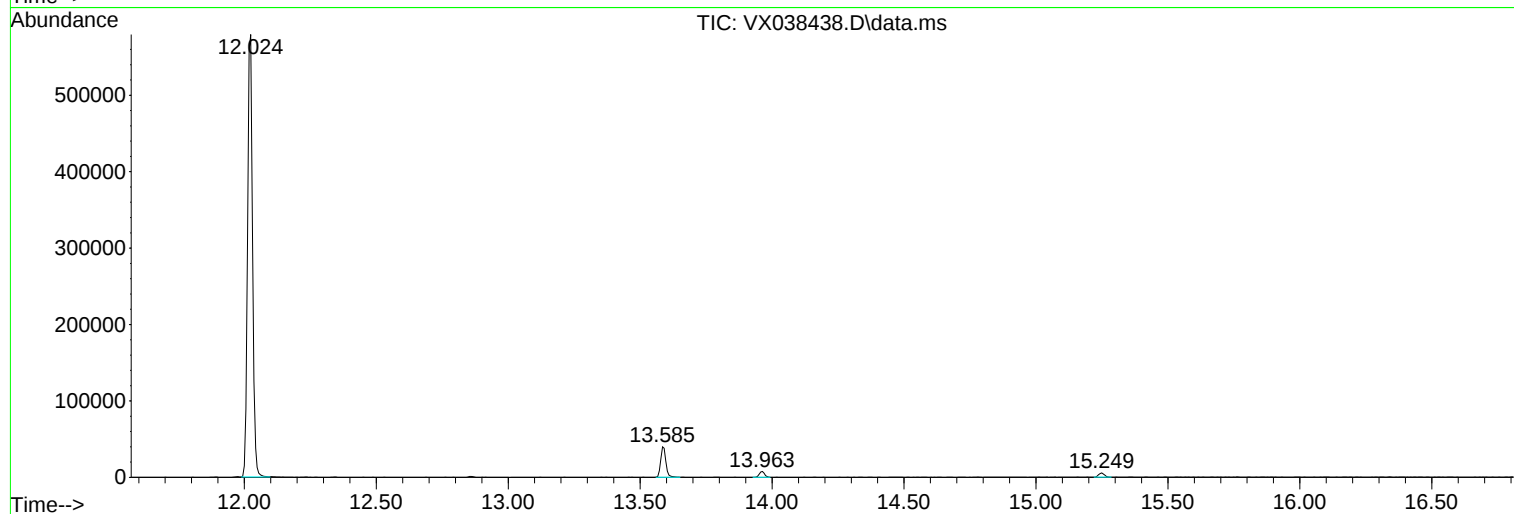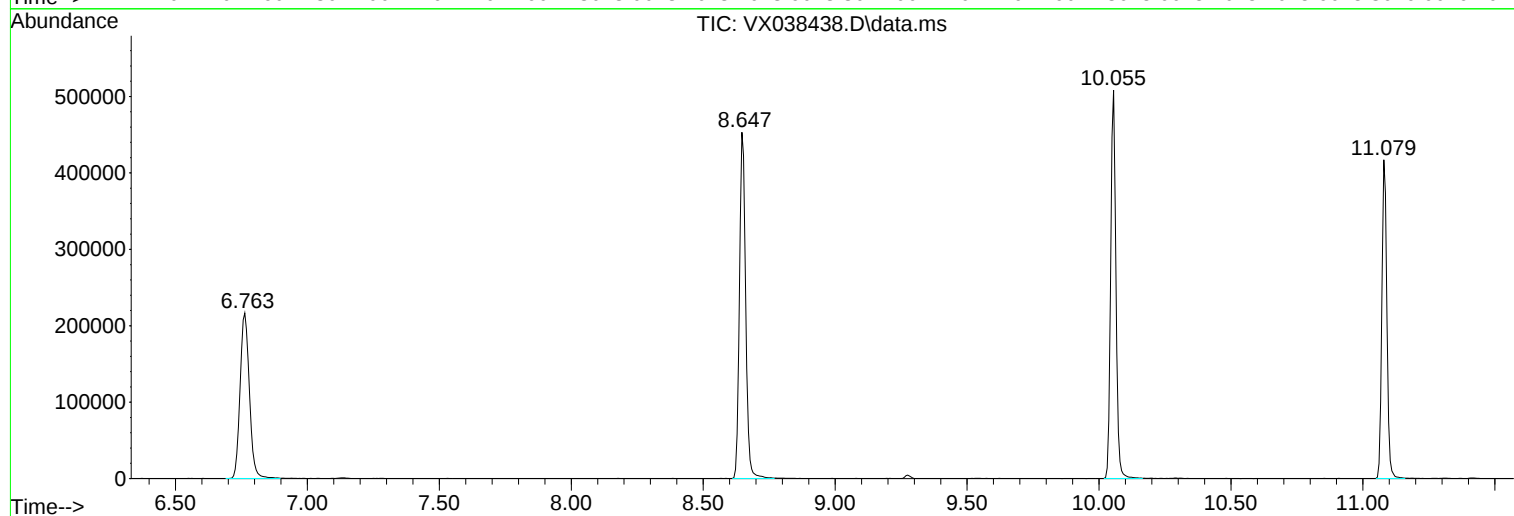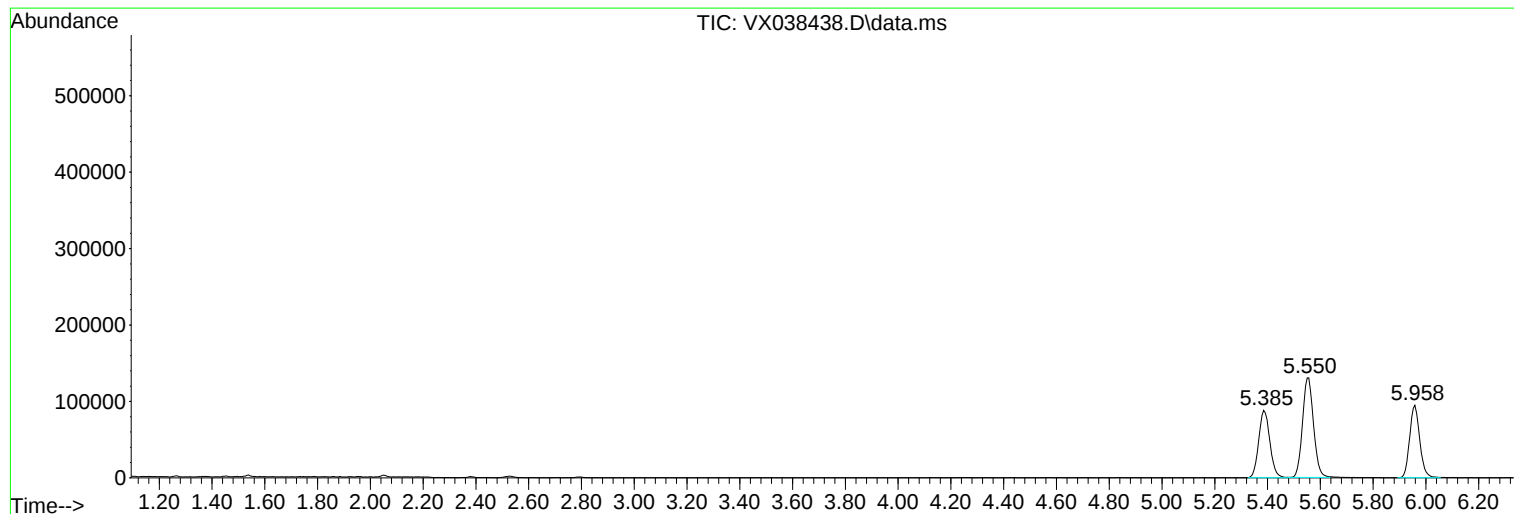

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038438.D
Acq On : 23 Oct 2023 17:24
Operator : JC/MD
Sample : 05007-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-25-10-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038438.D
Acq On : 23 Oct 2023 17:24
Operator : JC/MD
Sample : 05007-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-25-10-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc