

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
 Data File : VX038443.D
 Acq On : 23 Oct 2023 19:19
 Operator : JC/MD
 Sample : 05007-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GW-26-23-26

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	693	705	722	rBV	87551	259600	4.39%	2.024%
2	5.555	722	733	748	rVV	135879	386789	6.53%	3.016%
3	5.958	788	799	811	rBV	98856	259346	4.38%	2.022%
4	6.763	922	931	948	rBV	220623	532523	9.00%	4.152%
5	7.128	983	991	1004	rBV2	61656	131743	2.23%	1.027%
6	8.646	1234	1240	1264	rBV	462063	750956	12.69%	5.855%
7	9.274	1336	1343	1359	rBV	561419	806907	13.63%	6.291%
8	10.055	1465	1471	1489	rBV	524009	737054	12.45%	5.746%
9	11.079	1634	1639	1654	rBV	441799	567112	9.58%	4.421%
10	12.024	1789	1794	1804	rVB2	620552	880841	14.88%	6.867%
11	13.585	2045	2050	2073	rVB	4731349	5919548	100.00%	46.151%
12	13.962	2106	2112	2127	rVB	1122396	1428540	24.13%	11.137%
13	15.249	2317	2323	2330	rBV	121246	165458	2.80%	1.290%




Sum of corrected areas: 12826417

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038443.D
Acq On : 23 Oct 2023 19:19
Operator : JC/MD
Sample : 05007-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-26-23-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

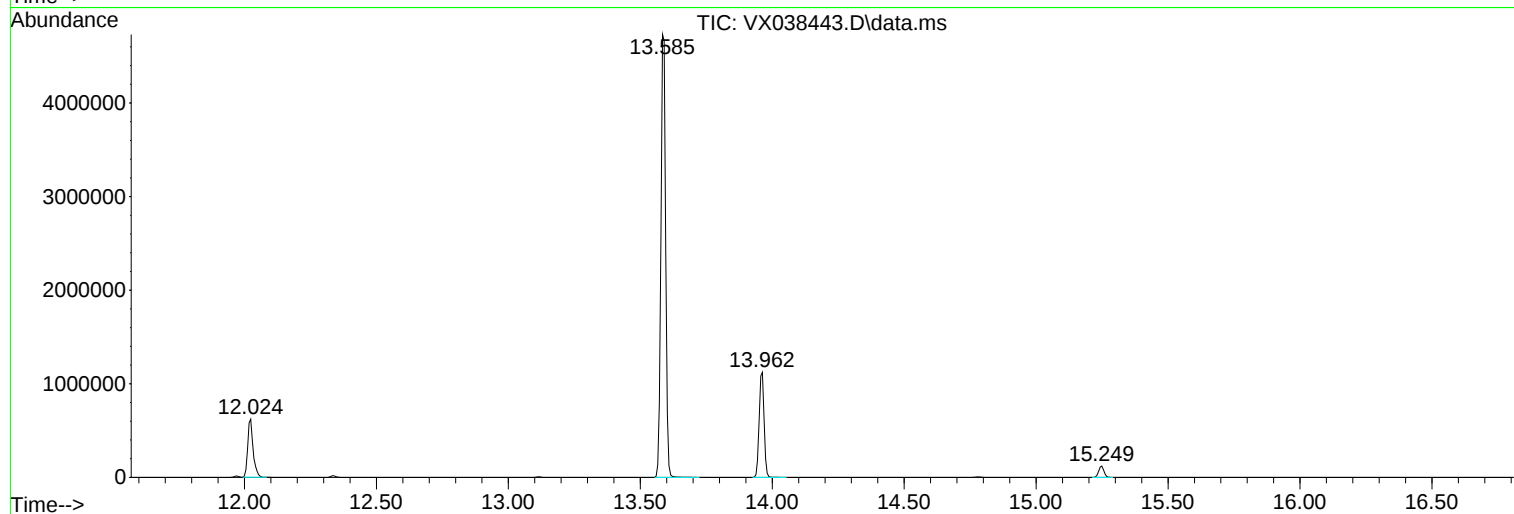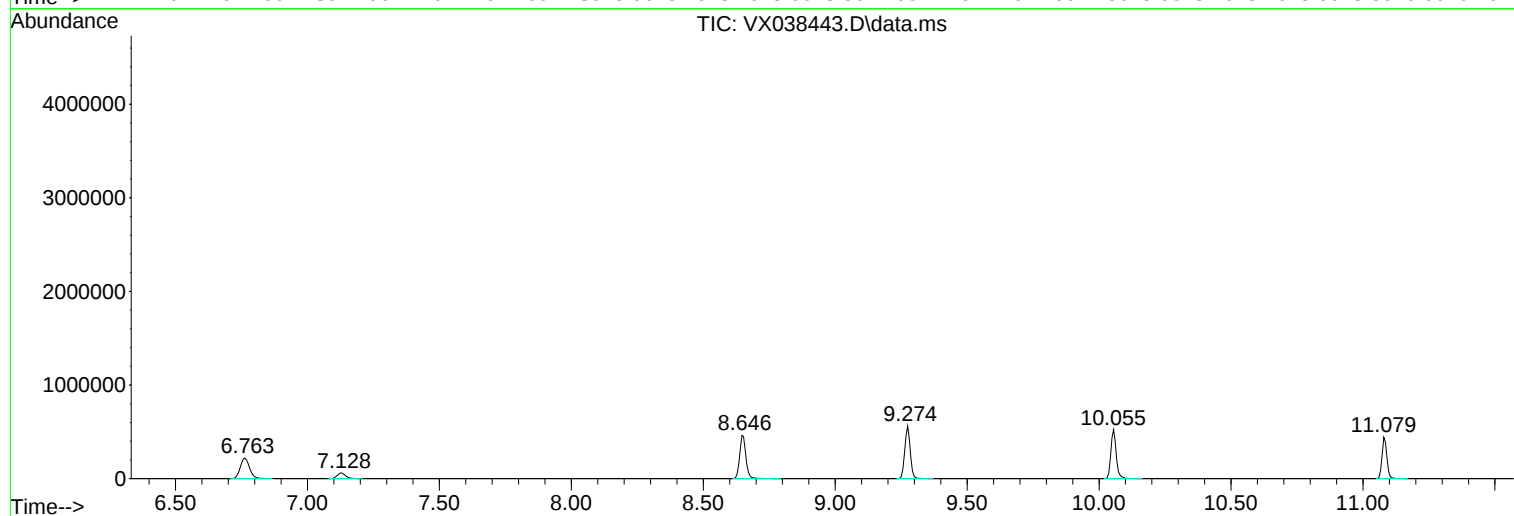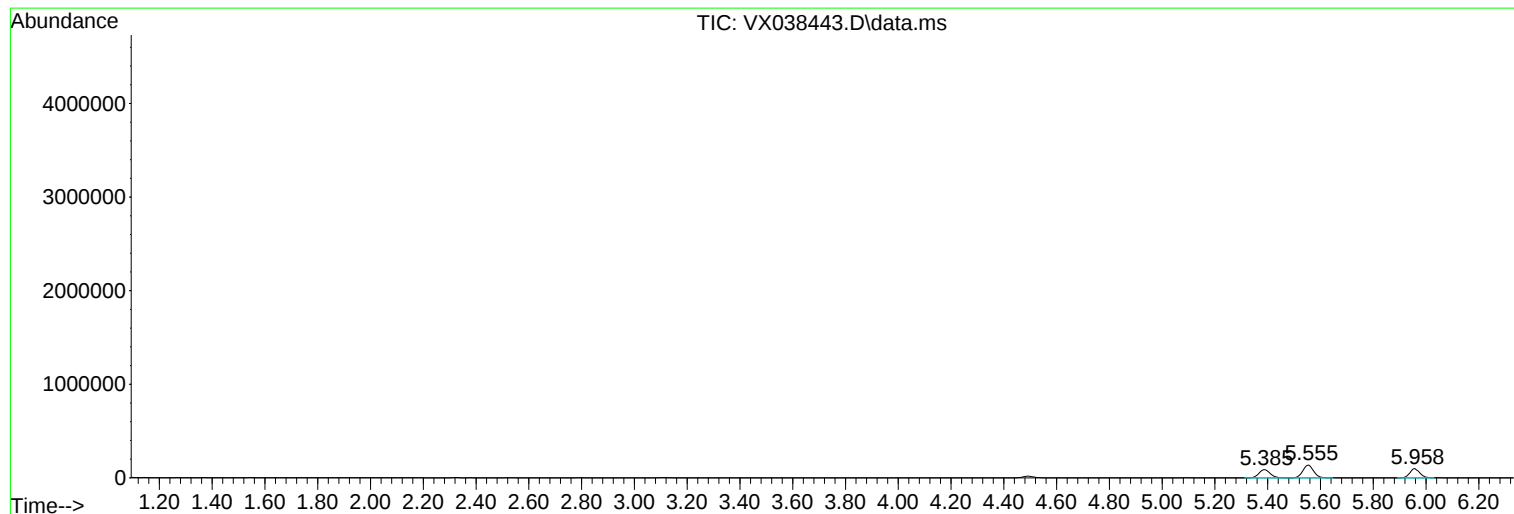

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038443.D
Acq On : 23 Oct 2023 19:19
Operator : JC/MD
Sample : 05007-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-26-23-26










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,2,3,4-tetrachloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.249	9.39 ug/l	165458	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,2,3,4-tetrachloro-	214	C6H2Cl4	000634-66-2	99
2			Benzene, 1,2,3,5-tetrachloro-	214	C6H2Cl4	000634-90-2	99
3			Benzene, 1,2,4,5-tetrachloro-	214	C6H2Cl4	000095-94-3	99
4			Imidazole, 4-bromo-2-trifluorome...	214	C4H2BrF3N2	219534-98-2	46
5			3,4-Dichlorobenzotrifluoride	214	C7H3Cl2F3	000328-84-7	38

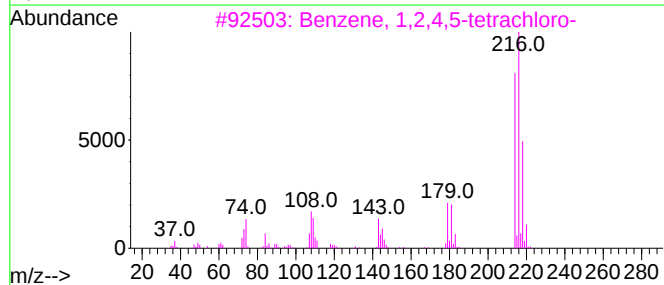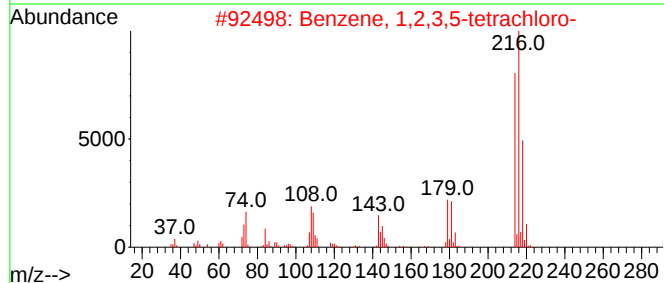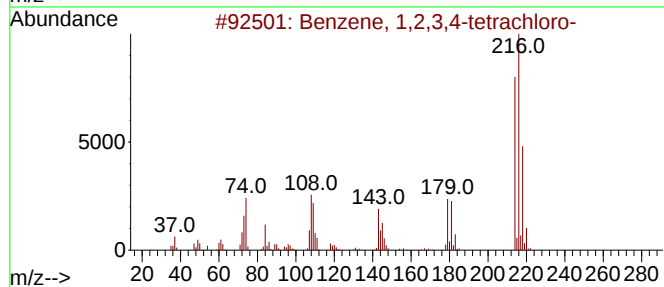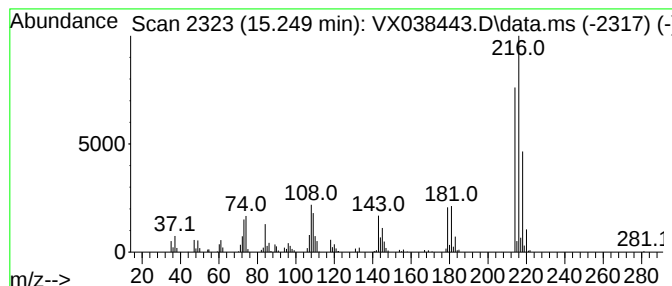

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038443.D
Acq On : 23 Oct 2023 19:19
Operator : JC/MD
Sample : 05007-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-26-23-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,2,3,...	15.249	9.4	ug/l	165458	4	12.024	880841	50.0