

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
 Data File : VX038444.D
 Acq On : 23 Oct 2023 19:43
 Operator : JC/MD
 Sample : 04980-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MAIN-BAILER-SUMP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Title : SW846 8260

Signal : TIC: VX038444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.495	549	559	567	rBV2	20186	56048	7.21%	1.234%
2	5.385	693	705	721	rBV	87899	257812	33.15%	5.678%
3	5.550	722	732	748	rVV	132173	378480	48.66%	8.336%
4	5.958	789	799	811	rBV2	92093	250920	32.26%	5.527%
5	6.763	921	931	951	rBV	222850	533148	68.55%	11.743%
6	7.135	985	992	1002	rVB2	6561	14227	1.83%	0.313%
7	8.647	1234	1240	1260	rBV	452921	745511	95.85%	16.420%
8	9.275	1337	1343	1357	rVB	87296	132440	17.03%	2.917%
9	10.055	1465	1471	1487	rBV	516661	713715	91.77%	15.720%
10	11.079	1634	1639	1652	rBV	428957	562431	72.31%	12.388%
11	12.024	1788	1794	1804	rBV	599877	777763	100.00%	17.130%
12	13.585	2043	2050	2063	rBV	68977	89884	11.56%	1.980%
13	13.963	2106	2112	2119	rBV	14971	19798	2.55%	0.436%
14	15.249	2318	2323	2328	rBV2	5447	8050	1.04%	0.177%




Sum of corrected areas: 4540227

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038444.D
Acq On : 23 Oct 2023 19:43
Operator : JC/MD
Sample : 04980-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MAIN-BAILER-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

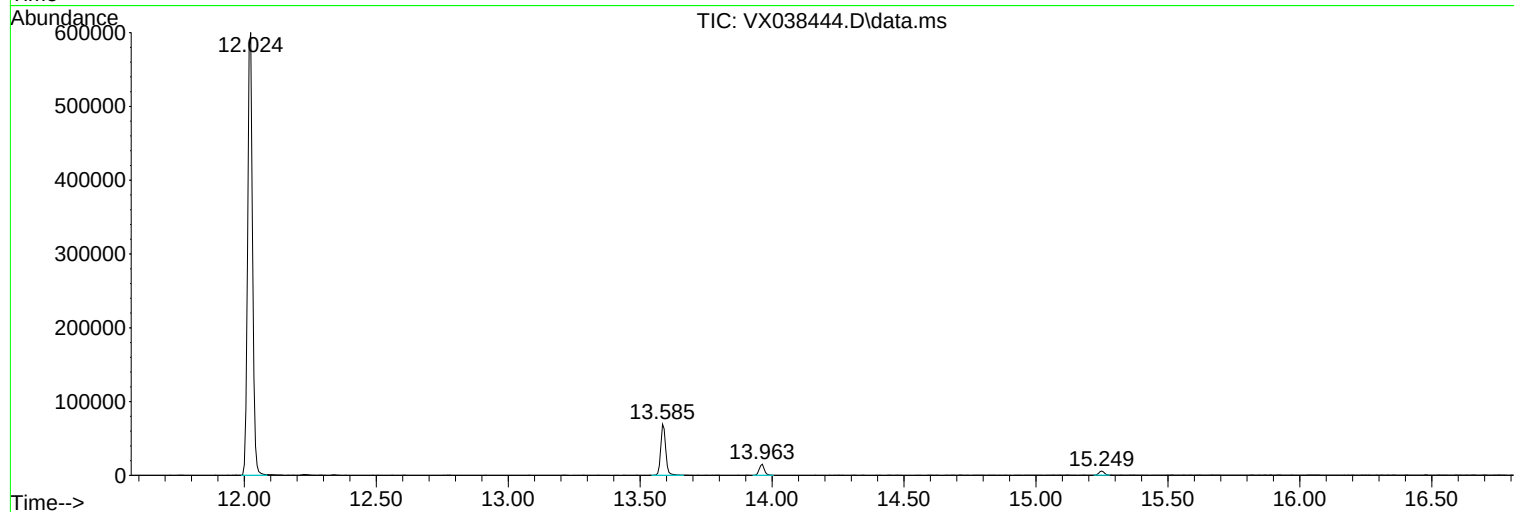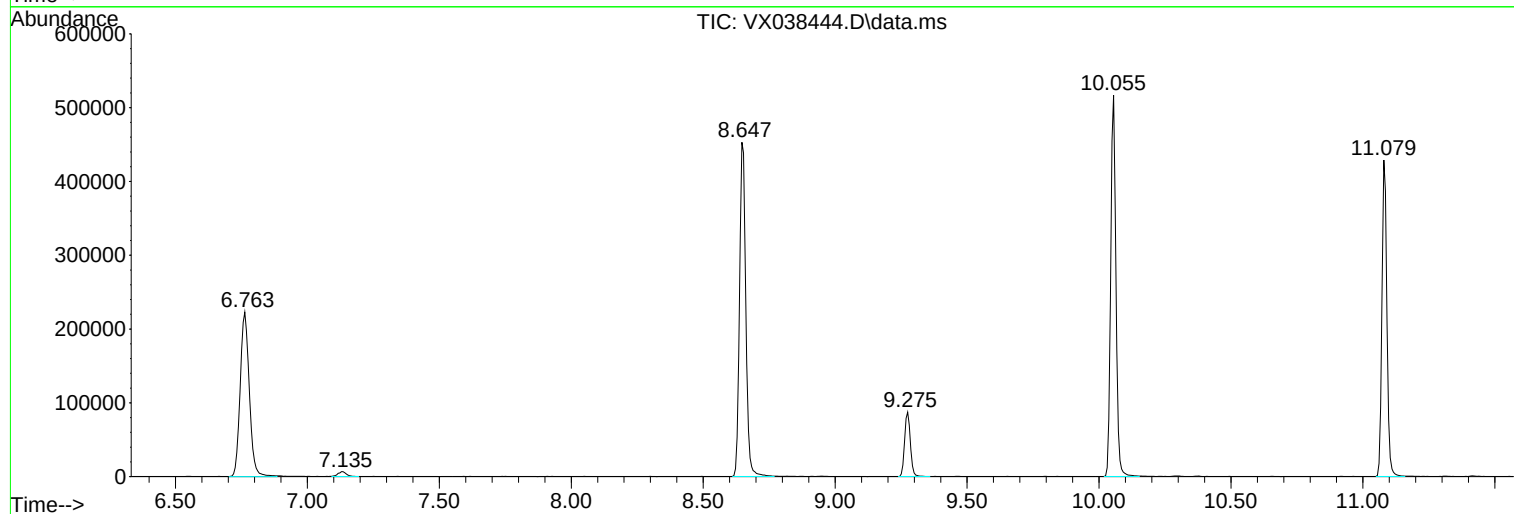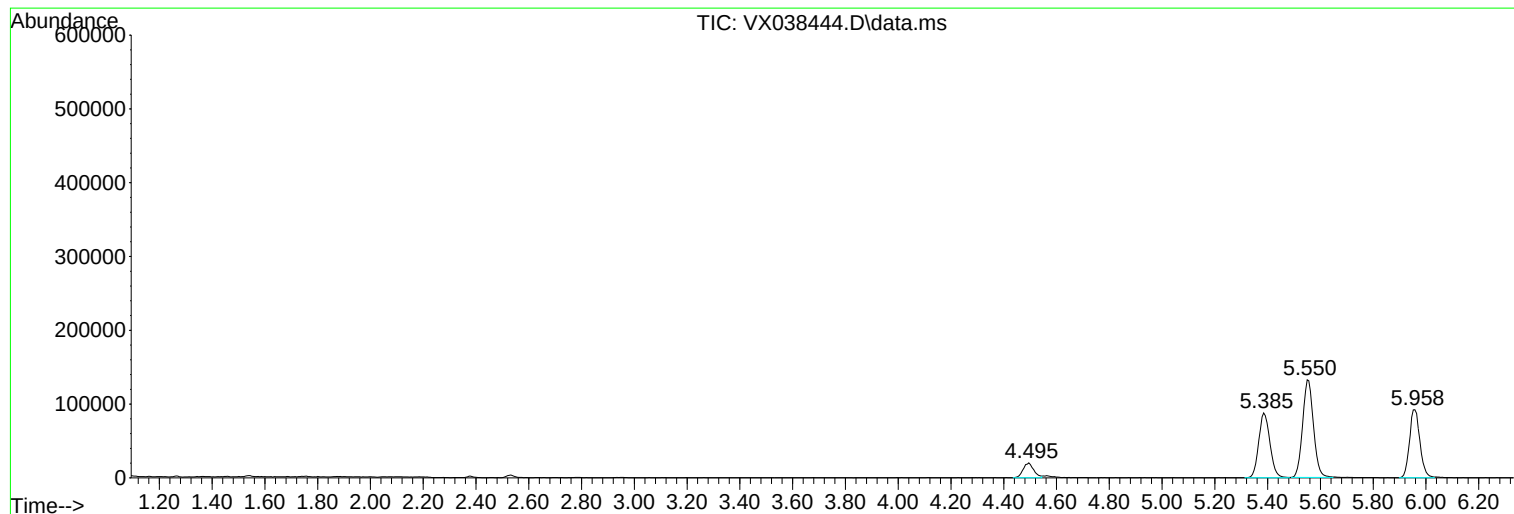

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038444.D
Acq On : 23 Oct 2023 19:43
Operator : JC/MD
Sample : 04980-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MAIN-BAILER-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038444.D
Acq On : 23 Oct 2023 19:43
Operator : JC/MD
Sample : 04980-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MAIN-BAILER-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------