

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
 Data File : VX038445.D
 Acq On : 23 Oct 2023 20:06
 Operator : JC/MD
 Sample : 04980-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BRIDAL-SHOP-BAY-SUMP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	692	705	722	rBV2	90553	264536	23.19%	4.853%
2	5.550	722	732	747	rBV	134740	389469	34.15%	7.144%
3	5.958	788	799	815	rBV2	95853	256913	22.53%	4.713%
4	6.763	921	931	945	rBV	224165	542321	47.55%	9.948%
5	8.647	1233	1240	1266	rBV	471682	764653	67.04%	14.027%
6	9.275	1335	1343	1364	rBV	779455	1140538	100.00%	20.922%
7	10.055	1465	1471	1485	rBV	527263	725252	63.59%	13.304%
8	11.079	1634	1639	1653	rBV	427017	562578	49.33%	10.320%
9	12.024	1788	1794	1806	rBV	582310	758556	66.51%	13.915%
10	13.591	2045	2051	2059	rBV	34222	46631	4.09%	0.855%




Sum of corrected areas: 5451447

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038445.D
Acq On : 23 Oct 2023 20:06
Operator : JC/MD
Sample : 04980-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BRIDAL-SHOP-BAY-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

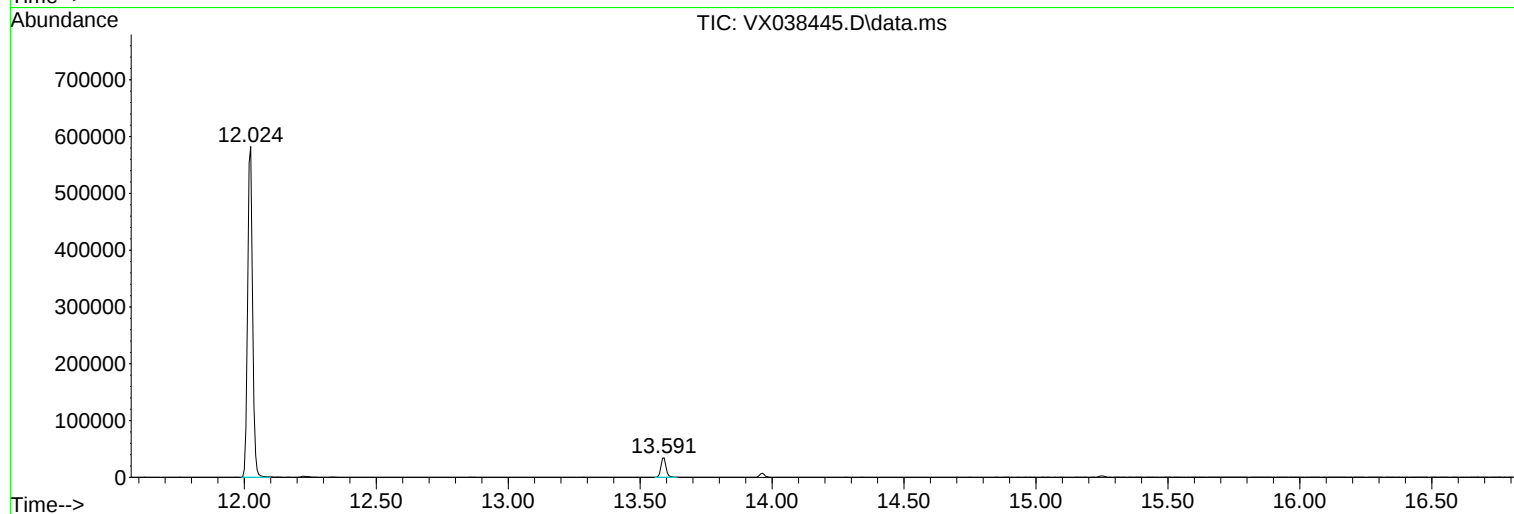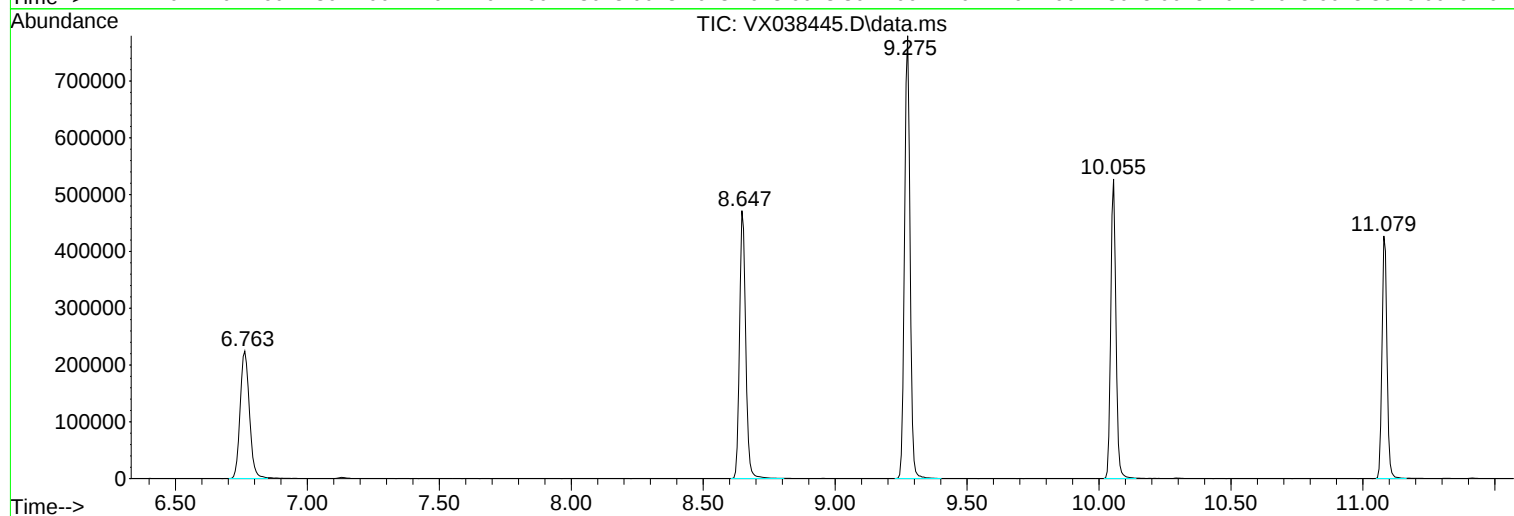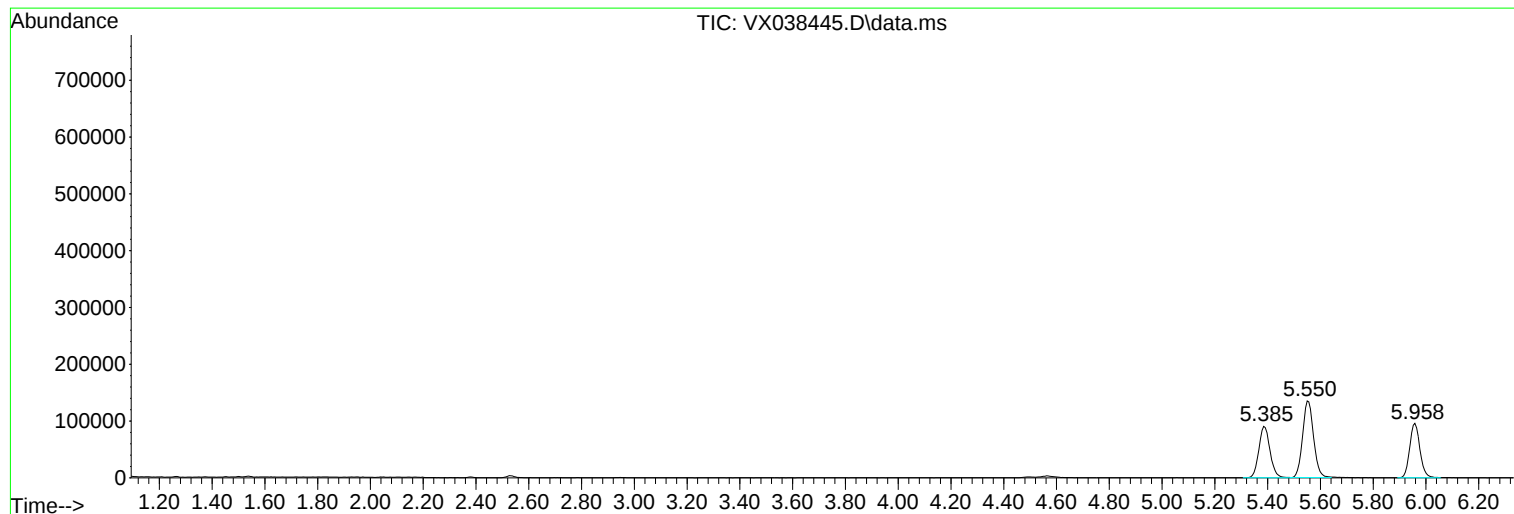

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038445.D
Acq On : 23 Oct 2023 20:06
Operator : JC/MD
Sample : 04980-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BRIDAL-SHOP-BAY-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038445.D
Acq On : 23 Oct 2023 20:06
Operator : JC/MD
Sample : 04980-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BRIDAL-SHOP-BAY-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
