
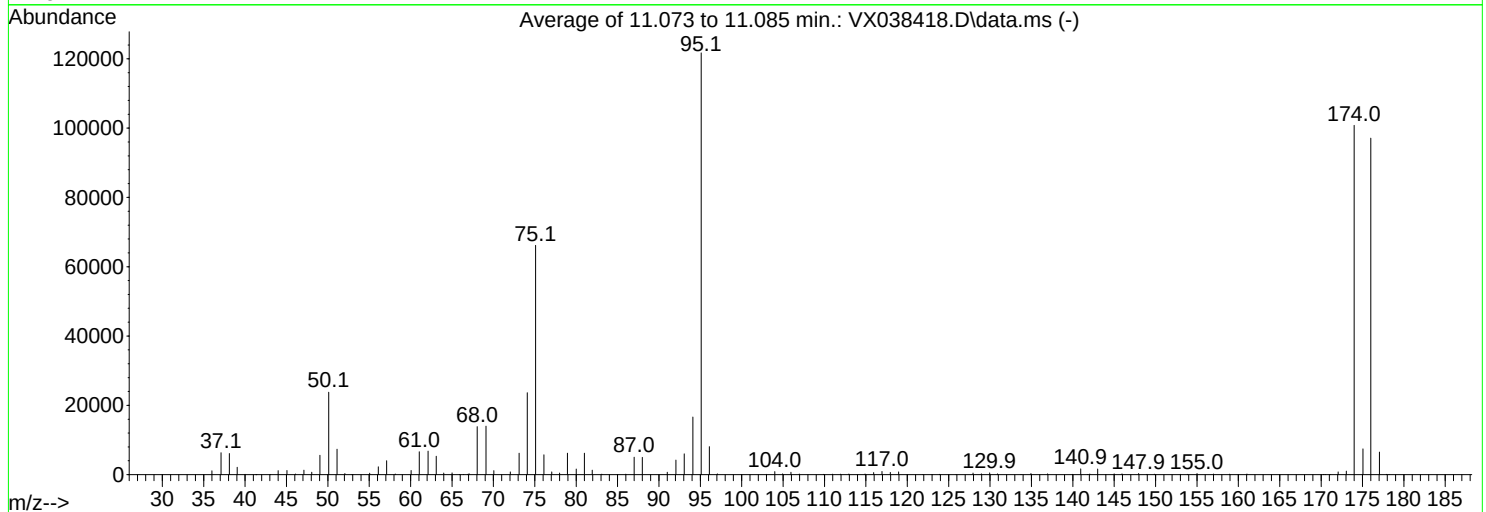


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102323\
Data File : VX038418.D
Acq On : 23 Oct 2023 08:51
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Title : SW846 8260
Last Update : Thu Oct 05 15:27:13 2023

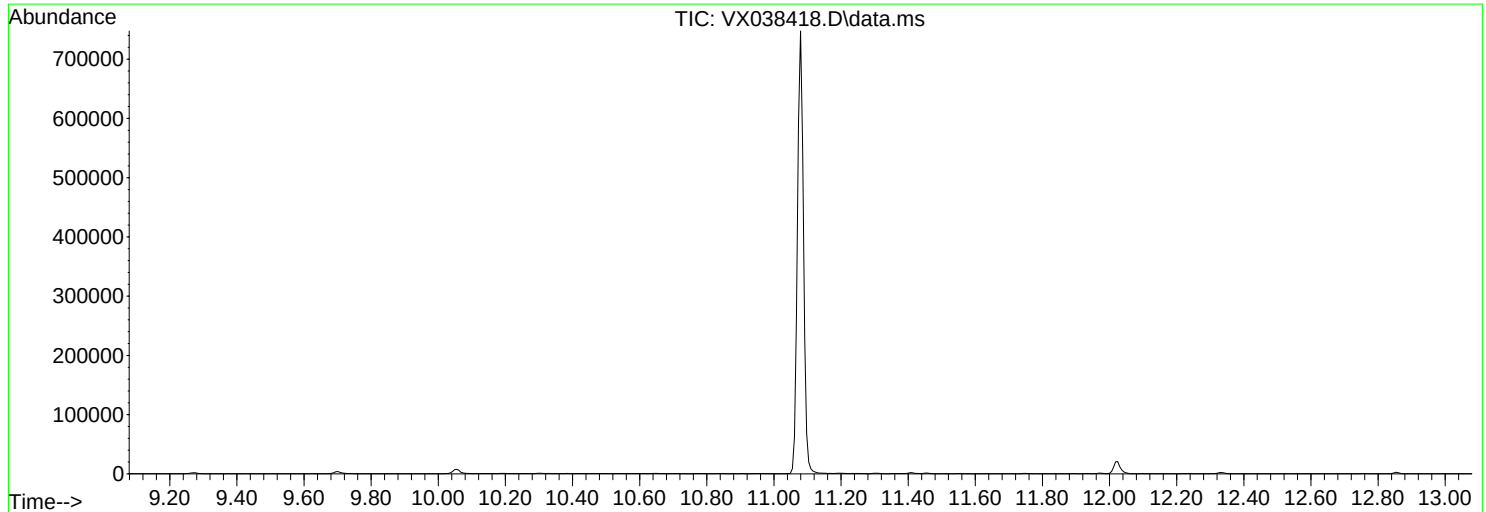

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	23803	PASS
75	95	30	60	54.4	66163	PASS
95	95	100	100	100.0	121725	PASS
96	95	5	9	6.6	8075	PASS
173	174	0.00	2	1.0	1019	PASS
174	95	50	100	82.8	100781	PASS
175	174	5	9	7.4	7445	PASS
176	174	95	101	96.4	97117	PASS
177	176	5	9	6.7	6527	PASS