

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102325\
 Data File : VX048331.D
 Acq On : 23 Oct 2025 17:09
 Operator : JC/MD
 Sample : Q3414-04 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Oct 24 05:49:41 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 20 14:13:59 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	128533	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	257143	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	267567	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	139217	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	102797	57.042	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 114.080%	
35) Dibromofluoromethane	5.379	113	70529	40.176	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 80.360%	
50) Toluene-d8	8.635	98	288452	46.878	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 93.760%	
62) 4-Bromofluorobenzene	11.061	95	131108	56.008	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 112.020%	


Target Compounds			Qvalue			
10) Methyl Iodide	2.465	142	1205	0.691	ug/l #	88
13) Acrolein	2.233	56	41	0.225	ug/l #	1
16) Acetone	2.374	43	2872	4.646	ug/l	96
18) Methyl Acetate	2.709	43	728	0.564	ug/l #	72
20) Methylene Chloride	2.788	84	630	0.418	ug/l #	81
36) 1,1-Dichloropropene	5.538	75	10689	4.284	ug/l #	50
38) Carbon Tetrachloride	5.531	117	13922	4.523	ug/l #	15
39) Methylcyclohexane	7.367	83	623	0.211	ug/l #	70
40) Benzene	6.025	78	646561	89.252	ug/l	98
42) 1,2-Dichloroethane	6.031	62	6260	2.342	ug/l #	76
48) Methyl methacrylate	7.787	41	4047	2.361	ug/l #	44
51) 4-Methyl-2-Pentanone	8.537	43	4714	2.407	ug/l #	50
52) Toluene	8.702	92	399804	86.874	ug/l	100
53) t-1,3-Dichloropropene	8.702	75	5064	1.814	ug/l #	1
54) cis-1,3-Dichloropropene	8.537	75	1799	0.597	ug/l #	46
55) 1,1,2-Trichloroethane	9.000	97	2985	1.744	ug/l #	18
59) 2-Hexanone	9.464	43	1664	1.218	ug/l #	56
67) Ethyl Benzene	10.177	91	59437	5.800	ug/l	99
68) m/p-Xylenes	10.281	106	123259	32.372	ug/l	100
69) o-Xylene	10.622	106	107237	29.173	ug/l	98
70) Styrene	10.640	104	36238	5.790	ug/l #	54
73) Isopropylbenzene	10.945	105	3312	0.326	ug/l	99
76) 1,2,3-Trichloropropane	11.061	75	70989	31.444	ug/l #	33
78) n-propylbenzene	11.287	91	7319	0.622	ug/l	99
79) 2-Chlorotoluene	11.360	91	5015	0.703	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.433	105	29275	3.479	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.061	75	70989	76.501	ug/l #	10
82) 4-Chlorotoluene	11.433	91	3622	0.427	ug/l #	46
84) 1,2,4-Trimethylbenzene	11.732	105	83706	9.967	ug/l	97
85) sec-Butylbenzene	11.732	105	83706	8.047	ug/l #	56
90) Hexachloroethane	12.530	117	734	0.413	ug/l #	16
95) Naphthalene	13.756	128	429379	53.105	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102325\
Data File : VX048331.D
Acq On : 23 Oct 2025 17:09
Operator : JC/MD
Sample : Q3414-04 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Oct 24 05:49:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Quant Title : SW846 8260
QLast Update : Mon Oct 20 14:13:59 2025
Response via : Initial Calibration




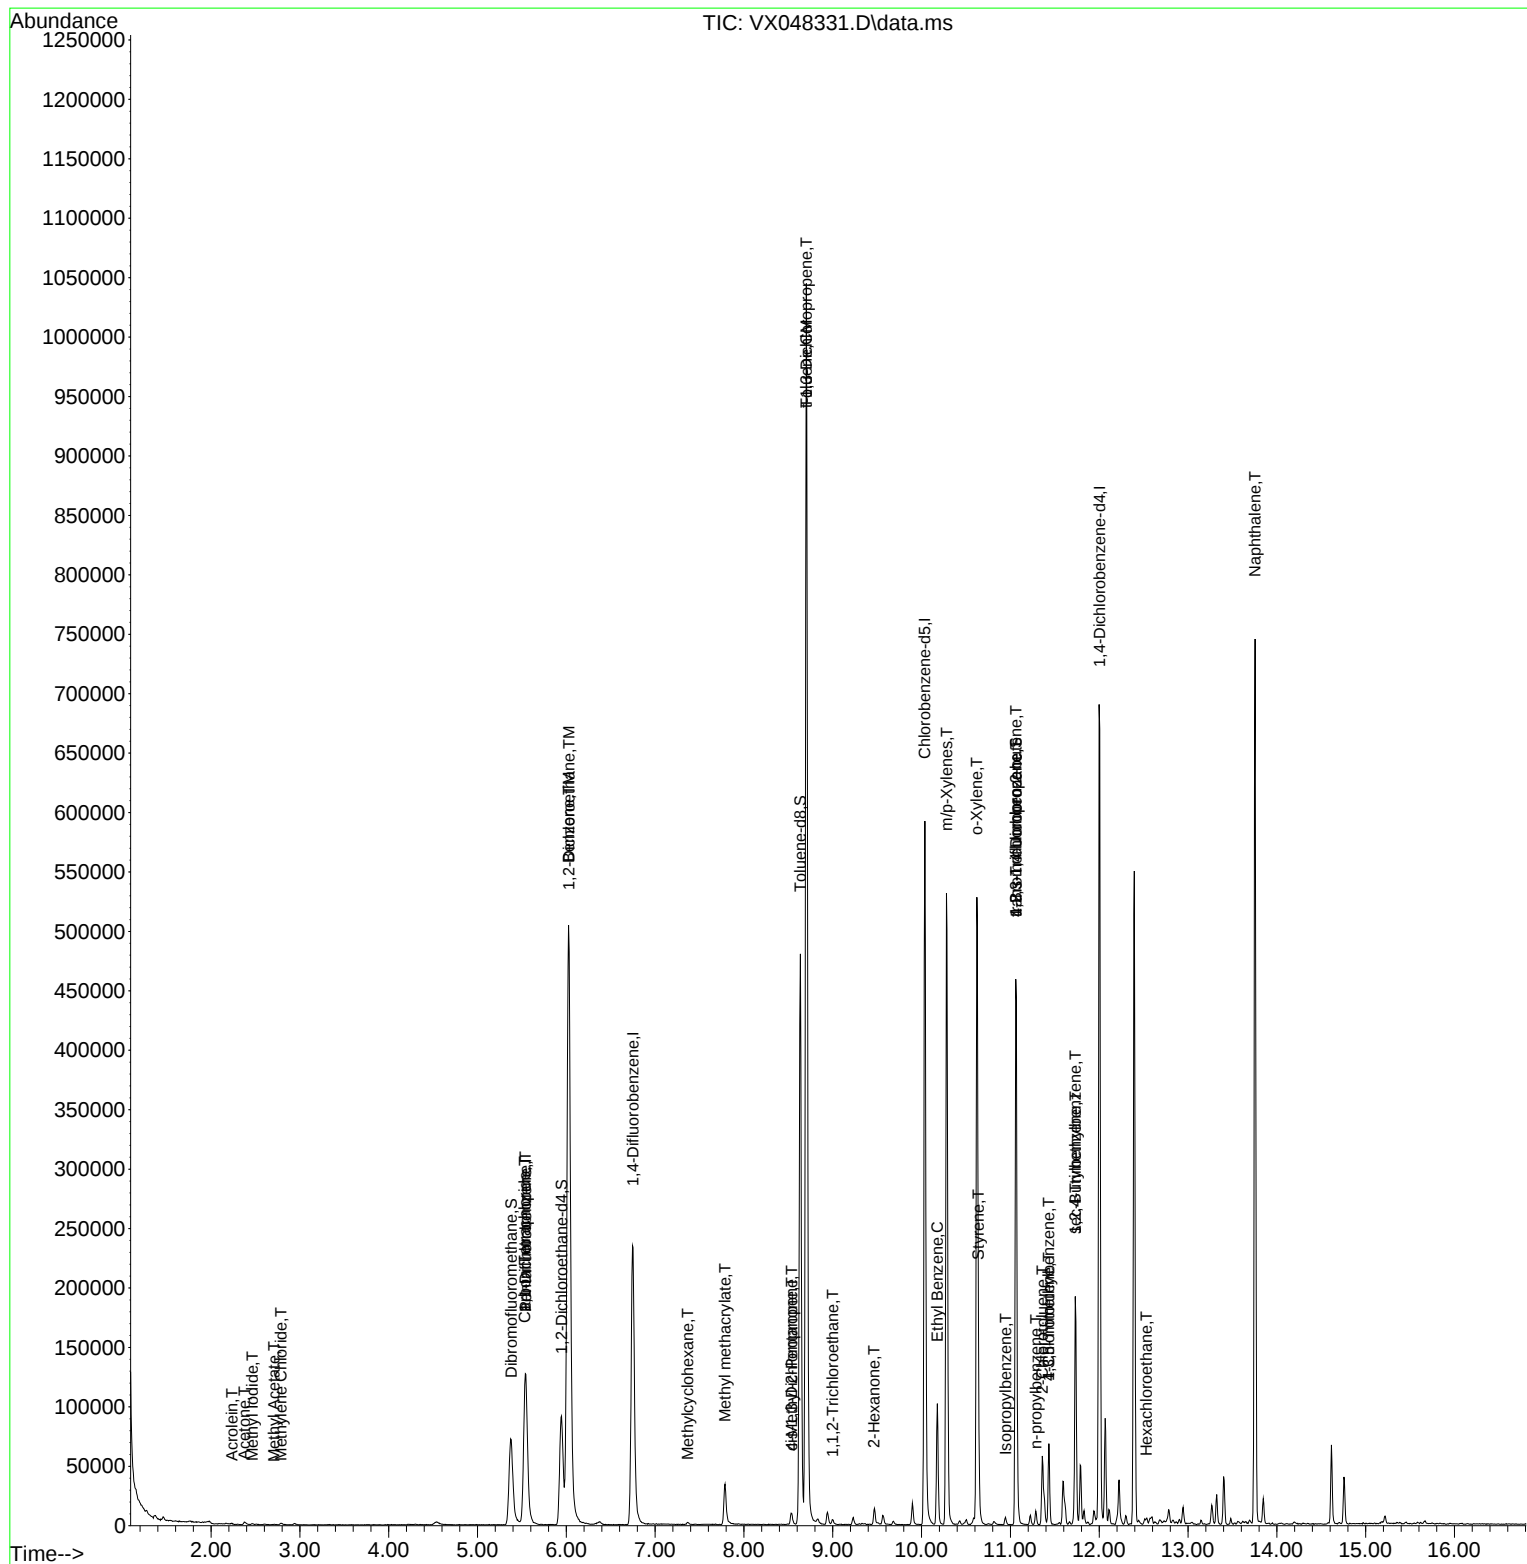




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 128533
Ion Ratio Lower Upper
168 100
99 63.3 46.4 69.6

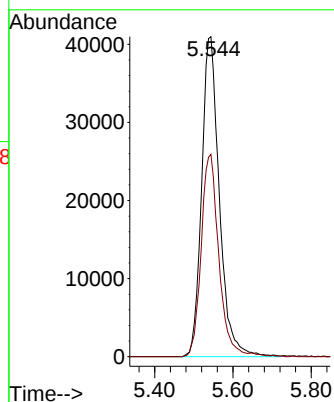

#10
Methyl Iodide
Concen: 0.691 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.006 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09


Tgt Ion:142 Resp: 1205
Ion Ratio Lower Upper
142 100
127 42.4 38.5 57.7
141 5.4 11.6 17.4#

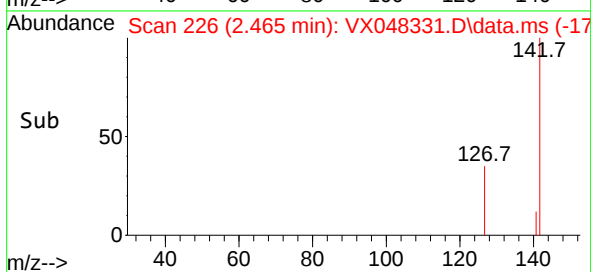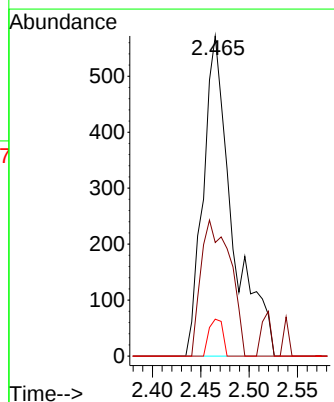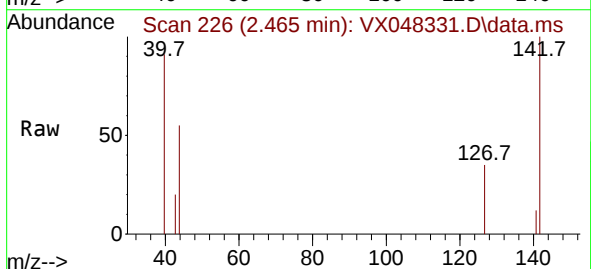






#13
Acrolein
Concen: 0.225 ug/l
RT: 2.233 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 41
Ion Ratio Lower Upper
56 100
55 448.8 56.1 84.1#

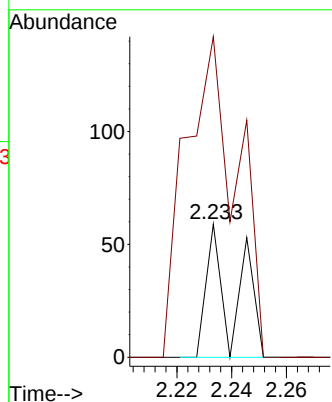

#16
Acetone
Concen: 4.646 ug/l
RT: 2.374 min Scan# 211
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Tgt Ion: 43 Resp: 2872
Ion Ratio Lower Upper
43 100
58 31.2 23.4 35.2


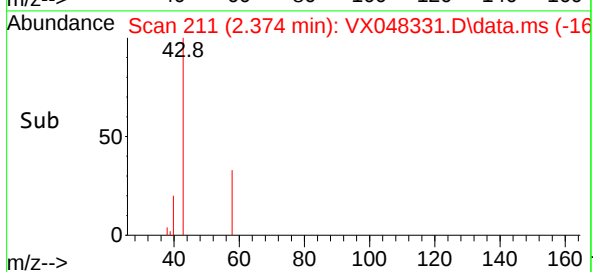
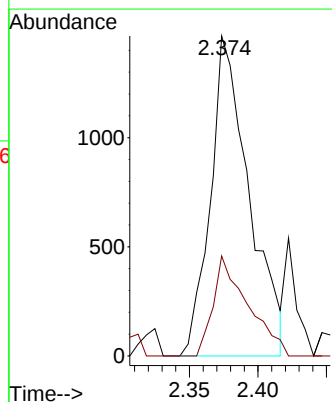
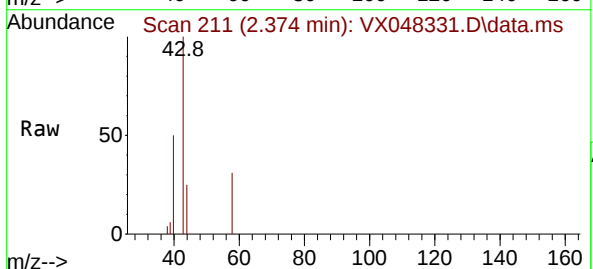




#18
Methyl Acetate
Concen: 0.564 ug/l
RT: 2.709 min Scan# 20
Delta R.T. 0.012 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 728
Ion Ratio Lower Upper
43 100
74 8.5 17.5 26.3#

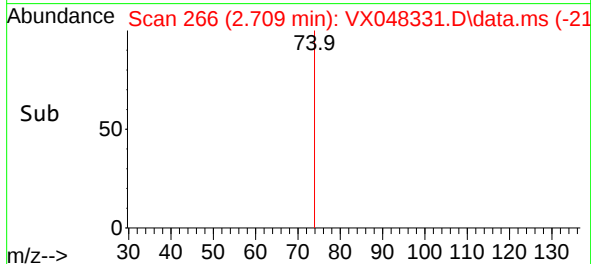

#20
Methylene Chloride
Concen: 0.418 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Tgt Ion: 84 Resp: 630
Ion Ratio Lower Upper
84 100
49 102.5 104.1 156.1#
51 41.6 31.3 46.9
86 50.6 51.3 76.9#

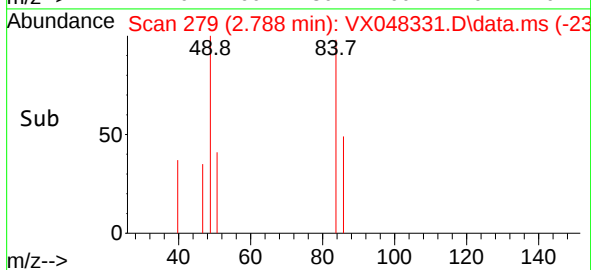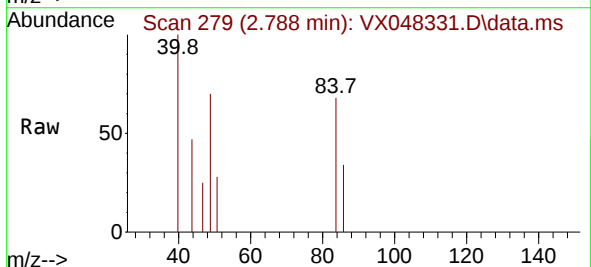



#33

1,2-Dichloroethane-d4

Concen: 57.042 ug/l

RT: 5.946 min Scan# 796

Delta R.T. 0.006 min

Lab File: VX048331.D

Acq: 23 Oct 2025 17:09

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 102797

Ion Ratio Lower Upper

65 100

67 50.2 0.0 105.0

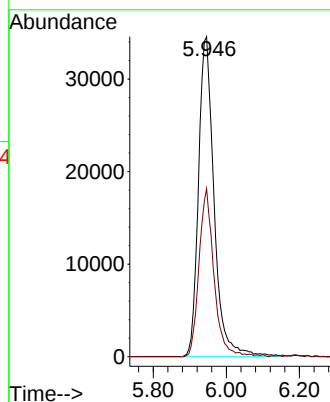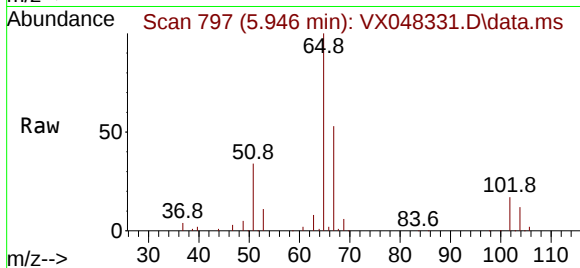

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.751 min Scan# 929

Delta R.T. 0.006 min

Lab File: VX048331.D

Acq: 23 Oct 2025 17:09




Tgt Ion: 114 Resp: 257143


Ion Ratio Lower Upper

114 100

63 21.4 0.0 43.2

88 15.8 0.0 33.6

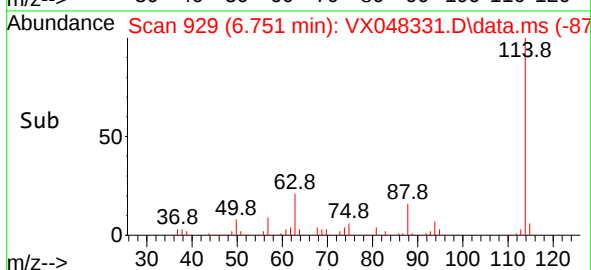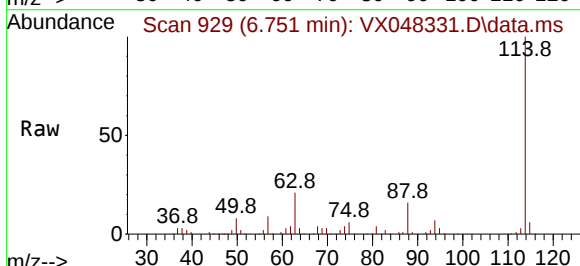



#35

Dibromofluoromethane

Concen: 40.176 ug/l

RT: 5.379 min Scan# 704

Delta R.T. 0.006 min


Lab File: VX048331.D

Acq: 23 Oct 2025 17:09

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion:113 Resp: 70529

Ion Ratio Lower Upper

113 100

111 101.0 82.2 123.4

192 17.3 15.1 22.7

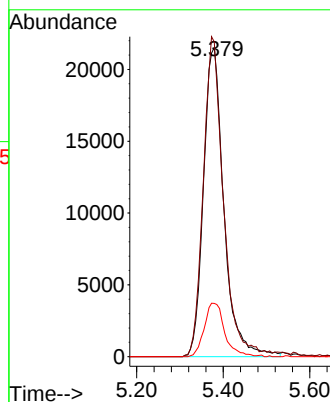

#36

1,1-Dichloropropene

Concen: 4.284 ug/l

RT: 5.538 min Scan# 730

Delta R.T. -0.146 min

Lab File: VX048331.D

Acq: 23 Oct 2025 17:09




Tgt Ion: 75 Resp: 10689


Ion Ratio Lower Upper

75 100

110 8.9 17.7 53.1#


77 0.0 24.3 36.5#

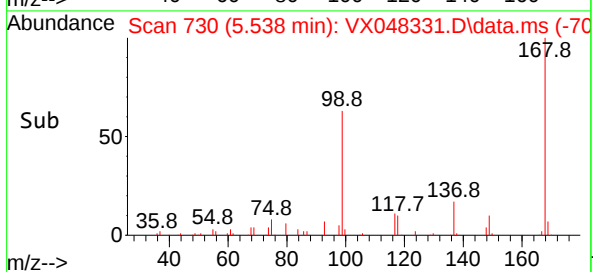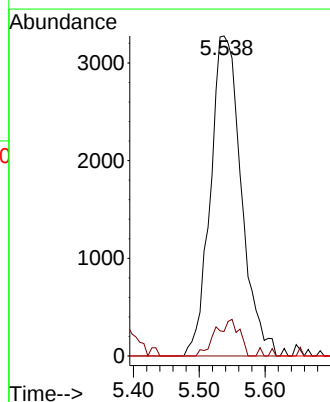






#38
Carbon Tetrachloride
Concen: 4.523 ug/l
RT: 5.531 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 13922
Ion Ratio Lower Upper
117 100
119 3.7 77.2 115.8#
121 0.0 24.8 37.2#

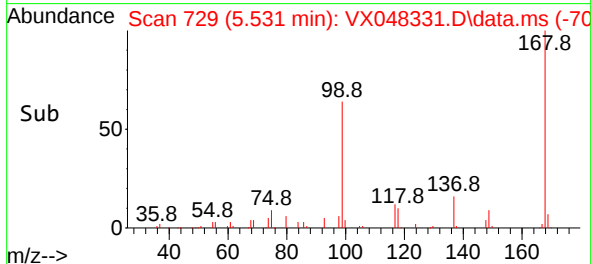

#39
Methylcyclohexane
Concen: 0.211 ug/l
RT: 7.367 min Scan# 1030
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Tgt Ion: 83 Resp: 623
Ion Ratio Lower Upper
83 100
55 109.6 66.2 99.2#
98 27.3 38.9 58.3#


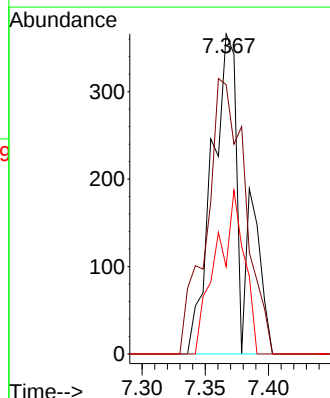
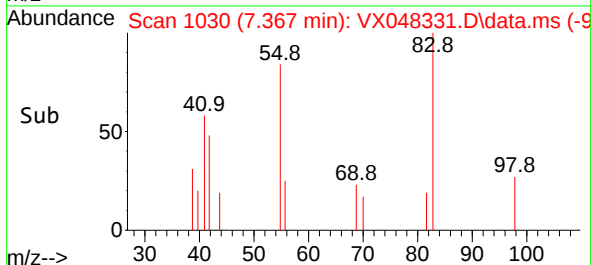
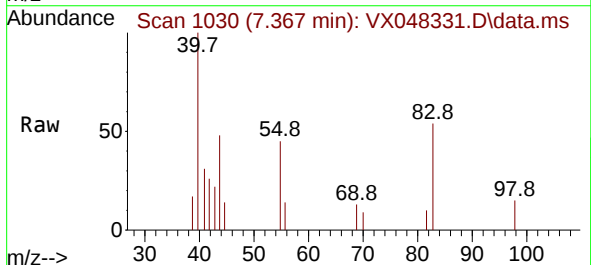




#40
Benzene
Concen: 89.252 ug/l
RT: 6.025 min Scan# 810
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 78 Resp: 646561
Ion Ratio Lower Upper
78 100
77 23.3 19.3 28.9

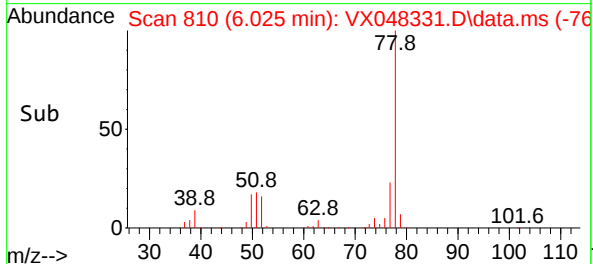

#42
1,2-Dichloroethane
Concen: 2.342 ug/l
RT: 6.031 min Scan# 811
Delta R.T. -0.037 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09


Tgt Ion: 62 Resp: 6260
Ion Ratio Lower Upper
62 100
98 0.0 0.0 17.2

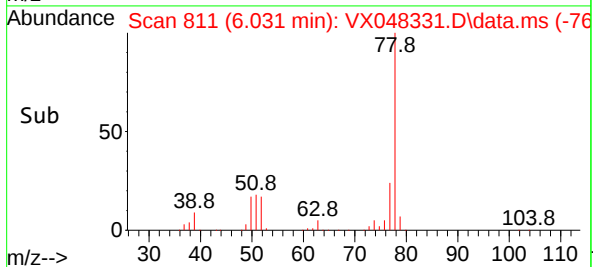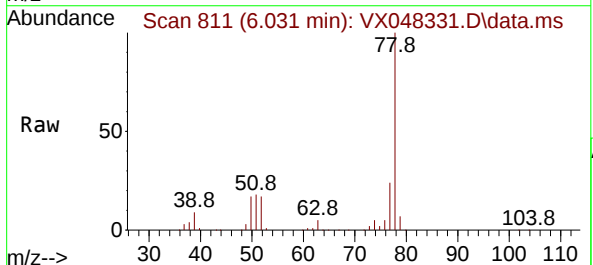






#48
Methyl methacrylate
Concen: 2.361 ug/l
RT: 7.787 min Scan# 1099
Delta R.T. 0.110 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 41 Resp: 4047
Ion Ratio Lower Upper
41 100
69 0.0 63.4 95.0#
39 51.7 47.1 70.7

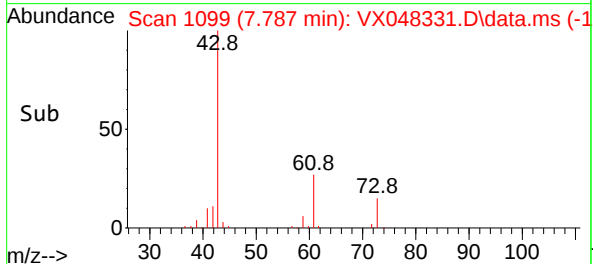

#50
Toluene-d8
Concen: 46.878 ug/l
RT: 8.635 min Scan# 1238
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Tgt Ion: 98 Resp: 288452
Ion Ratio Lower Upper
98 100
100 65.6 53.0 79.4

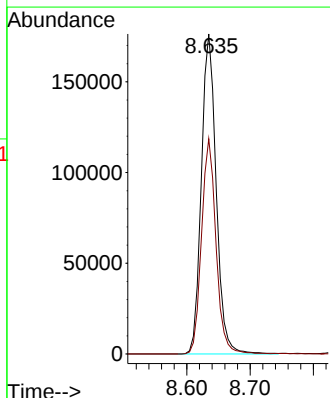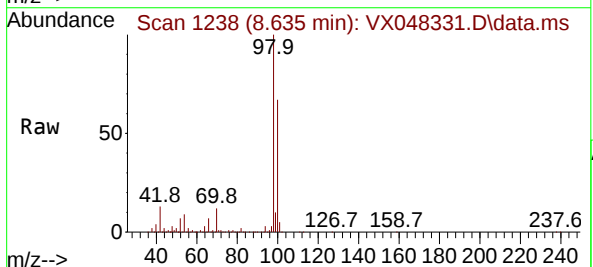



#51

4-Methyl-2-Pentanone

Concen: 2.407 ug/l

RT: 8.537 min Scan# 11

Delta R.T. -0.018 min

Lab File: VX048331.D

Acq: 23 Oct 2025 17:09

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 4714

Ion Ratio Lower Upper

43 100

58 7.2 29.5 44.3#

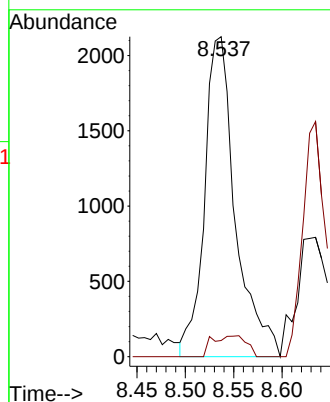

#52

Toluene

Concen: 86.874 ug/l

RT: 8.702 min Scan# 1249

Delta R.T. -0.000 min

Lab File: VX048331.D




Acq: 23 Oct 2025 17:09


Tgt Ion: 92 Resp: 399804

Ion Ratio Lower Upper

92 100

91 169.8 136.1 204.1

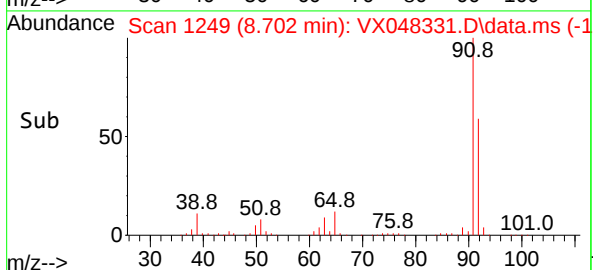



#53

t-1,3-Dichloropropene

Concen: 1.814 ug/l

RT: 8.702 min Scan# 11

Delta R.T. -0.262 min

Lab File: VX048331.D

Acq: 23 Oct 2025 17:09

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 5064

Ion Ratio Lower Upper

75 100

77 156.1 25.0 37.6#

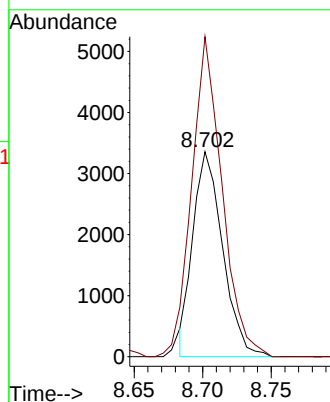

#54

cis-1,3-Dichloropropene

Concen: 0.597 ug/l

RT: 8.537 min Scan# 1222

Delta R.T. 0.189 min

Lab File: VX048331.D

Acq: 23 Oct 2025 17:09




Tgt Ion: 75 Resp: 1799


Ion Ratio Lower Upper

75 100

77 0.0 24.9 37.3#


39 90.2 42.6 64.0#

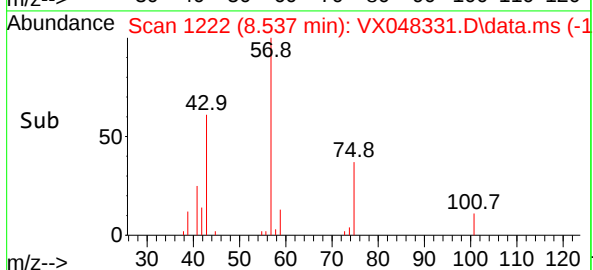






#55
 1,1,2-Trichloroethane
 Concen: 1.744 ug/l
 RT: 9.000 min Scan# 11
 Delta R.T. -0.134 min
 Lab File: VX048331.D
 Acq: 23 Oct 2025 17:09

Instrument :
 MSVOA_X
 ClientSampleId :







Tgt Ion	Ratio	Lower	Upper
97	100		
83	0.0	70.6	105.8#
85	0.0	45.0	67.6#
99	10.3	50.9	76.3#

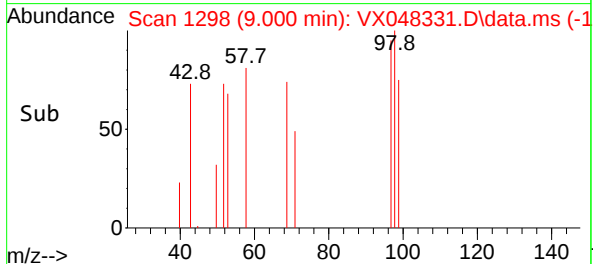

#59
 2-Hexanone
 Concen: 1.218 ug/l
 RT: 9.464 min Scan# 1374
 Delta R.T. 0.049 min
 Lab File: VX048331.D
 Acq: 23 Oct 2025 17:09

Tgt Ion	Ratio	Lower	Upper
43	100		
58	21.2	26.3	78.8#


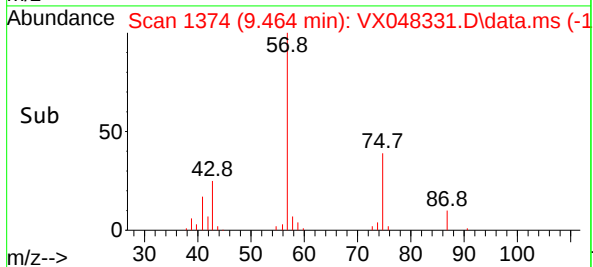
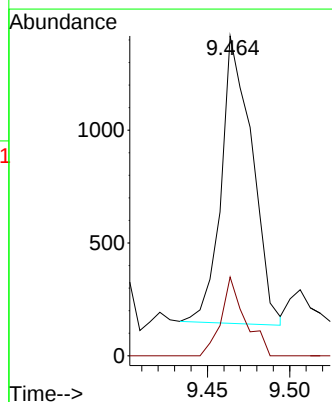
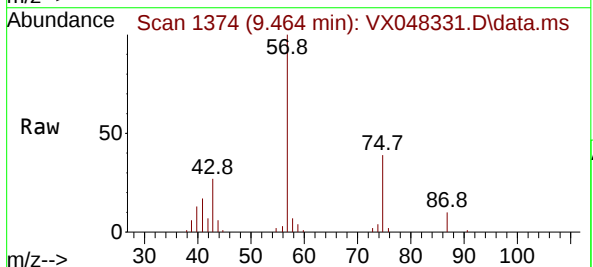




#62
4-Bromofluorobenzene
Concen: 56.008 ug/l
RT: 11.061 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 131108
Ion Ratio Lower Upper
95 100
174 72.1 0.0 147.8
176 71.2 0.0 142.8

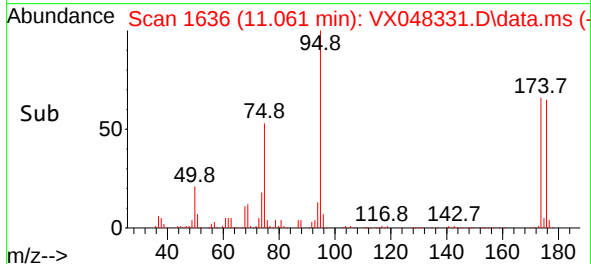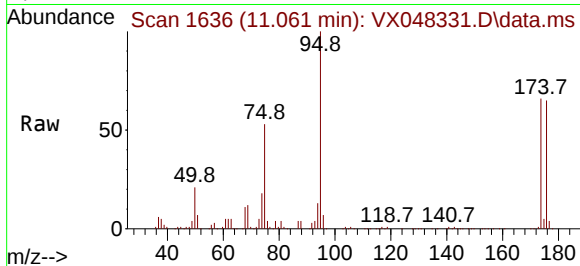

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Tgt Ion: 117 Resp: 267567
Ion Ratio Lower Upper
117 100
82 57.1 46.5 69.7
119 32.1 25.9 38.9


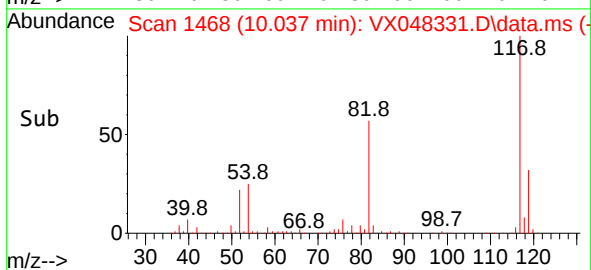

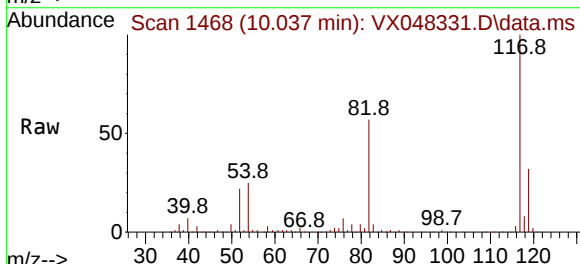




#67
Ethyl Benzene
Concen: 5.800 ug/l
RT: 10.177 min Scan# 1491
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 59437
Ion Ratio Lower Upper
91 100
106 30.3 23.8 35.6

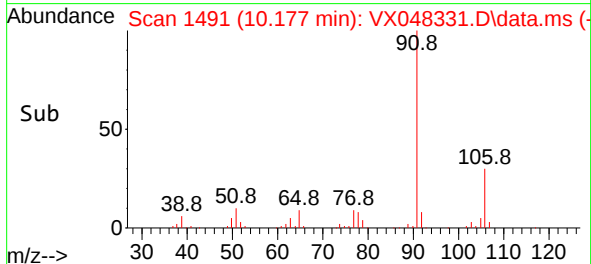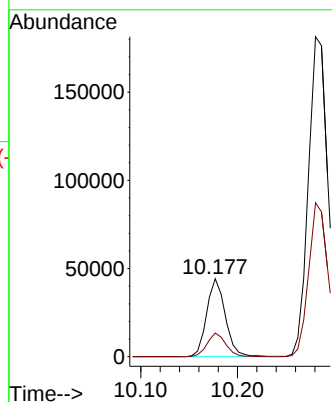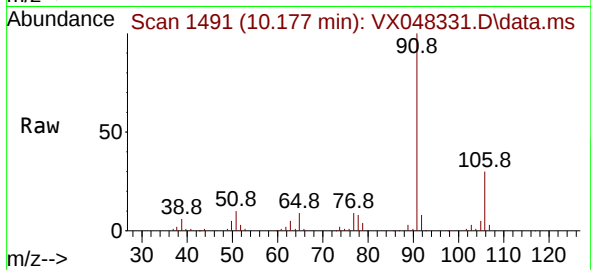

#68
m/p-Xylenes
Concen: 32.372 ug/l
RT: 10.281 min Scan# 1508
Delta R.T. -0.006 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Tgt Ion:106 Resp: 123259
Ion Ratio Lower Upper
106 100
91 210.3 167.9 251.9


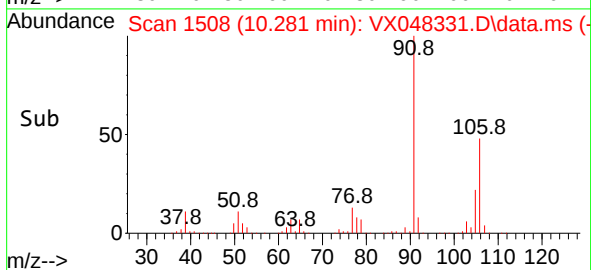
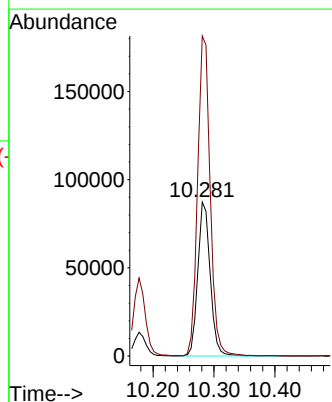
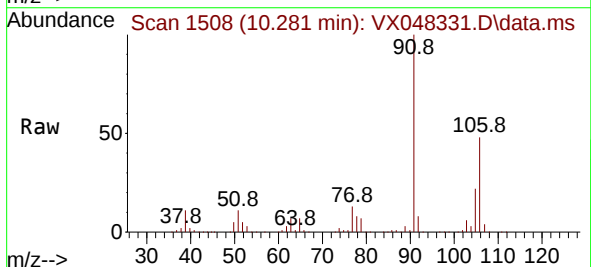




#69
o-Xylene
Concen: 29.173 ug/l
RT: 10.622 min Scan# 1564
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 107237
Ion Ratio Lower Upper
106 100
91 226.2 111.3 333.9

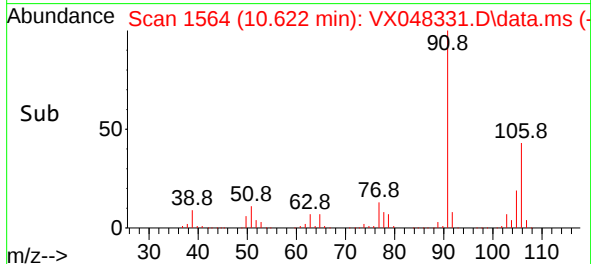

#70
Styrene
Concen: 5.790 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09


Tgt Ion:104 Resp: 36238
Ion Ratio Lower Upper
104 100
78 88.6 42.2 63.4#
103 82.9 43.0 64.4#

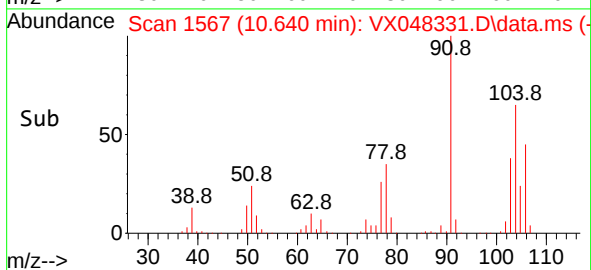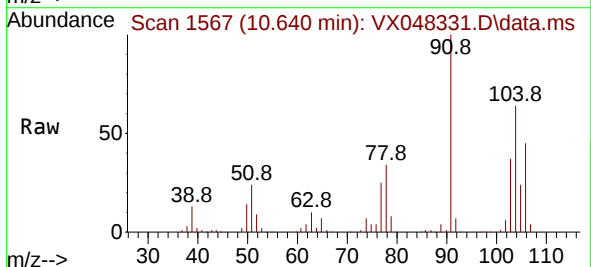






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion:152 Resp: 139217
Ion Ratio Lower Upper
152 100
115 64.2 43.1 129.4
150 159.9 0.0 353.0

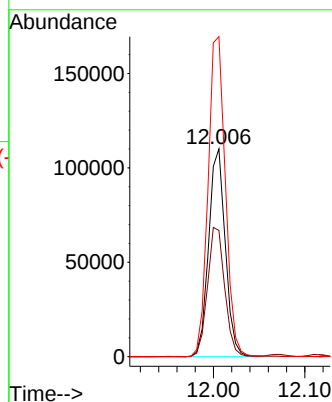


#73
Isopropylbenzene
Concen: 0.326 ug/l
RT: 10.945 min Scan# 1617
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09



Tgt Ion:105 Resp: 3312
Ion Ratio Lower Upper
105 100
120 25.2 13.0 38.9




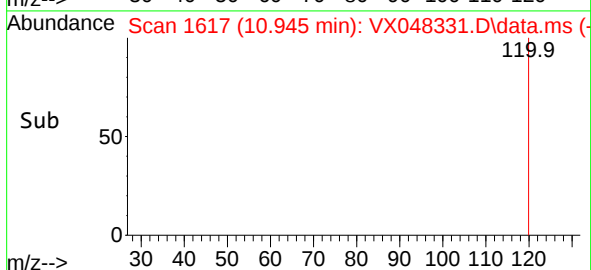




#76
1,2,3-Trichloropropane
Concen: 31.444 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.159 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 70989
Ion Ratio Lower Upper
75 100
77 1.2 22.4 67.2#

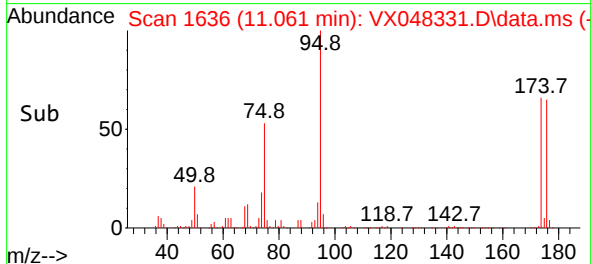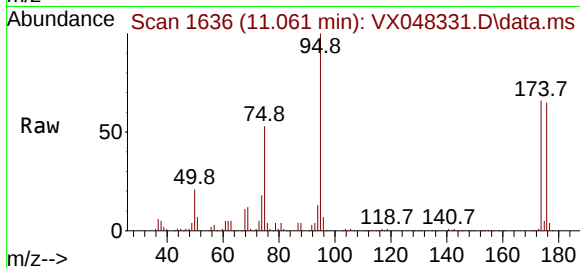

#78
n-propylbenzene
Concen: 0.622 ug/l
RT: 11.287 min Scan# 1673
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Tgt Ion: 91 Resp: 7319
Ion Ratio Lower Upper
91 100
120 22.8 11.1 33.1

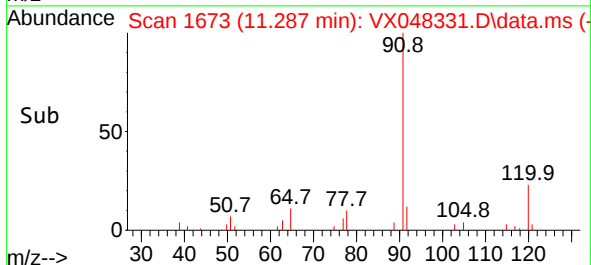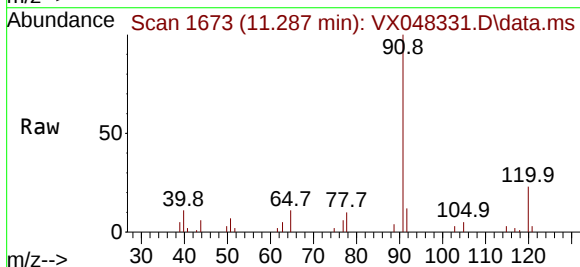



#79

2-Chlorotoluene

Concen: 0.703 ug/l

RT: 11.360 min Scan# 1685

Delta R.T. 0.012 min

Lab File: VX048331.D

Acq: 23 Oct 2025 17:09

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 5015

Ion Ratio Lower Upper

91 100

126 1.1 16.4 49.4#

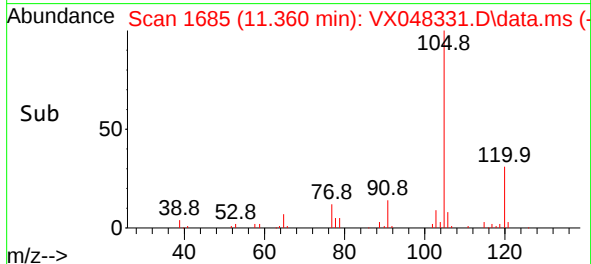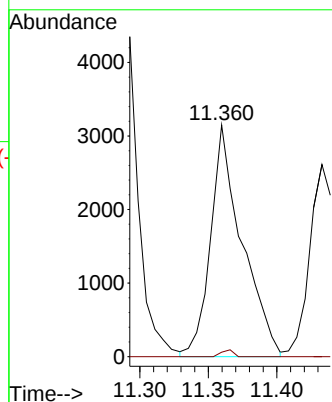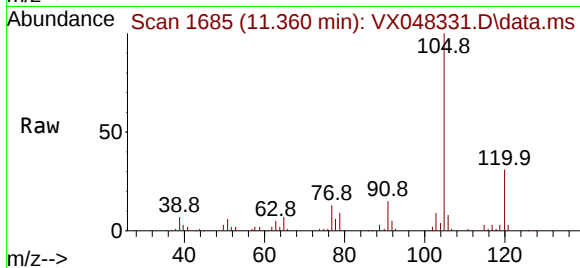

#80

1,3,5-Trimethylbenzene

Concen: 3.479 ug/l

RT: 11.433 min Scan# 1697

Delta R.T. -0.000 min

Lab File: VX048331.D




Acq: 23 Oct 2025 17:09


Tgt Ion: 105 Resp: 29275

Ion Ratio Lower Upper

105 100

120 48.4 24.0 72.0


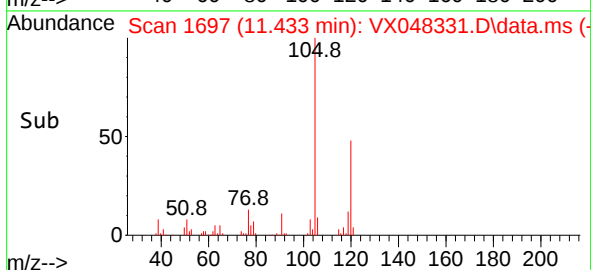

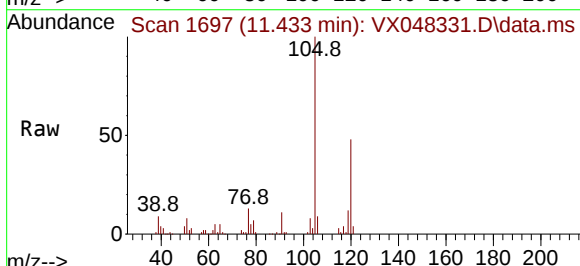




#81
trans-1,4-Dichloro-2-butene
Concen: 76.501 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.061 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 70989
Ion Ratio Lower Upper
75 100
53 0.0 79.5 119.3#
89 0.0 36.8 55.2#

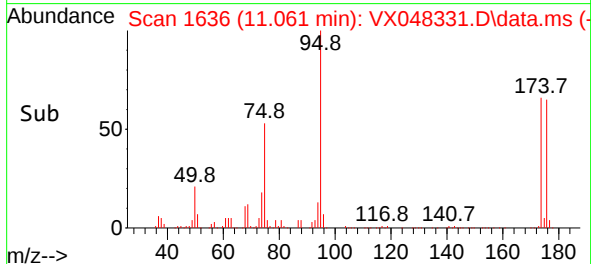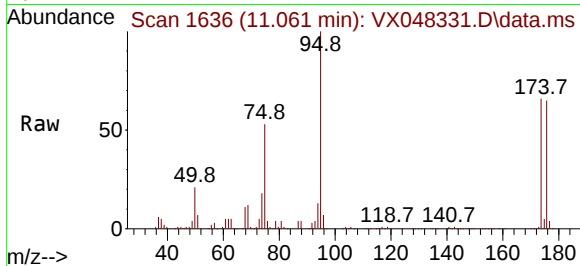

#82
4-Chlorotoluene
Concen: 0.427 ug/l
RT: 11.433 min Scan# 1697
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Tgt Ion: 91 Resp: 3622
Ion Ratio Lower Upper
91 100
126 0.0 14.1 42.4#


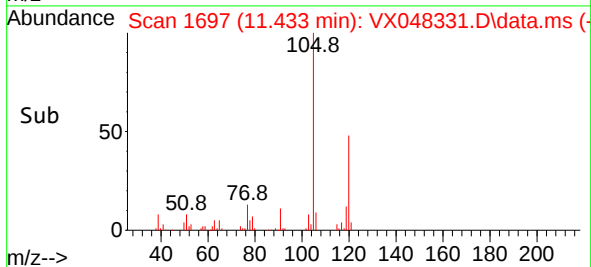

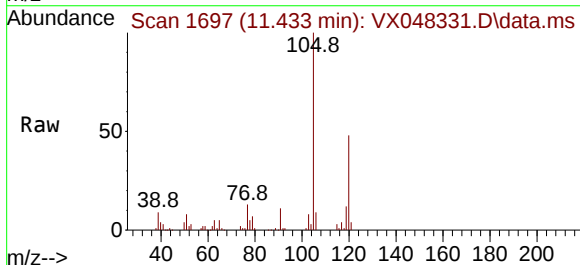




#84
1,2,4-Trimethylbenzene
Concen: 9.967 ug/l
RT: 11.732 min Scan# 1746
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 83706
Ion Ratio Lower Upper
105 100
120 42.1 22.1 66.5

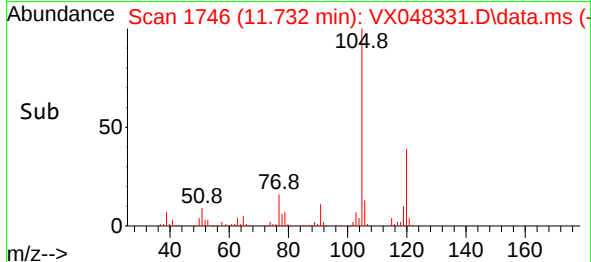

#85
sec-Butylbenzene
Concen: 8.047 ug/l
RT: 11.732 min Scan# 1746
Delta R.T. -0.140 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Tgt Ion:105 Resp: 83706
Ion Ratio Lower Upper
105 100
134 0.0 10.1 30.1#


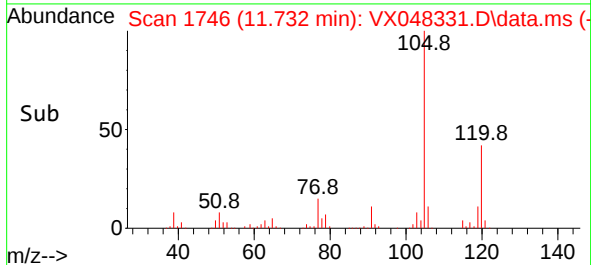

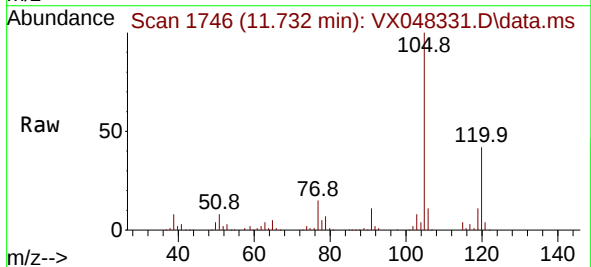




#90
Hexachloroethane
Concen: 0.413 ug/l
RT: 12.530 min Scan# 117
Delta R.T. 0.012 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:117 Resp: 734
Ion Ratio Lower Upper
117 100
201 0.0 34.1 102.2#

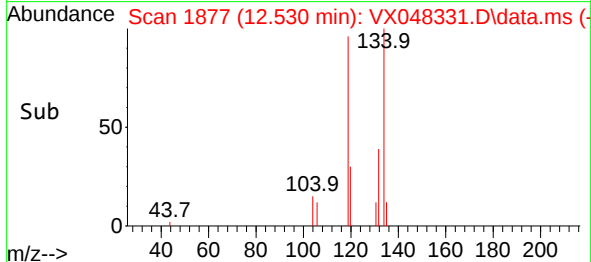

#95
Naphthalene
Concen: 53.105 ug/l
RT: 13.756 min Scan# 2078
Delta R.T. -0.000 min
Lab File: VX048331.D
Acq: 23 Oct 2025 17:09

Tgt Ion:128 Resp: 429379
Ion Ratio Lower Upper
128 100
127 12.9 10.2 15.4
129 10.9 8.6 12.8

