


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX102418\  
 Data File : VX005531.D  
 Acq On : 24 Oct 2018 09:57  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X102418W.M  
 Title : SW846 8260  
 Last Update : Thu Oct 25 02:52:45 2018

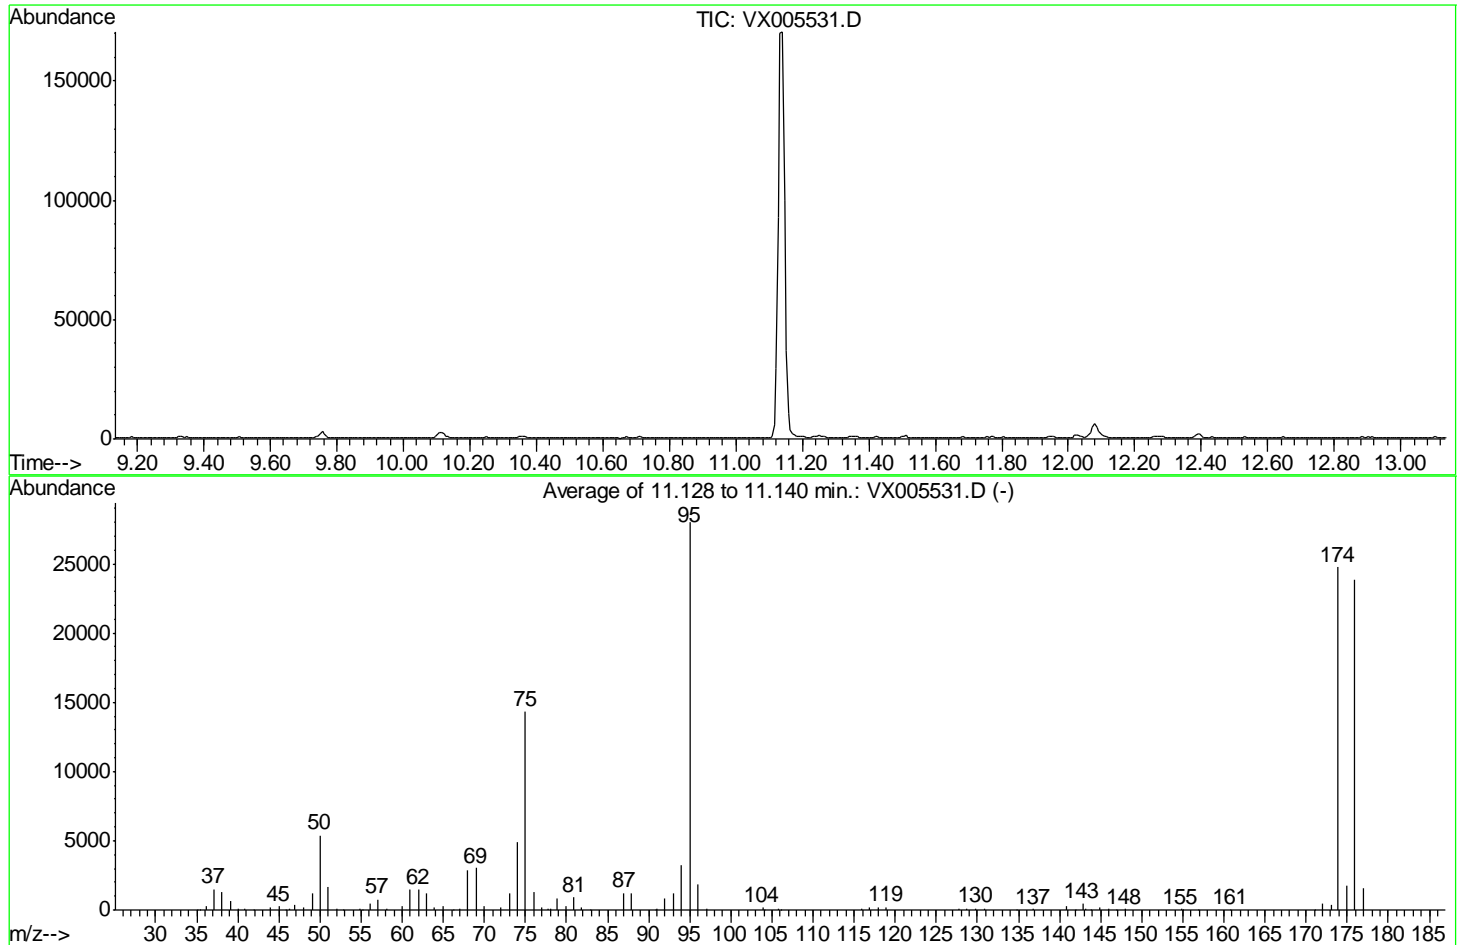

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	5374	PASS
75	95	30	60	51.1	14290	PASS
95	95	100	100	100.0	27992	PASS
96	95	5	9	6.7	1880	PASS
173	174	0.00	2	1.5	379	PASS
174	95	50	100	88.4	24745	PASS
175	174	5	9	7.3	1802	PASS
176	174	95	101	96.4	23864	PASS
177	176	5	9	6.8	1616	PASS