


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX102418\
Data File : VX005556.D
Acq On : 24 Oct 2018 22:18
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102418W.M
Title : SW846 8260
Last Update : Thu Oct 25 02:52:45 2018

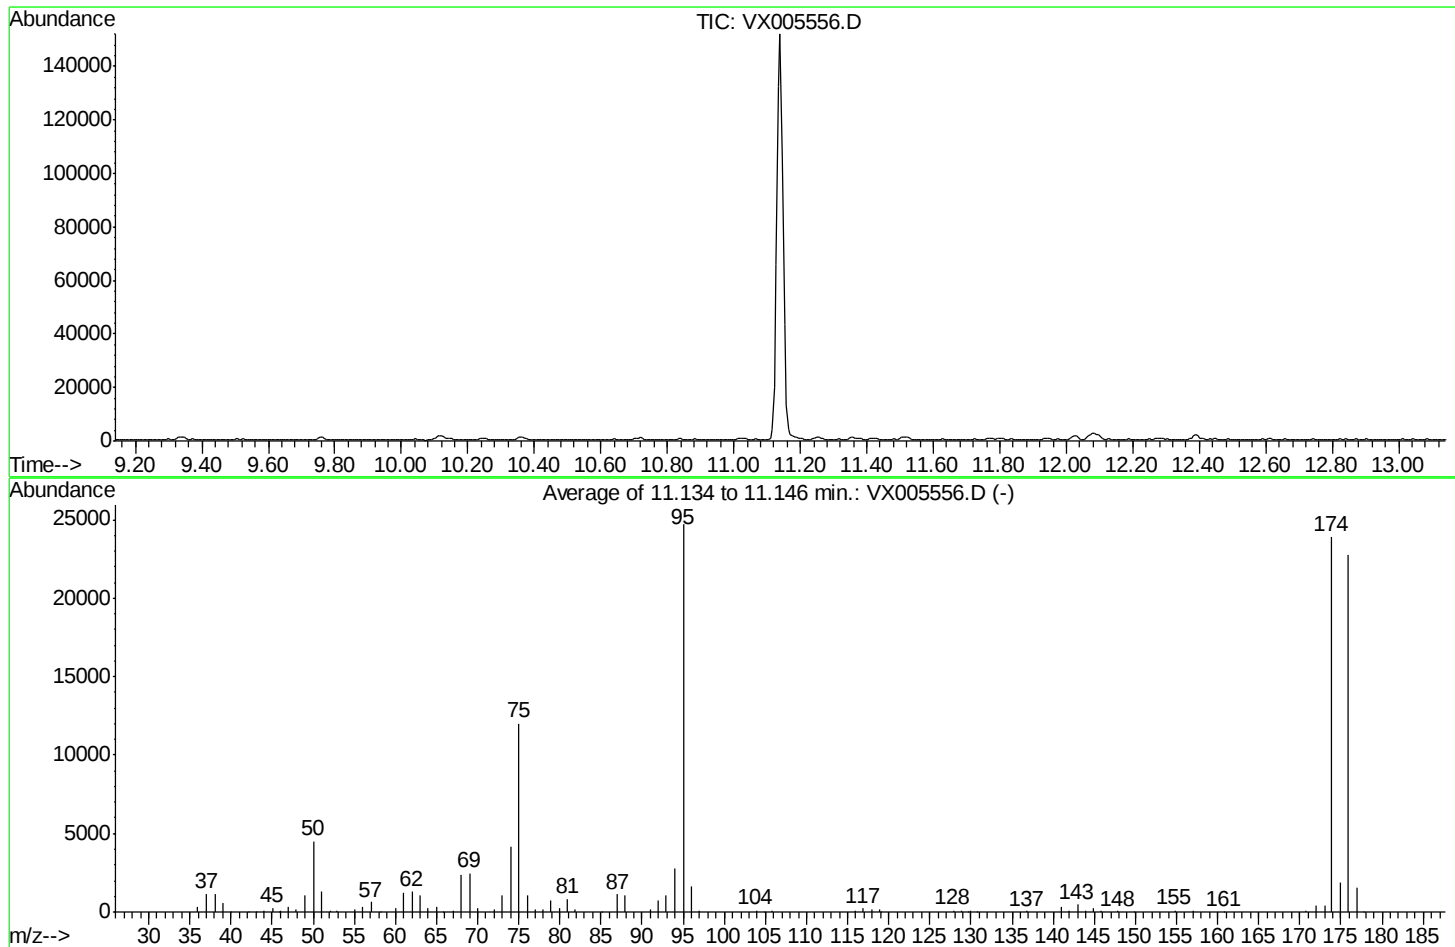

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	4513	PASS
75	95	30	60	48.7	12019	PASS
95	95	100	100	100.0	24701	PASS
96	95	5	9	6.5	1616	PASS
173	174	0.00	2	1.6	385	PASS
174	95	50	100	96.8	23917	PASS
175	174	5	9	8.0	1903	PASS
176	174	95	101	95.0	22730	PASS
177	176	5	9	6.7	1519	PASS