




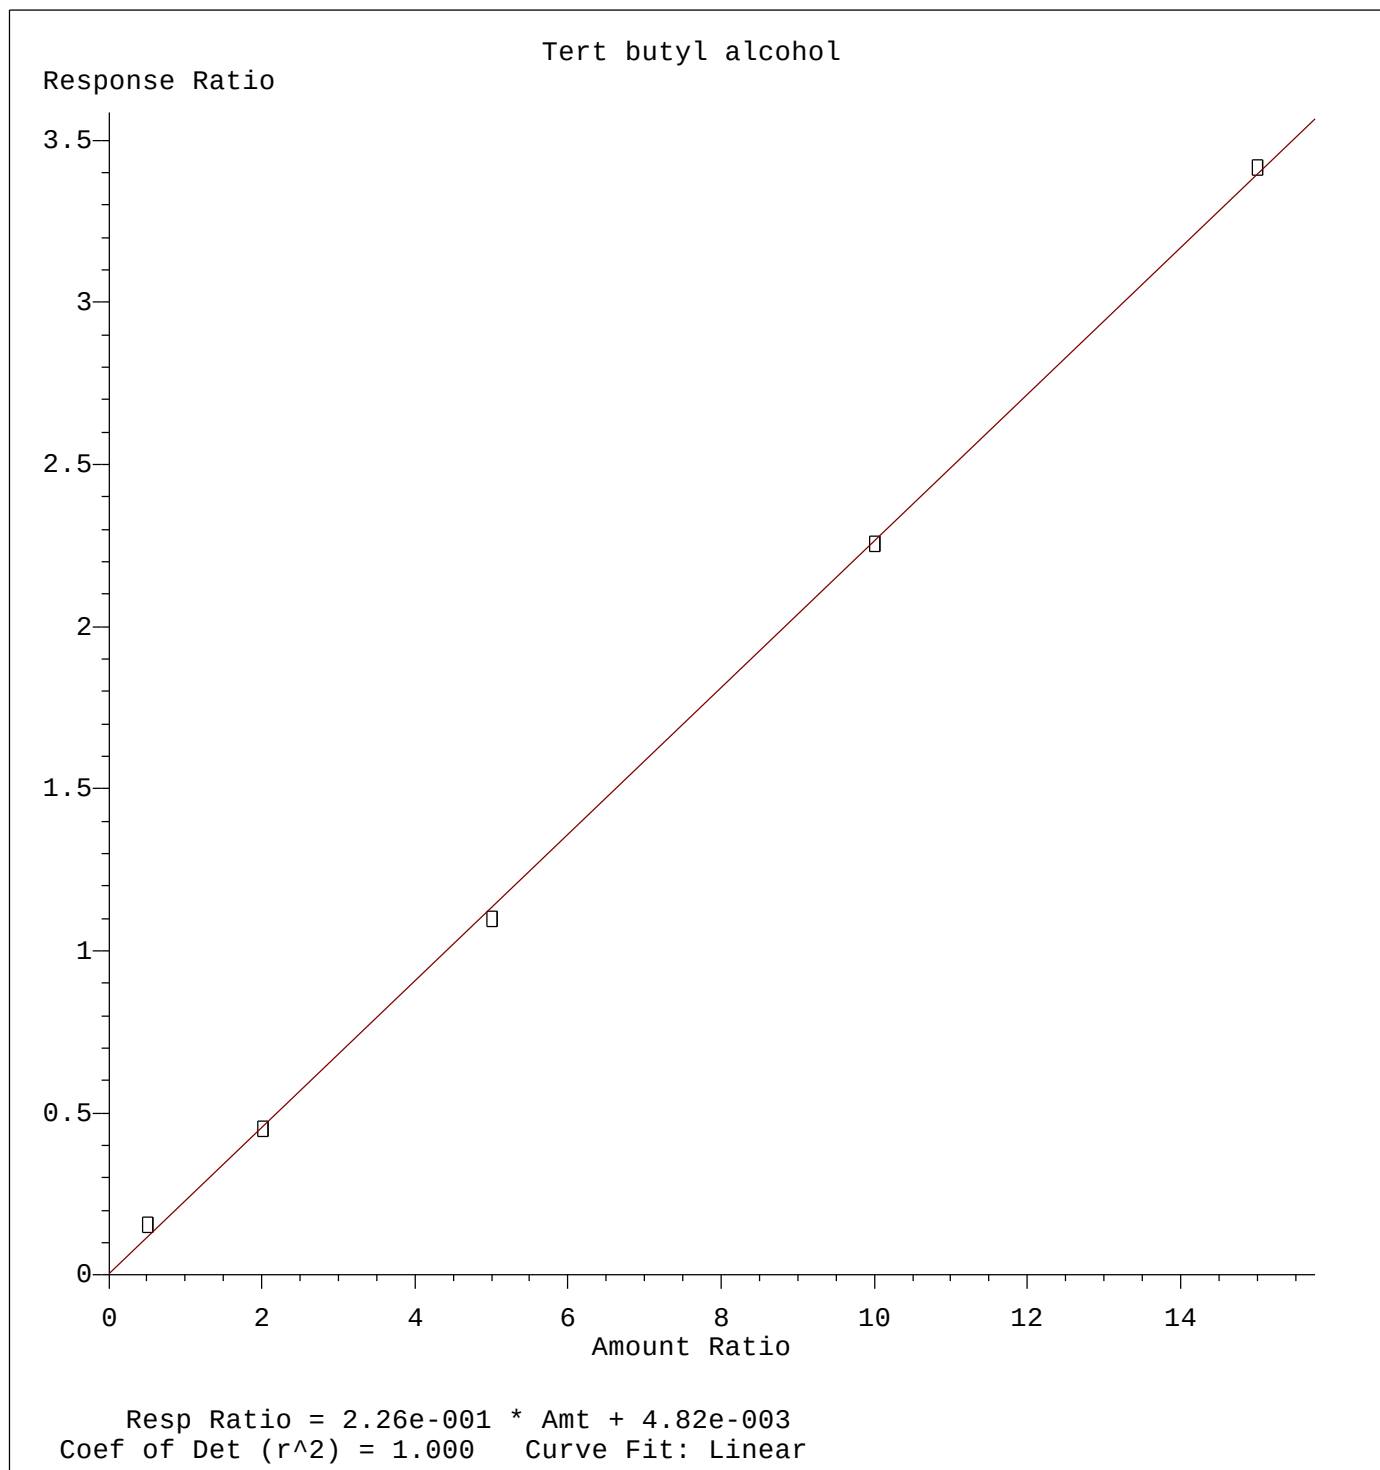

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Calibration Table Last Updated: Thu Oct 24 03:56:38 2019

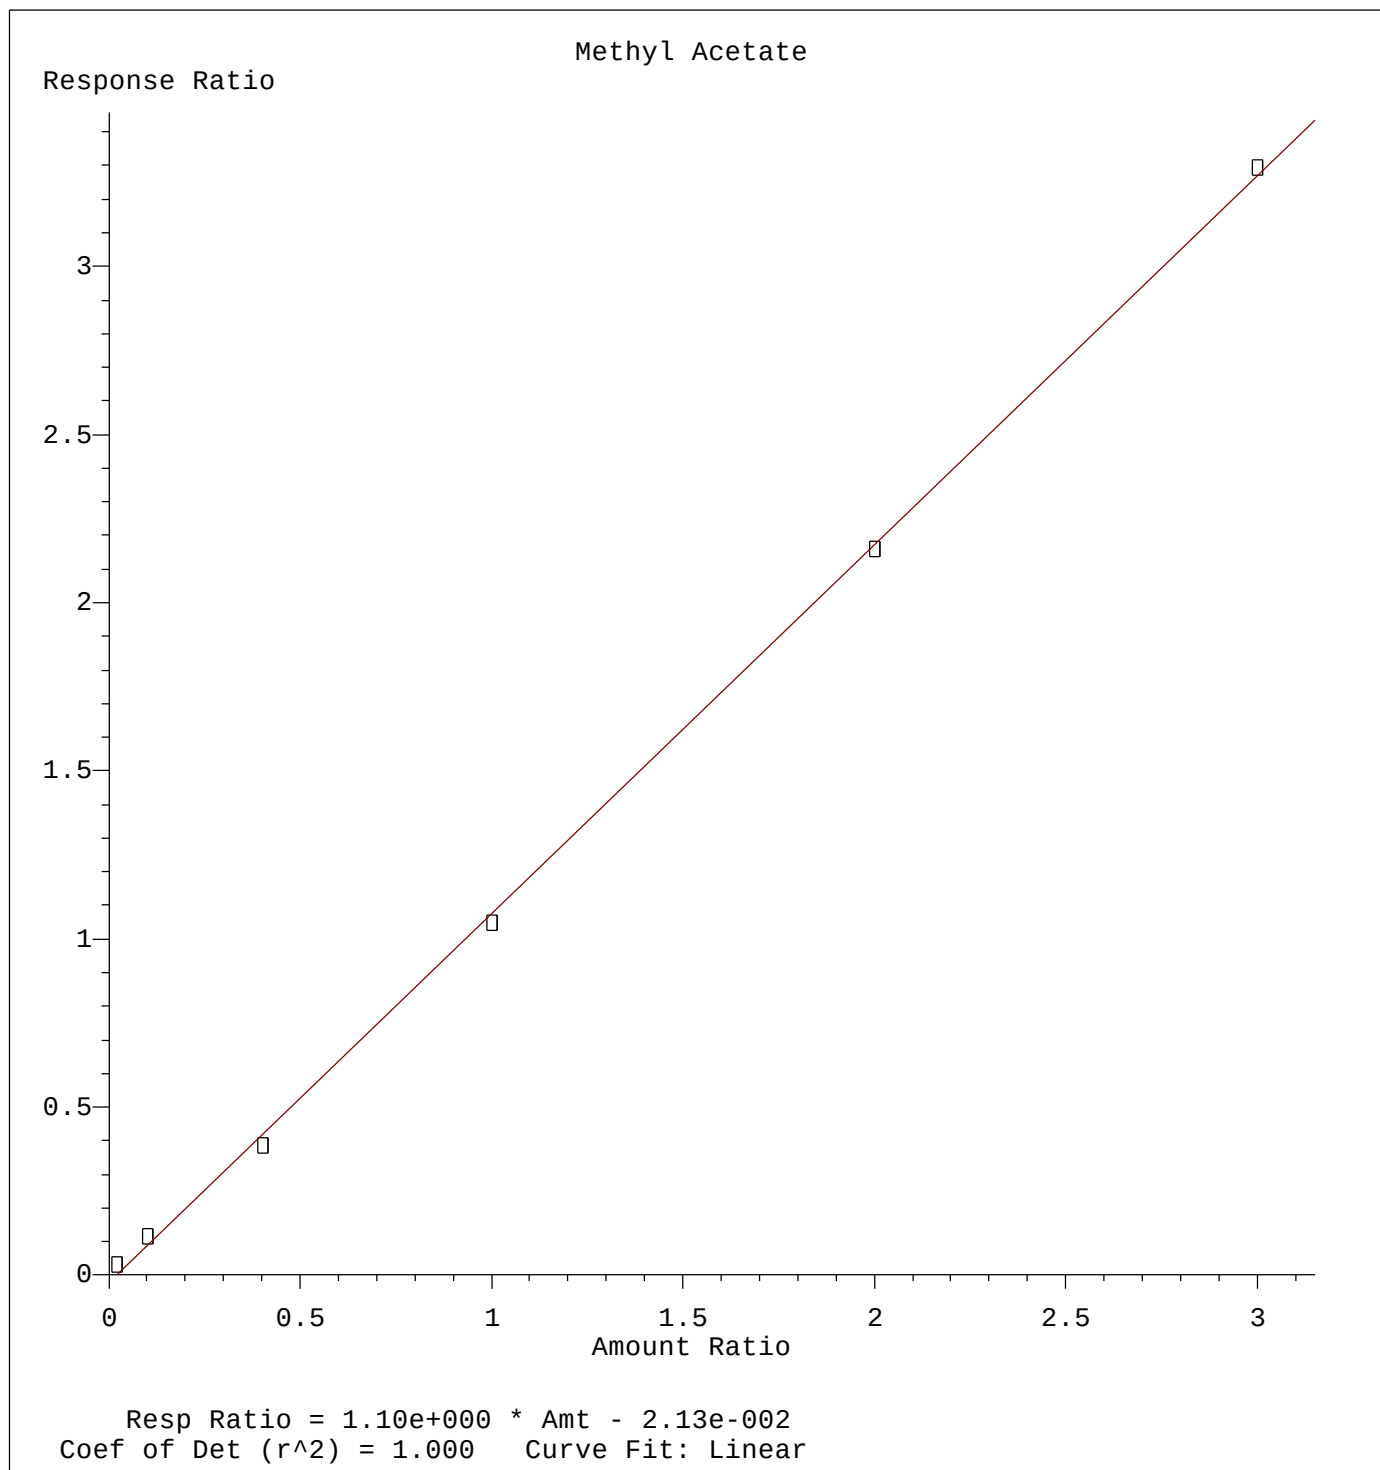


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Calibration Table Last Updated: Thu Oct 24 03:56:38 2019

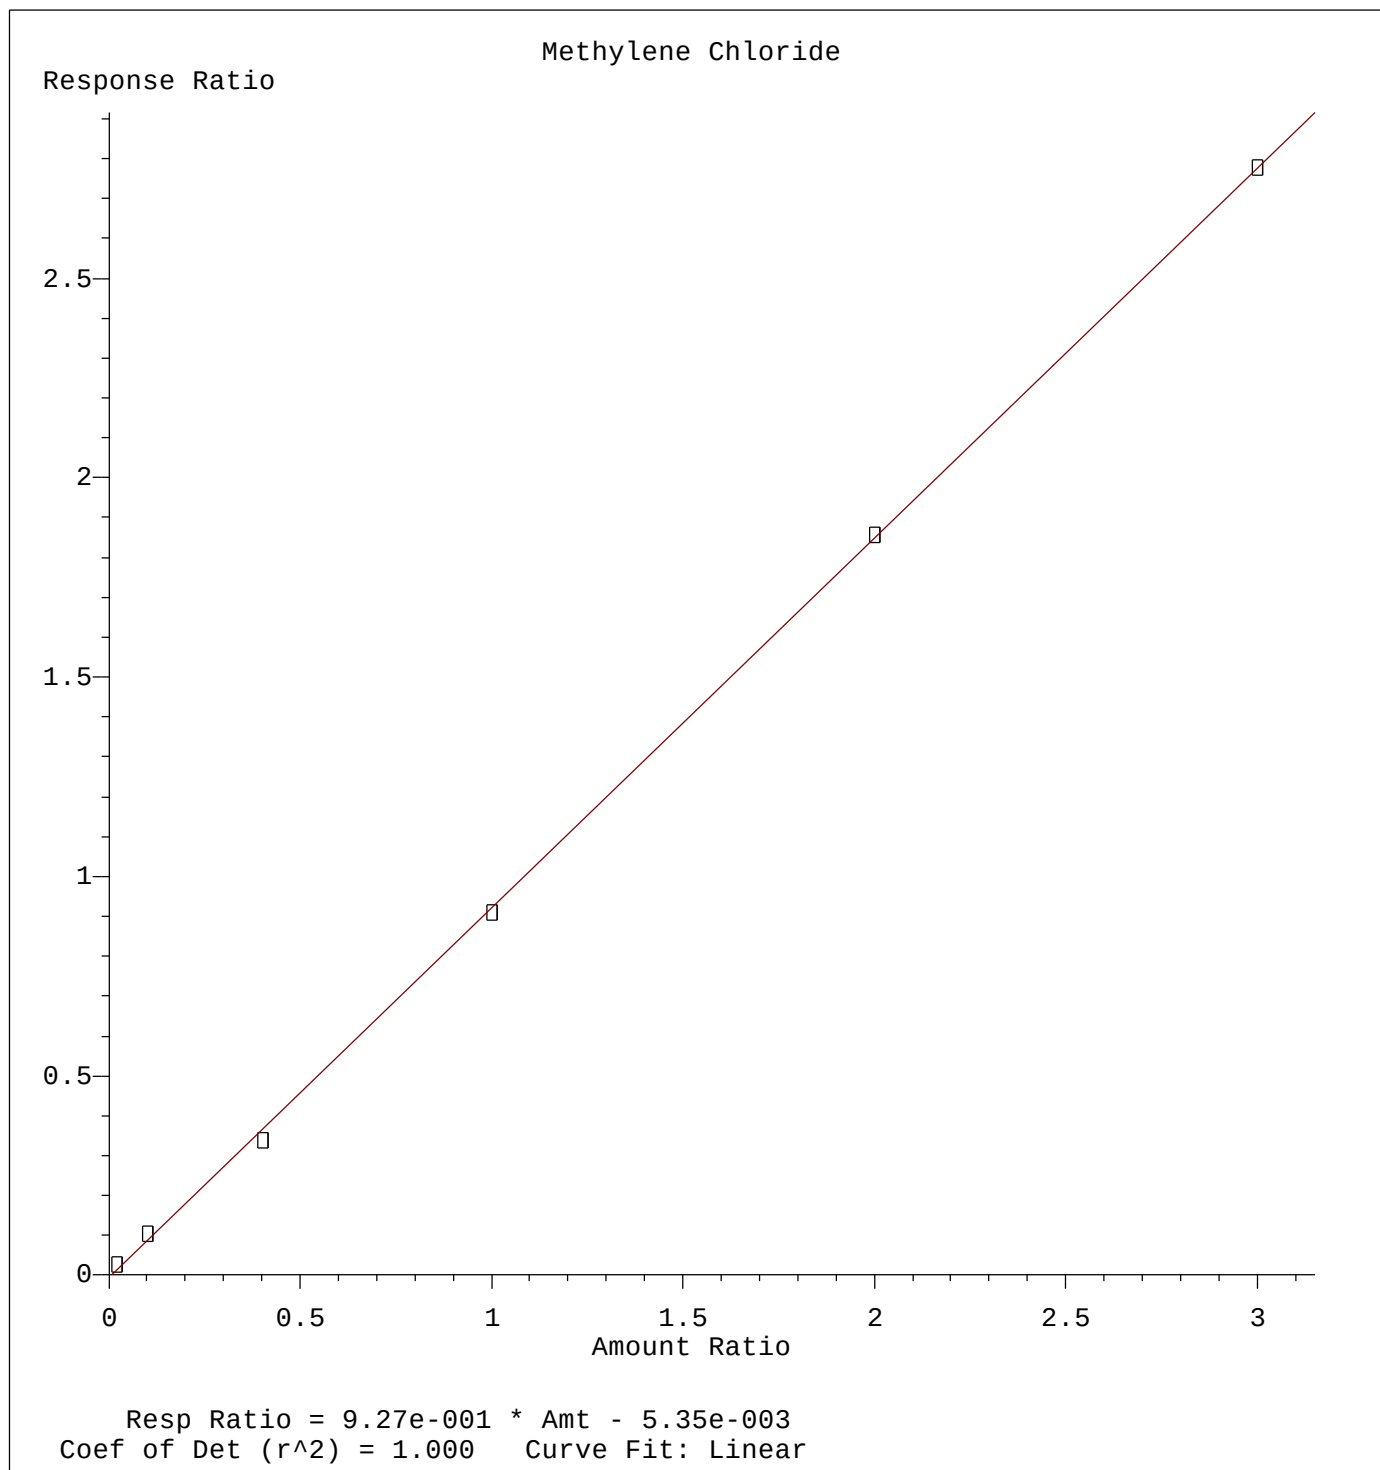

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Calibration Table Last Updated: Thu Oct 24 03:56:38 2019


trans-1,2-Dichloroethene

Response Ratio

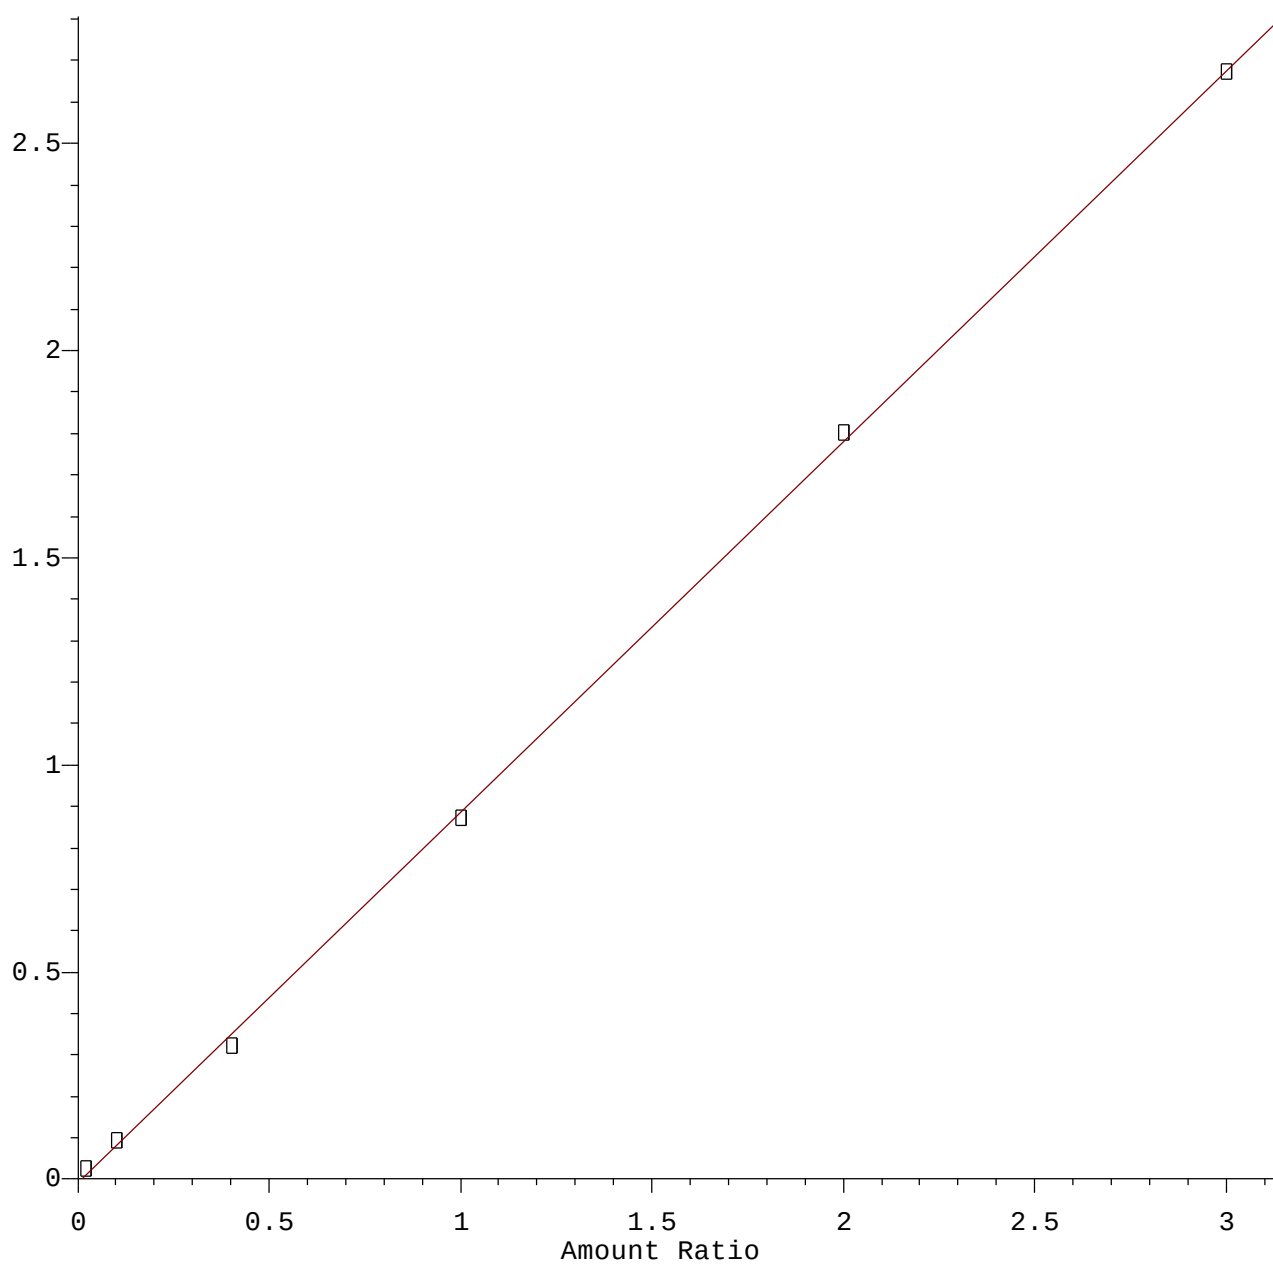

Resp Ratio = 8.95e-001 * Amt - 8.52e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Calibration Table Last Updated: Thu Oct 24 03:56:38 2019

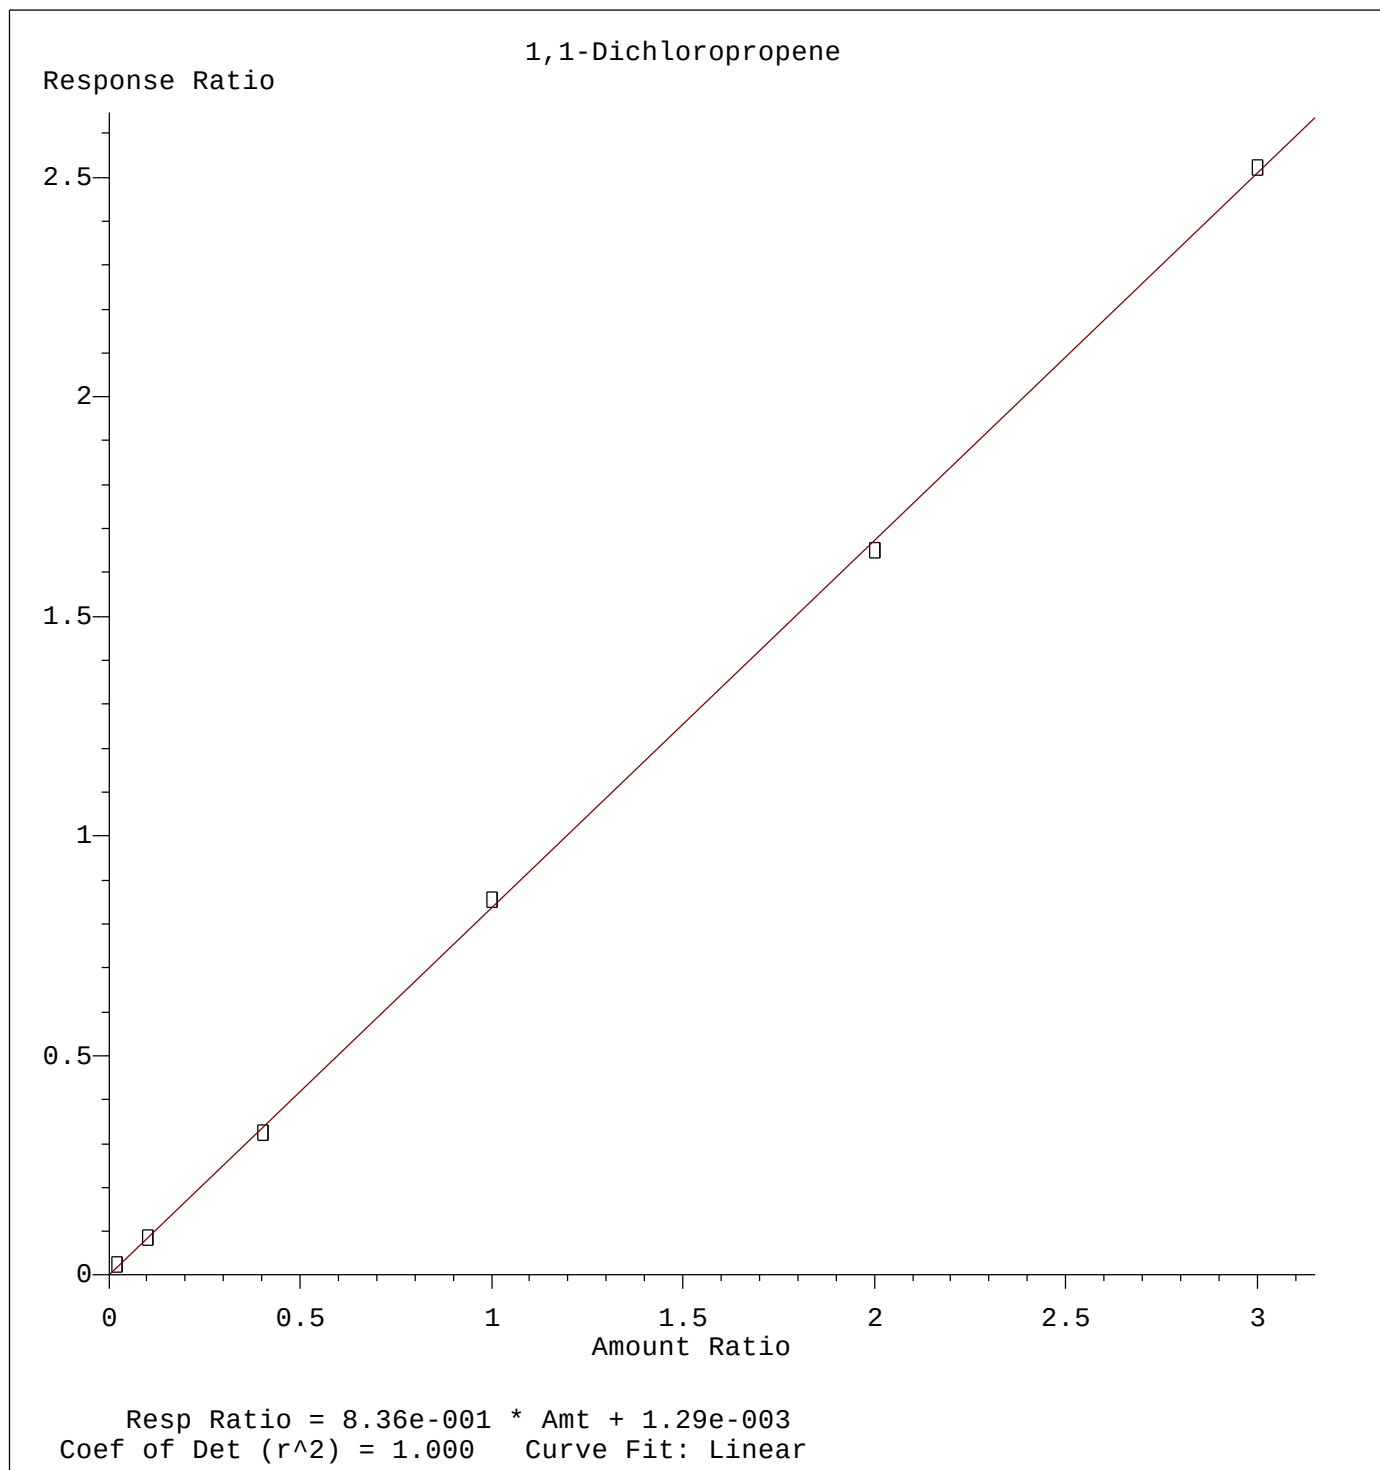

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Calibration Table Last Updated: Thu Oct 24 03:56:38 2019


Tetrachloroethene

Response Ratio

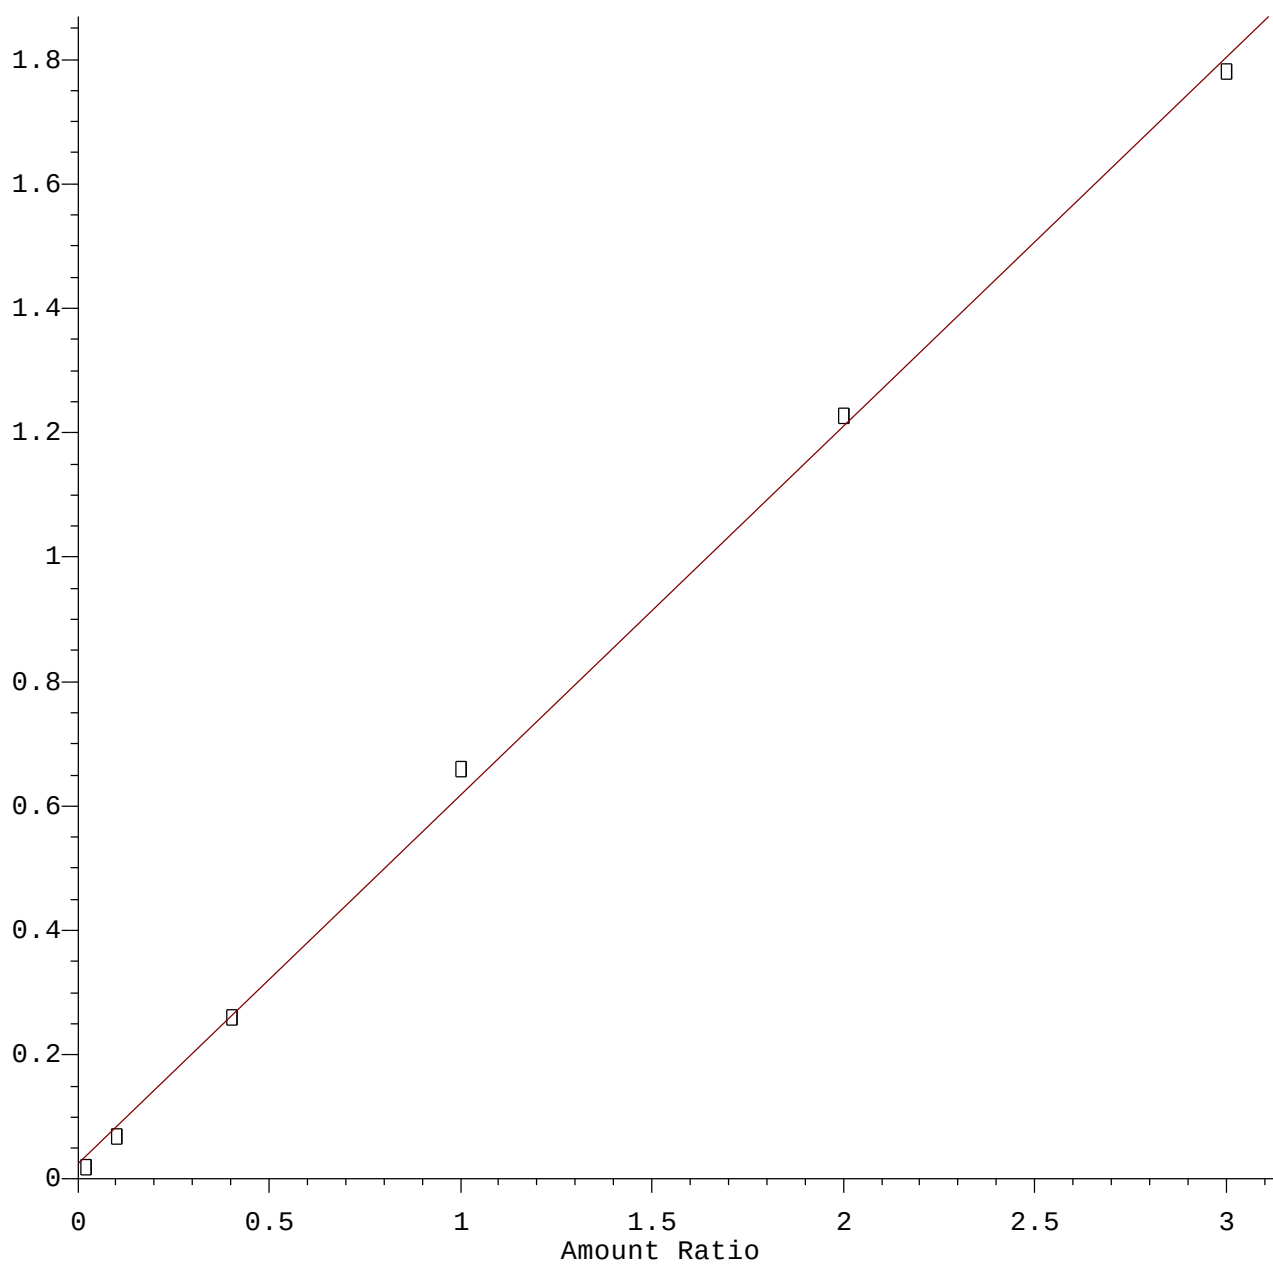


Resp Ratio = $5.93 \times 10^{-1} \times \text{Amt} + 2.38 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Calibration Table Last Updated: Thu Oct 24 03:56:38 2019

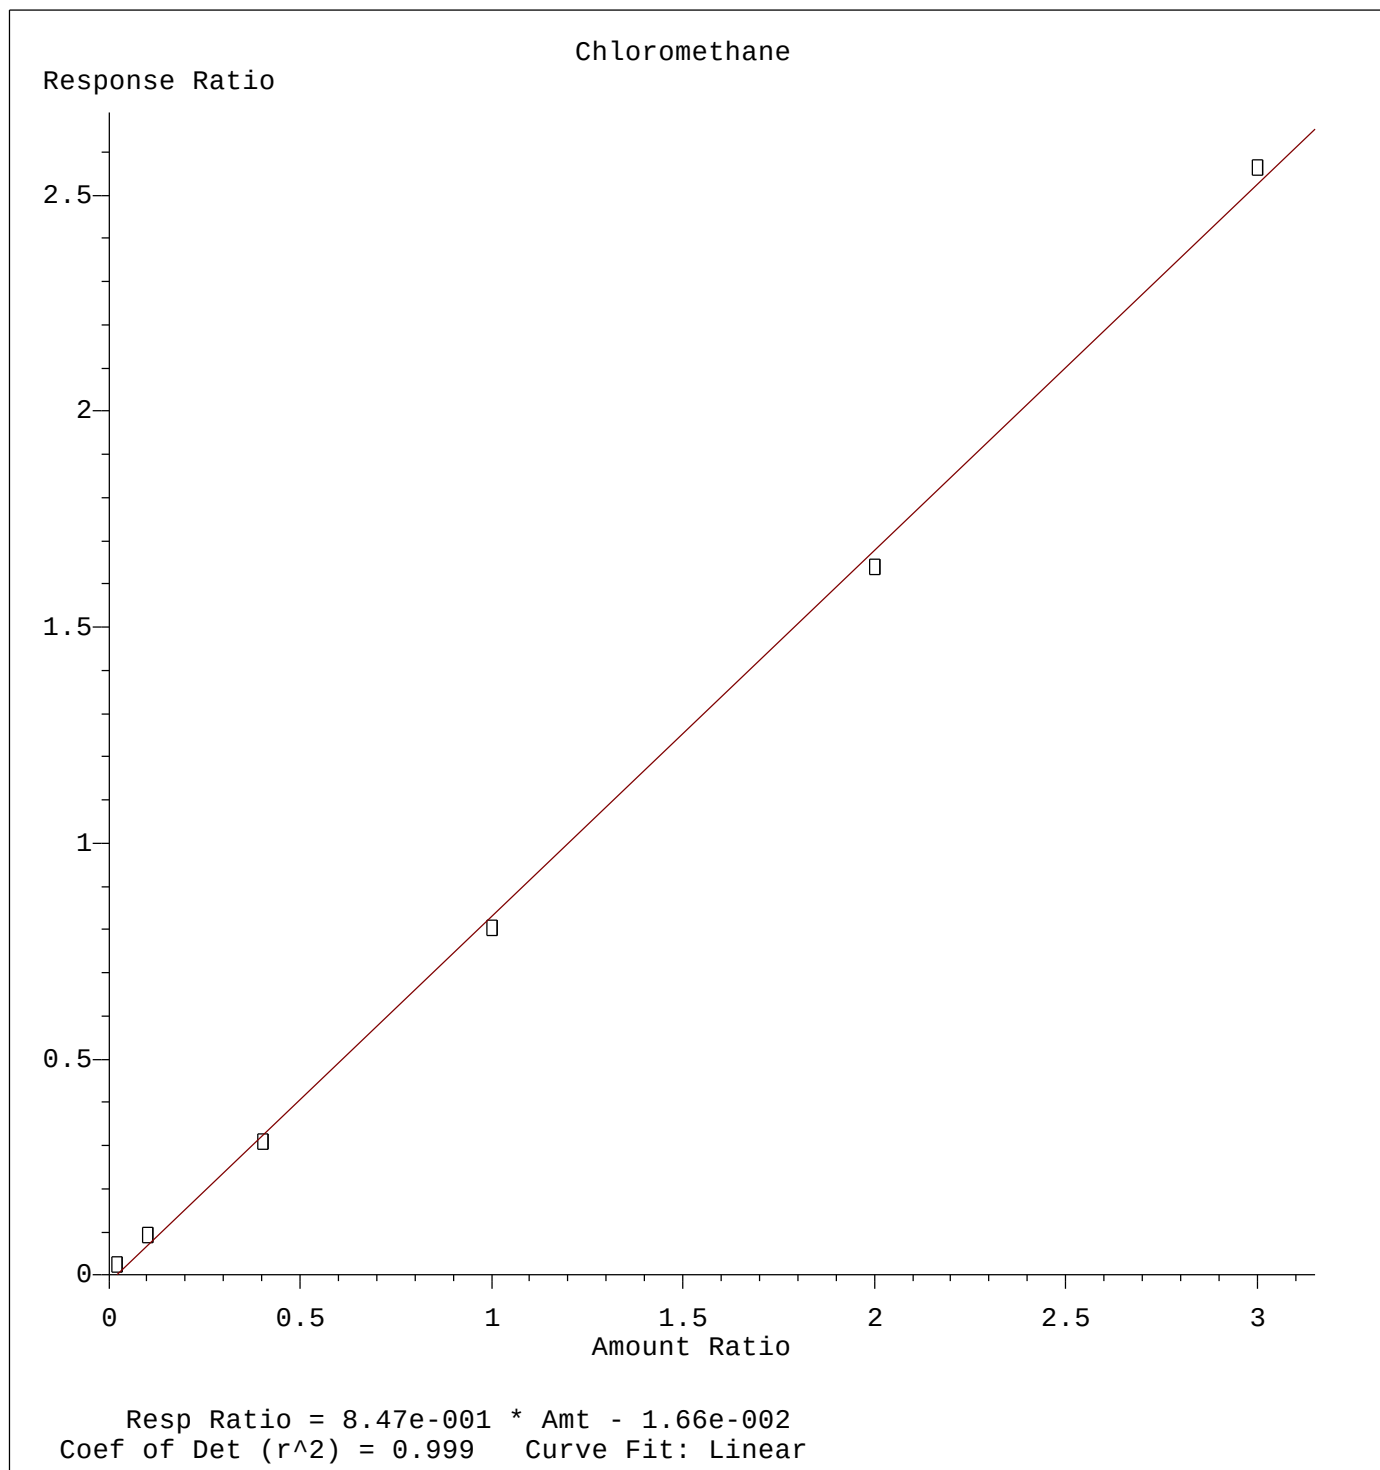


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Calibration Table Last Updated: Thu Oct 24 03:56:38 2019

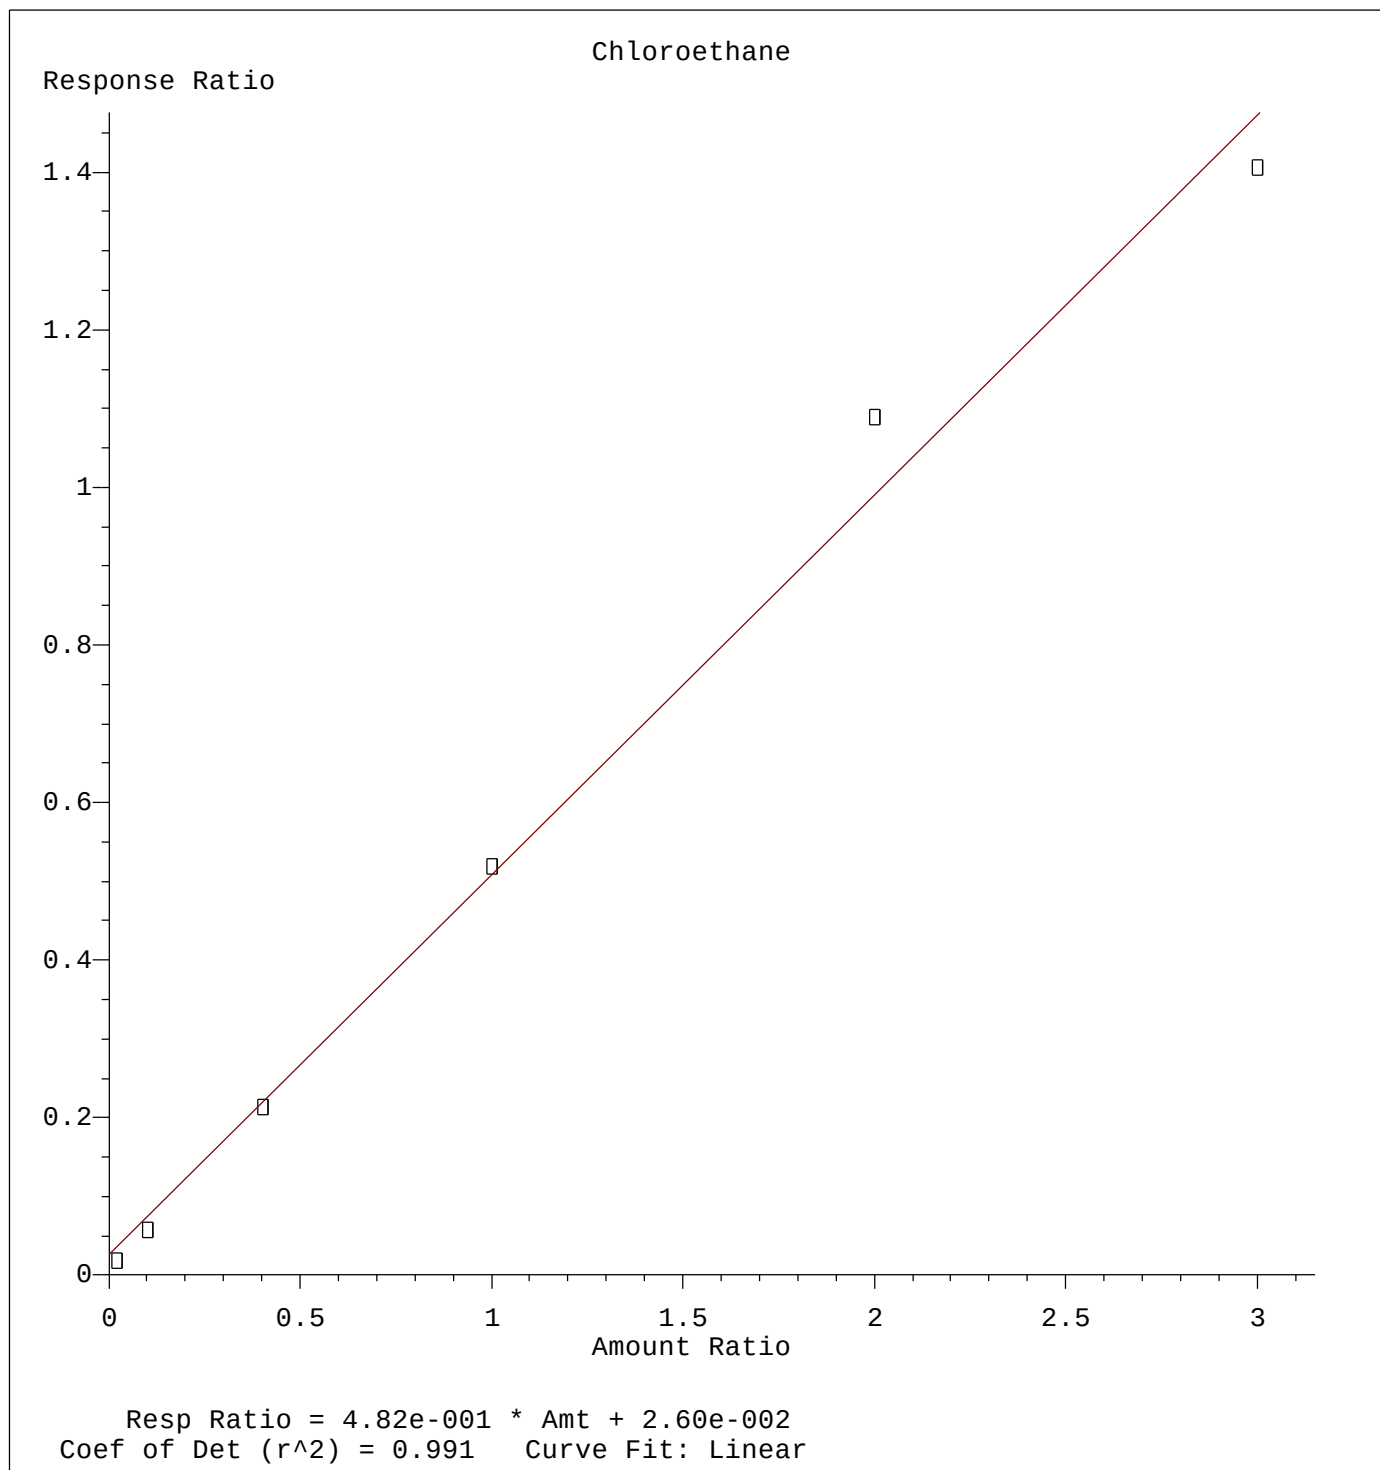

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Calibration Table Last Updated: Thu Oct 24 03:56:38 2019


Trichlorofluoromethane

Response Ratio

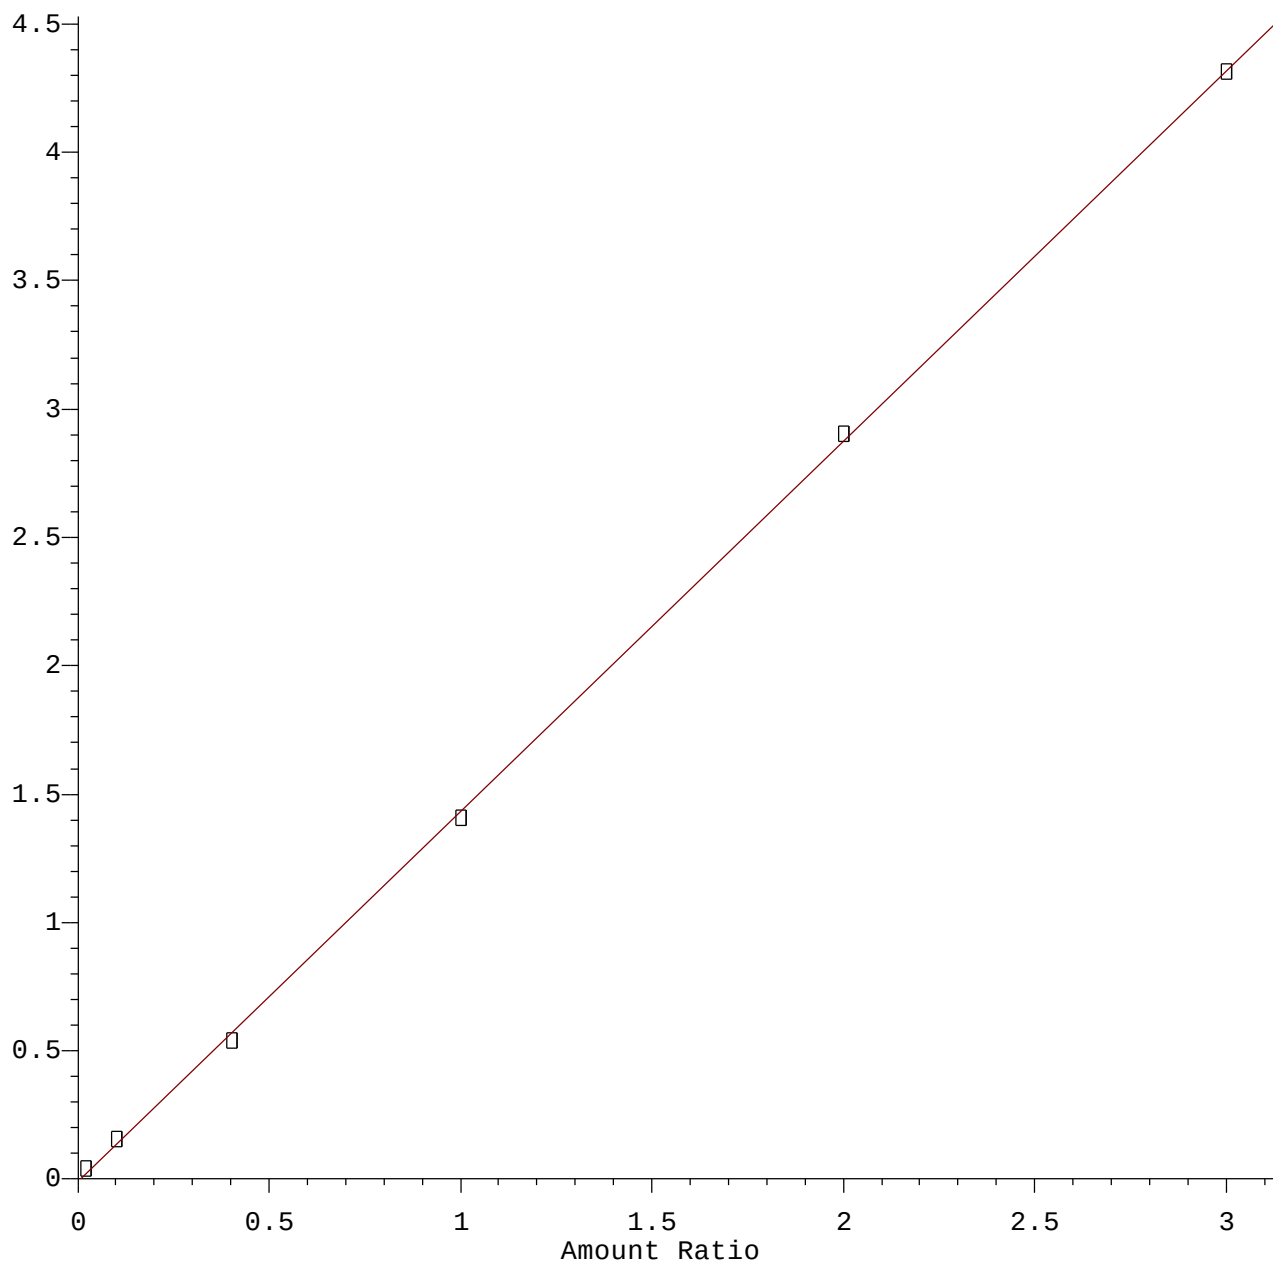

Resp Ratio = 1.44e+000 * Amt - 8.61e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Calibration Table Last Updated: Thu Oct 24 03:56:38 2019

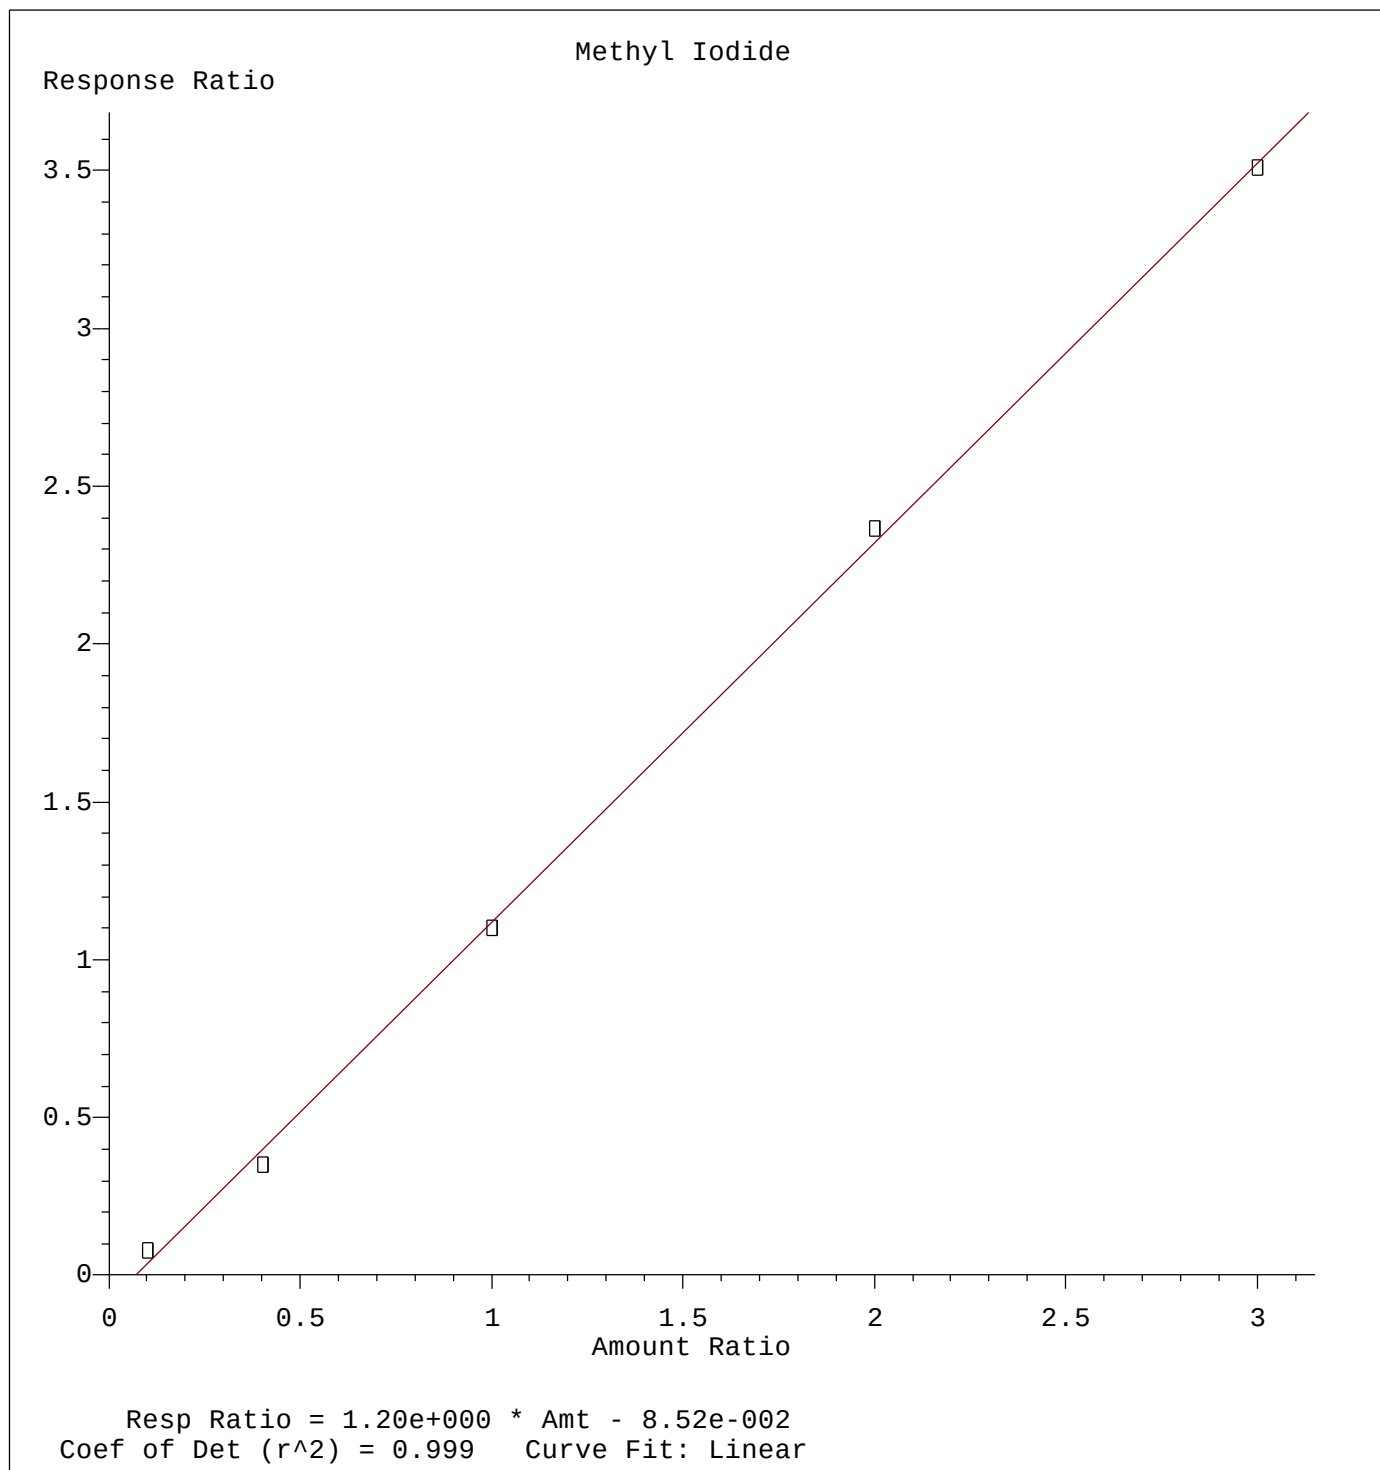

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Calibration Table Last Updated: Thu Oct 24 03:56:38 2019