


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX102419\
 Data File : VX013182.D
 Acq On : 23 Oct 2019 08:34
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
 Title : SW846 8260
 Last Update : Thu Oct 24 03:56:38 2019

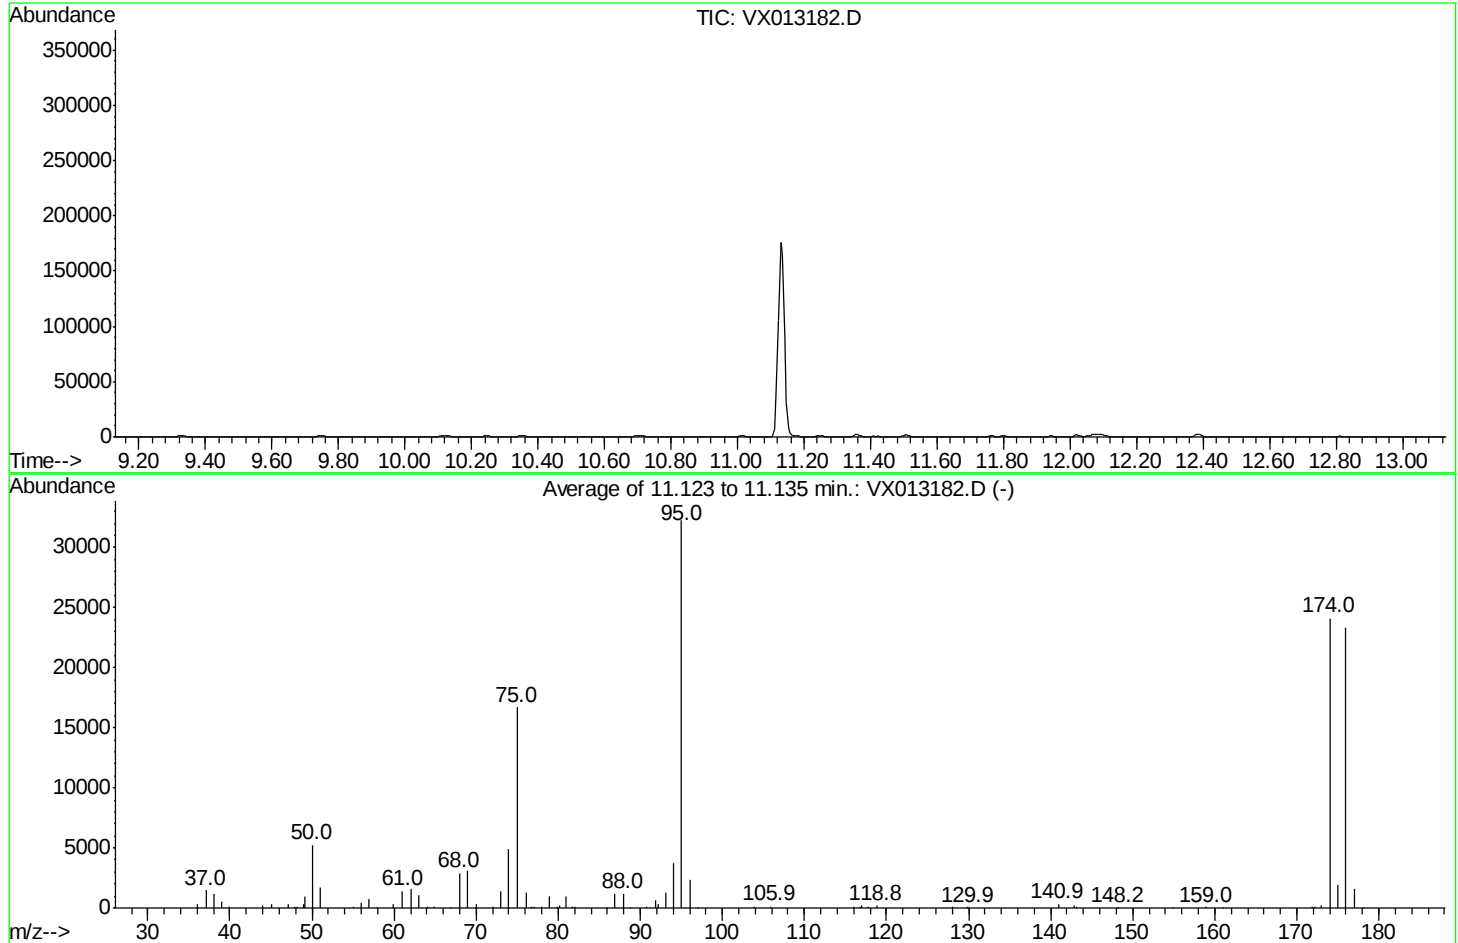

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	5272	PASS
75	95	30	60	51.8	16717	PASS
95	95	100	100	100.0	32269	PASS
96	95	5	9	7.1	2298	PASS
173	174	0.00	2	0.8	187	PASS
174	95	50	100	74.7	24091	PASS
175	174	5	9	8.1	1959	PASS
176	174	95	101	96.7	23292	PASS
177	176	5	9	6.9	1600	PASS