

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102422\
 Data File : VX032348.D
 Acq On : 24 Oct 2022 18:17
 Operator : JC/MD
 Sample : N5260-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB-2022-10-21

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
 Title : SW846 8260

Signal : TIC: VX032348.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	50	rVB	6361	6934	1.07%	0.191%
2	1.752	103	109	117	rBV	13379	19221	2.97%	0.531%
3	1.953	138	142	152	rVB3	5630	8958	1.38%	0.247%
4	4.300	520	527	537	rVB4	2435	6774	1.05%	0.187%
5	5.092	648	657	671	rVB2	7414	22698	3.50%	0.627%
6	5.391	694	706	719	rBV2	77288	227413	35.10%	6.277%
7	5.556	720	733	753	rVB	140948	401470	61.97%	11.081%
8	5.958	788	799	815	rBV2	86068	225066	34.74%	6.212%
9	6.763	920	931	945	rBV	208757	488330	75.38%	13.479%
10	8.653	1230	1241	1249	rBV	410332	647841	100.00%	17.881%
11	10.055	1465	1471	1485	rVB	422660	556073	85.83%	15.348%
12	10.195	1490	1494	1500	rVB	9912	12988	2.00%	0.358%
13	10.305	1505	1512	1519	rBV	12489	16729	2.58%	0.462%
14	11.079	1634	1639	1652	rBV	334132	436492	67.38%	12.048%
15	11.402	1685	1692	1697	rBV	5221	7339	1.13%	0.203%
16	11.750	1745	1749	1755	rBV	12294	16314	2.52%	0.450%
17	12.024	1788	1794	1801	rBV	420392	522341	80.63%	14.417%




Sum of corrected areas: 3622981

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102422\
Data File : VX032348.D
Acq On : 24 Oct 2022 18:17
Operator : JC/MD
Sample : N5260-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2022-10-21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

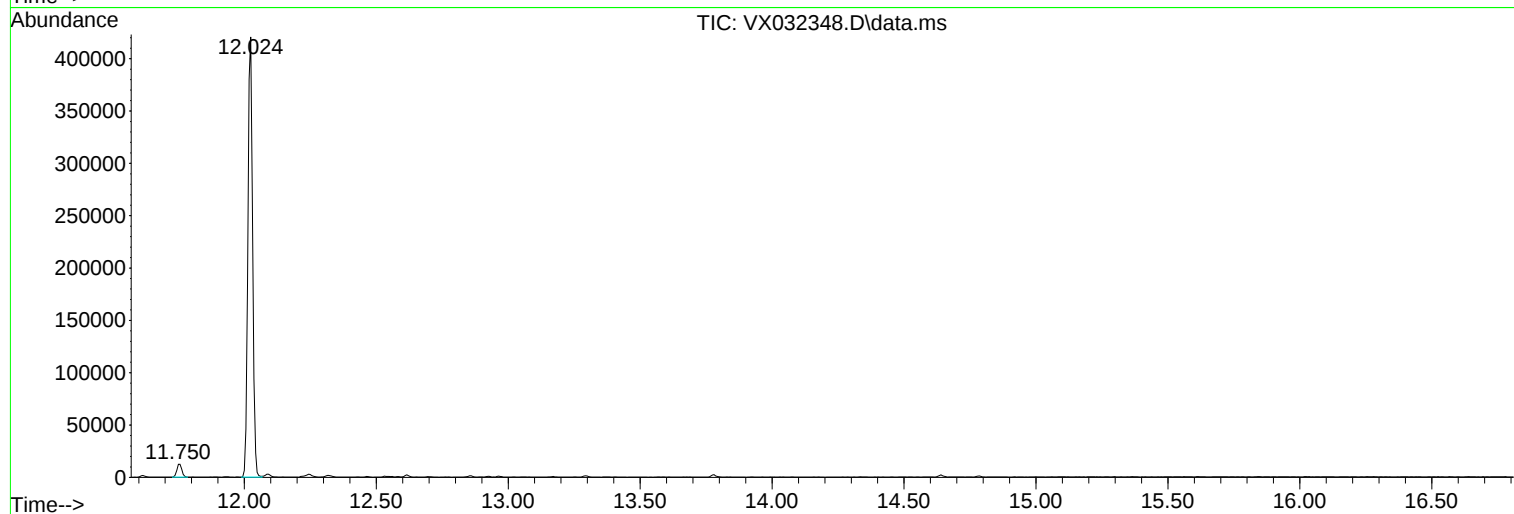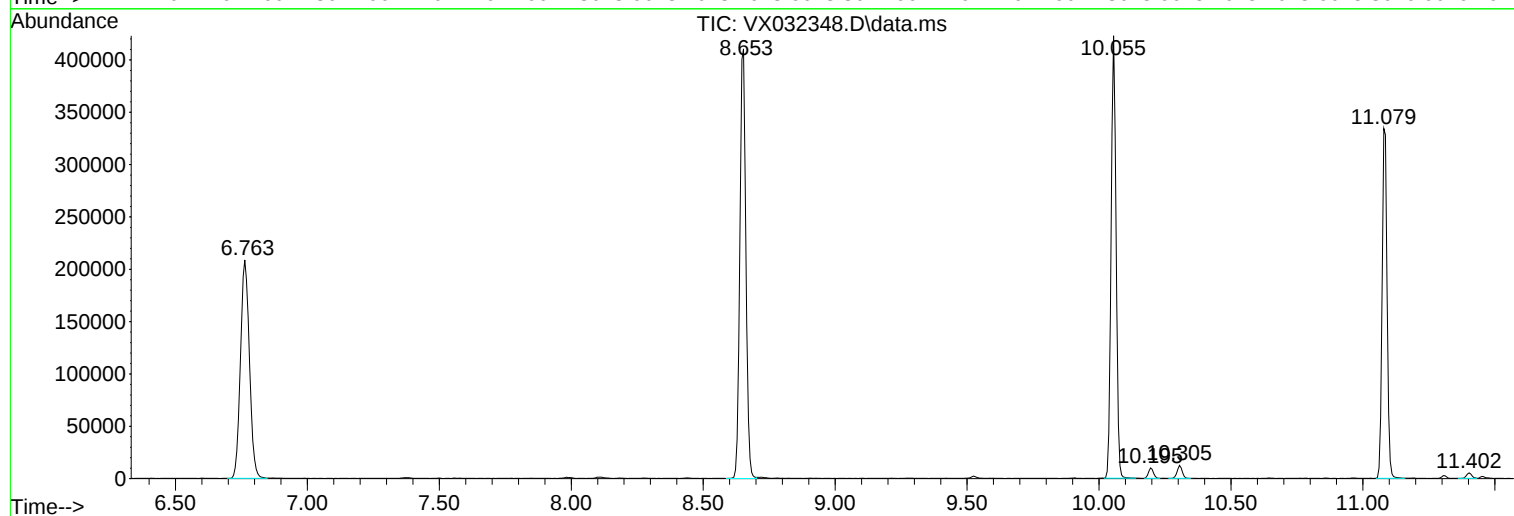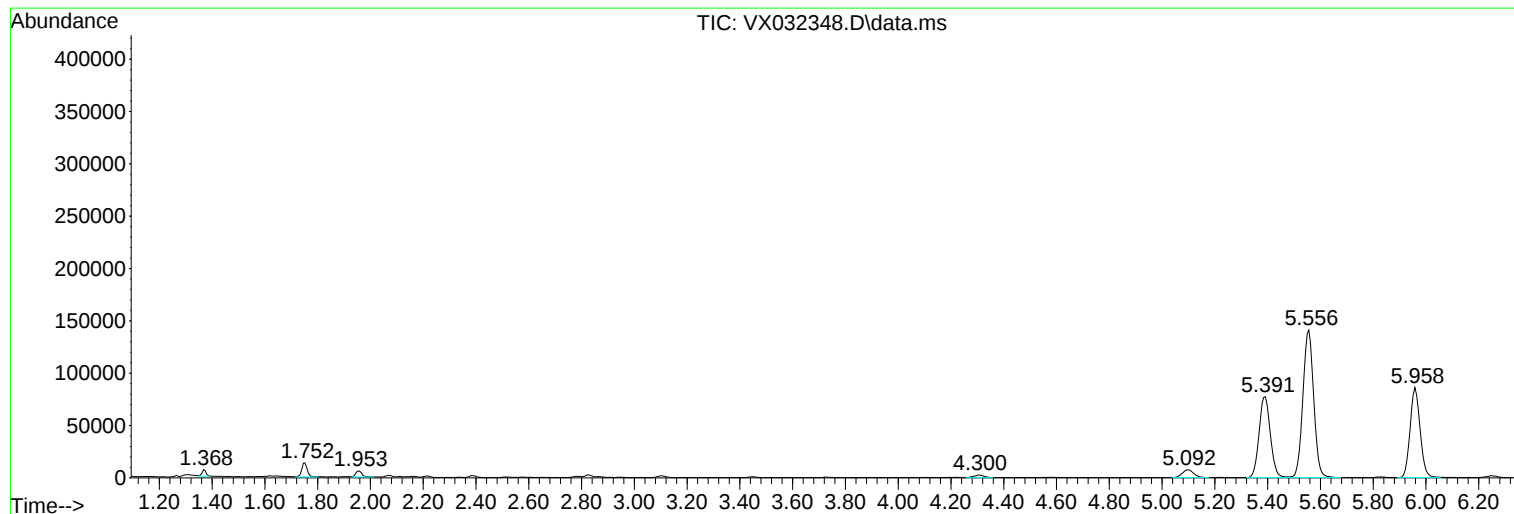

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102422\
Data File : VX032348.D
Acq On : 24 Oct 2022 18:17
Operator : JC/MD
Sample : N5260-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2022-10-21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102422\
Data File : VX032348.D
Acq On : 24 Oct 2022 18:17
Operator : JC/MD
Sample : N5260-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2022-10-21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------