

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102423\
 Data File : VX038456.D
 Acq On : 24 Oct 2023 15:31
 Operator : JC/MD
 Sample : 04975-01
 Misc : 1.12g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Oct 25 06:09:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 05 15:27:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	157814	50.000	ug/l	#-0.01
34) 1,4-Difluorobenzene	6.757	114	270856	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	269308	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	156222	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	99062	39.026	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	78.060%
35) Dibromofluoromethane	5.385	113	83123	42.590	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	85.180%
50) Toluene-d8	8.647	98	328823	44.091	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	88.180%#
62) 4-Bromofluorobenzene	11.085	95	132057	46.707	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.420%
Target Compounds						
					Qvalue	
5) Bromomethane	1.599	94	594	Below Cal		92
6) Chloroethane	1.679	64	148	Below Cal		96
10) Methyl Iodide	2.428	142	1314	0.615 ug/l	#	82
11) Tert butyl alcohol	2.947	59	1585	Below Cal	#	82
20) Methylene Chloride	2.776	84	1005	0.504 ug/l		94
31) Cyclohexane	5.489	56	4419	1.607 ug/l	#	44
36) 1,1-Dichloropropene	5.544	75	11531	4.284 ug/l	#	51
38) Carbon Tetrachloride	5.550	117	15935	6.019 ug/l	#	15
39) Methylcyclohexane	7.373	83	3281	1.041 ug/l	#	91
43) Isopropyl Acetate	6.355	43	1001	0.210 ug/l	#	62
51) 4-Methyl-2-Pentanone	8.653	43	1438	0.437 ug/l	#	1
52) Toluene	8.720	92	202674	41.333 ug/l		94
53) t-1,3-Dichloropropene	8.714	75	2488	0.862 ug/l	#	1
55) 1,1,2-Trichloroethane	9.104	97	535	0.255 ug/l	#	26
67) Ethyl Benzene	10.201	91	3083	0.306 ug/l	#	88
68) m/p-Xylenes	10.305	106	3895	1.001 ug/l		93
69) o-Xylene	10.647	106	1768	0.466 ug/l		93
76) 1,2,3-Trichloropropane	11.085	75	69181	19.479 ug/l	#	39
78) n-propylbenzene	11.305	91	5380	0.420 ug/l		99
79) 2-Chlorotoluene	11.378	91	2690	0.354 ug/l	#	43
80) 1,3,5-Trimethylbenzene	11.457	105	4946	0.547 ug/l		92
81) trans-1,4-Dichloro-2-b...	11.085	75	69181	56.324 ug/l	#	5
84) 1,2,4-Trimethylbenzene	11.756	105	18455	2.048 ug/l		97
85) sec-Butylbenzene	11.890	105	2806	0.245 ug/l		92
86) p-Isopropyltoluene	11.976	119	2886	0.306 ug/l		99
89) n-Butylbenzene	12.335	91	8065	0.858 ug/l	#	53
90) Hexachloroethane	12.530	117	574	0.367 ug/l	#	17
93) 1,2,4-Trichlorobenzene	13.591	180	1953	0.590 ug/l	#	78
95) Naphthalene	13.774	128	5216	0.452 ug/l	#	87
96) 1,2,3-Trichlorobenzene	13.963	180	732	0.228 ug/l	#	7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102423\
Data File : VX038456.D
Acq On : 24 Oct 2023 15:31
Operator : JC/MD
Sample : 04975-01
Misc : 1.12g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Oct 25 06:09:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 05 15:27:13 2023
Response via : Initial Calibration

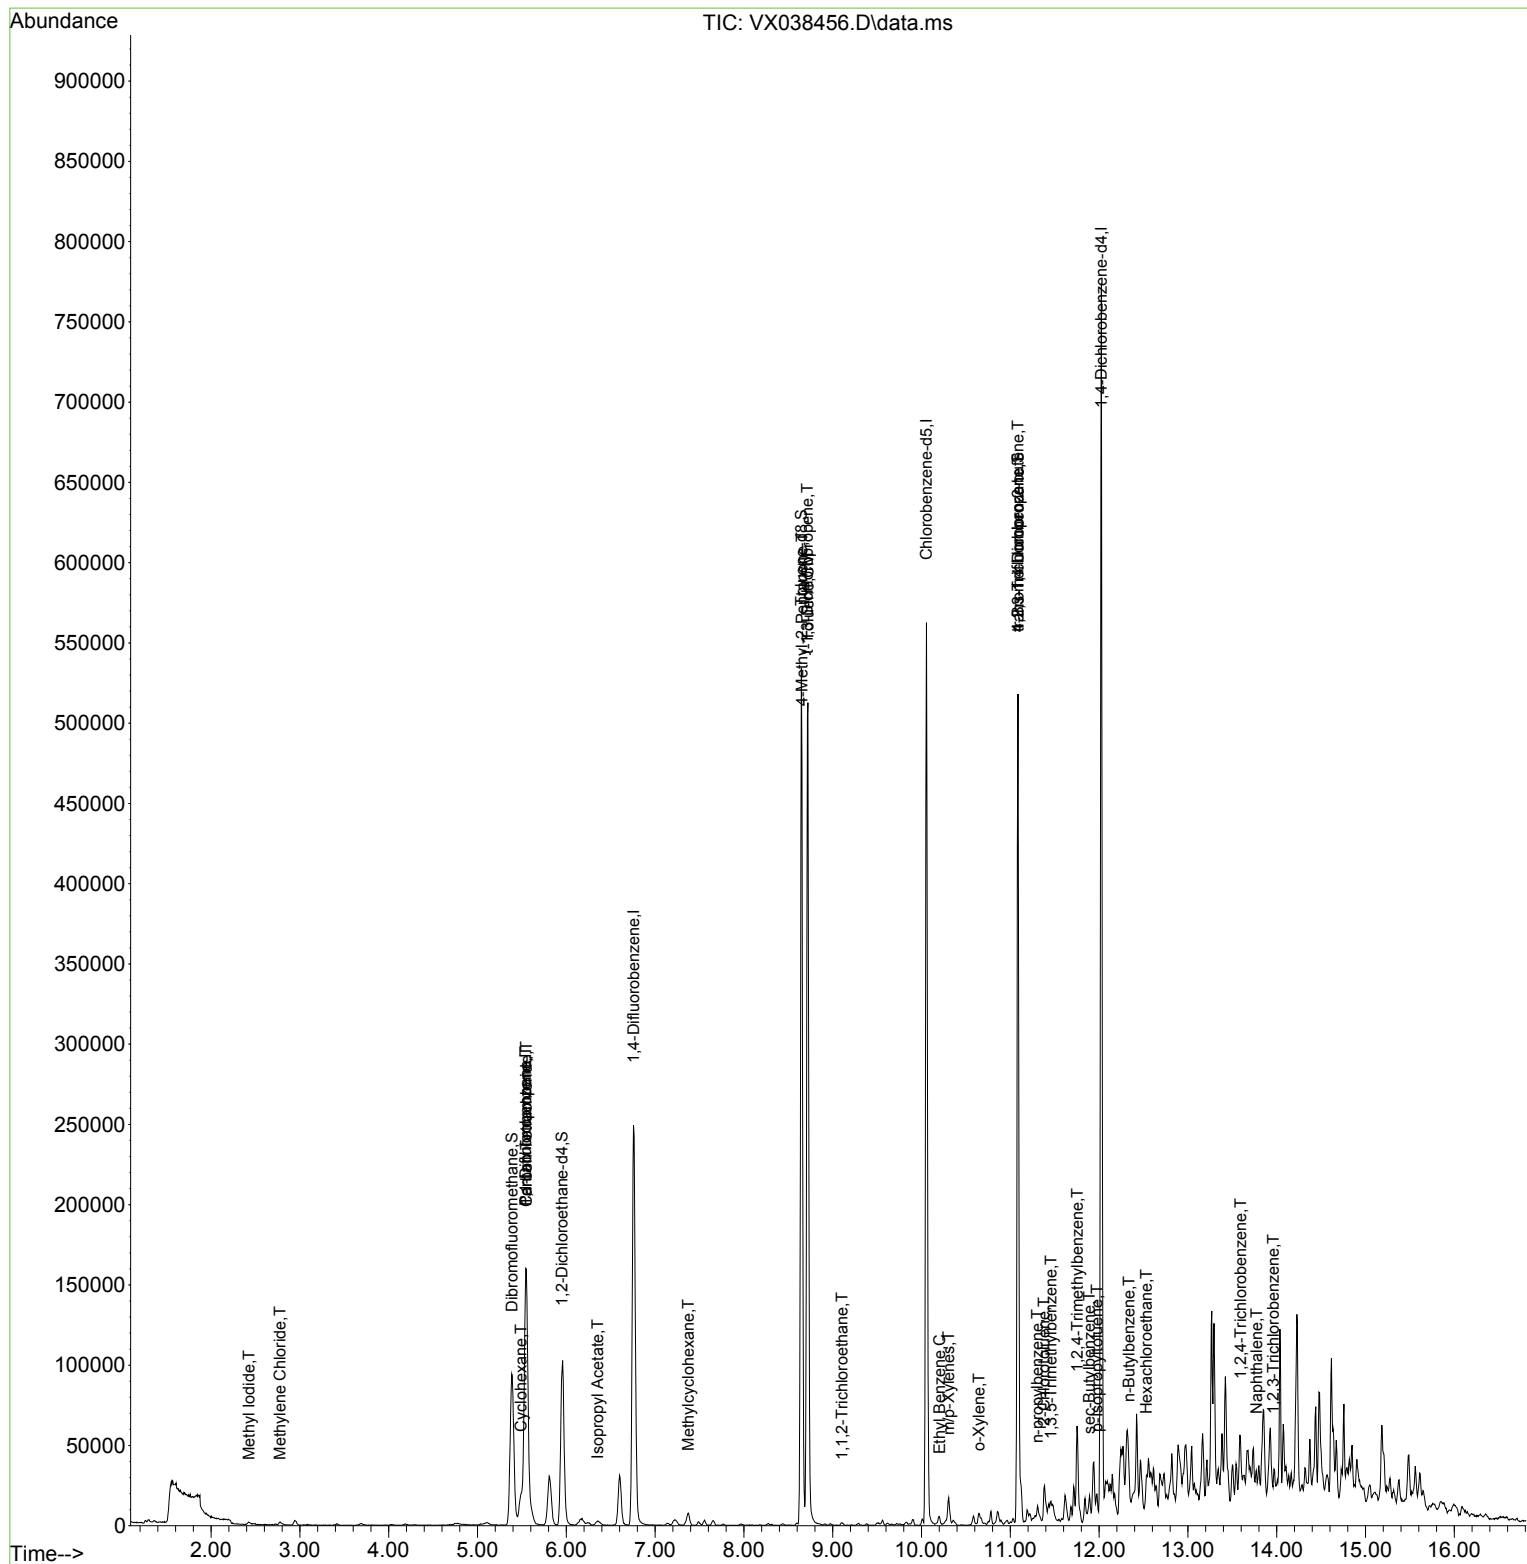






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.012 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 157814
Ion Ratio Lower Upper
168 100
99 54.5 56.6 85.0#



#5
Bromomethane
Concen: Below Cal
RT: 1.599 min Scan# 84
Delta R.T. 0.000 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Tgt Ion: 94 Resp: 594
Ion Ratio Lower Upper
94 100
96 100.7 74.6 111.8

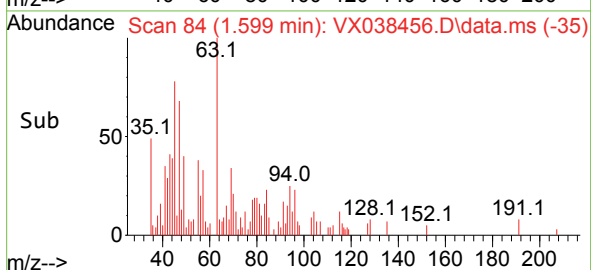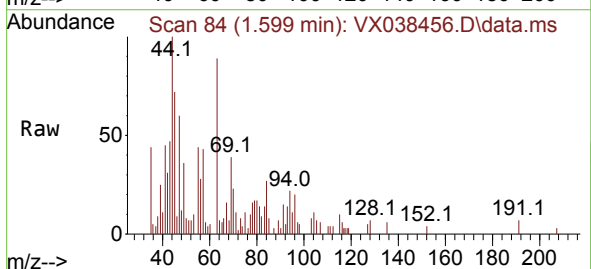

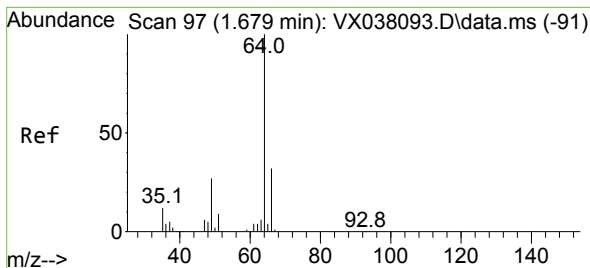

#6

Chloroethane

Concen: Below Cal

RT: 1.679 min Scan# 91

Delta R.T. -0.000 min

Lab File: VX038456.D

Acq: 24 Oct 2023 15:31

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 64 Resp: 148

Ion Ratio Lower Upper

64 100

66 33.9 25.1 37.7

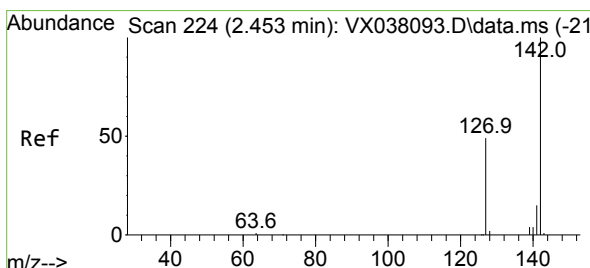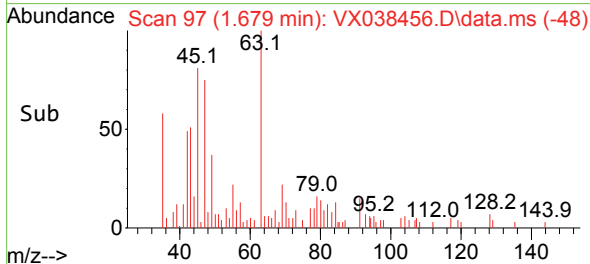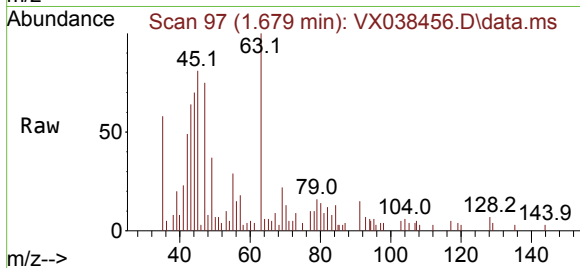

#10

Methyl Iodide

Concen: 0.615 ug/l

RT: 2.428 min Scan# 220

Delta R.T. -0.025 min

Lab File: VX038456.D

Acq: 24 Oct 2023 15:31




Tgt Ion: 142 Resp: 1314


Ion Ratio Lower Upper

142 100

127 36.8 41.6 62.4#

141 11.5 11.6 17.4#

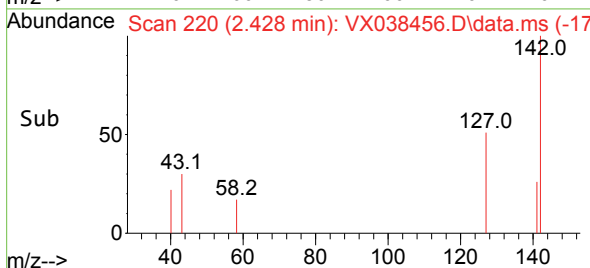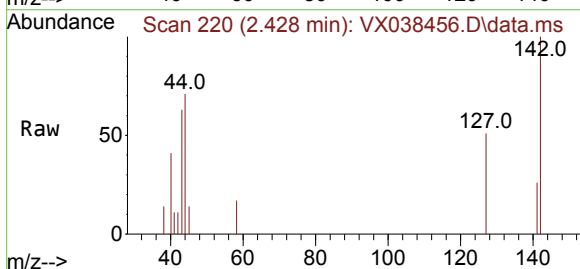

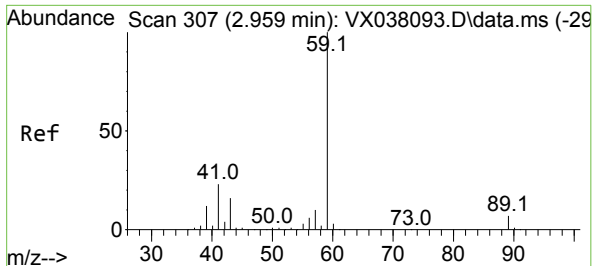

#11

Tert butyl alcohol

Concen: Below Cal

RT: 2.947 min Scan# 307

Delta R.T. -0.012 min

Lab File: VX038456.D

Acq: 24 Oct 2023 15:31

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 59 Resp: 1585

Ion Ratio Lower Upper

59 100

57 1.2 6.0 9.0#

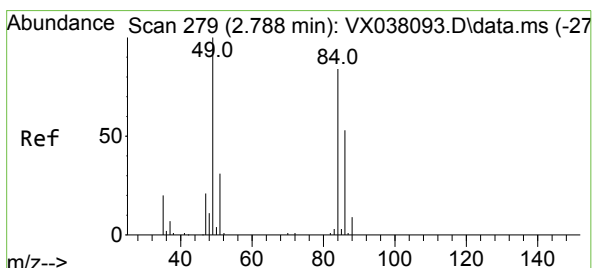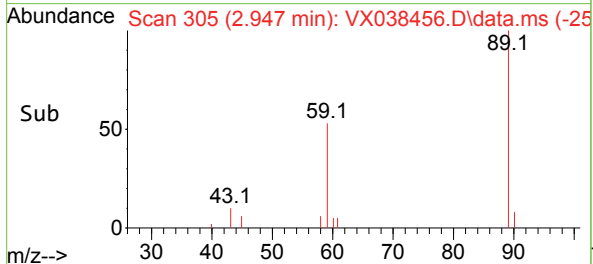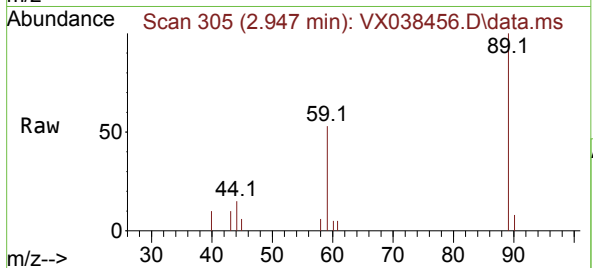

#20

Methylene Chloride

Concen: 0.504 ug/l

RT: 2.776 min Scan# 277

Delta R.T. -0.012 min

Lab File: VX038456.D

Acq: 24 Oct 2023 15:31

Tgt Ion: 84 Resp: 1005




Ion Ratio Lower Upper


84 100

49 120.4 103.6 155.4

51 38.4 33.8 50.6


86 64.4 49.4 74.0

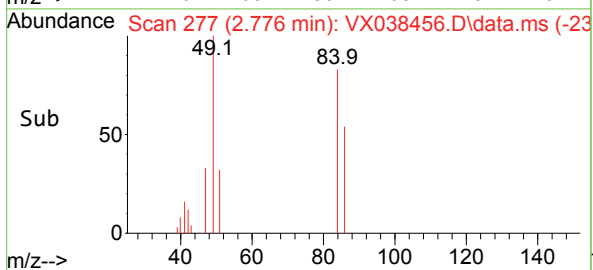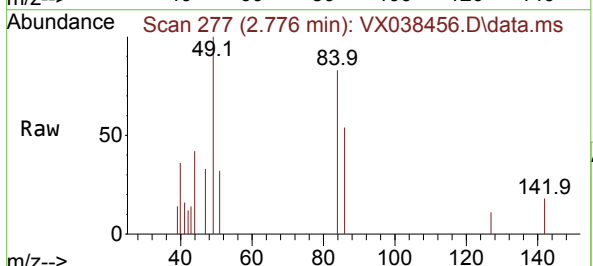



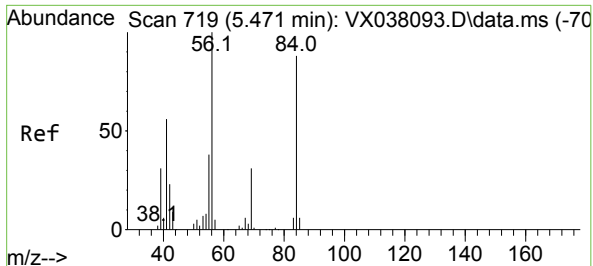


#31
Cyclohexane
Concen: 1.607 ug/l
RT: 5.489 min Scan# 719
Delta R.T. 0.018 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Instrument :
MSVOA_X
ClientSampleId :



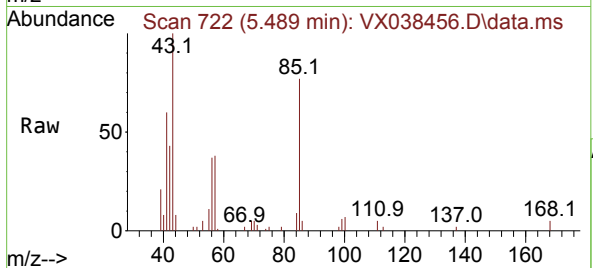



Tgt Ion: 56 Resp: 4419
Ion Ratio Lower Upper
56 100
69 12.3 23.4 35.2#
84 24.5 65.9 98.9#

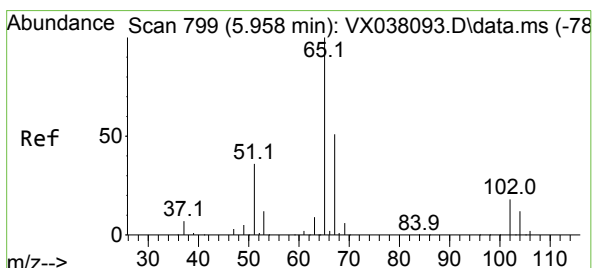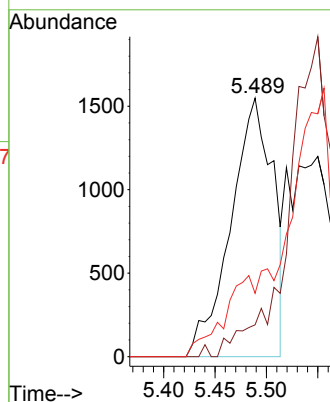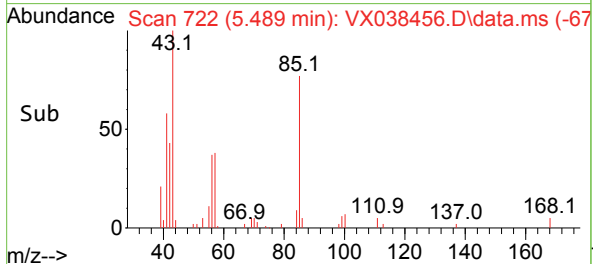

#33
1,2-Dichloroethane-d4
Concen: 39.026 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31


Tgt Ion: 65 Resp: 99062
Ion Ratio Lower Upper
65 100
67 52.0 0.0 100.2

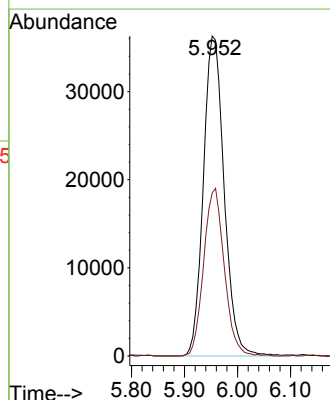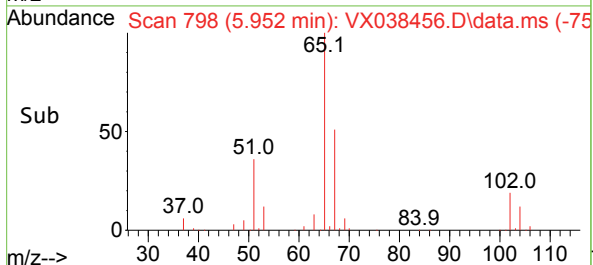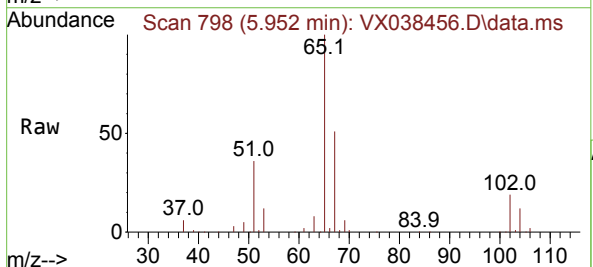



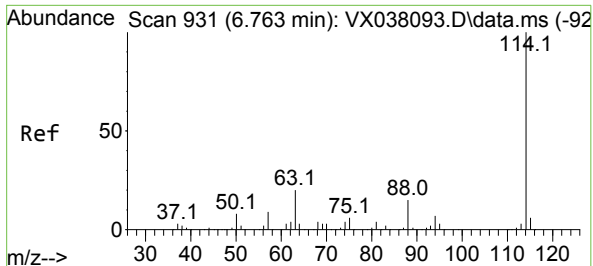


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 911
Delta R.T. -0.006 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Instrument :
MSVOA_X
ClientSampleId :



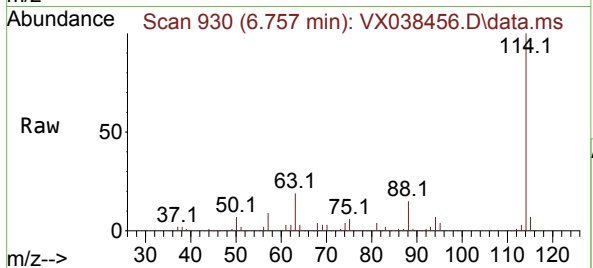



Tgt Ion:114 Resp: 270856
Ion Ratio Lower Upper
114 100
63 19.0 0.0 45.0
88 15.2 0.0 36.6

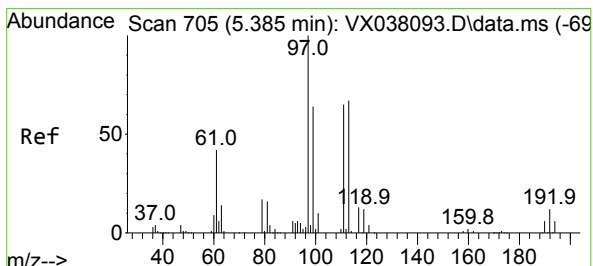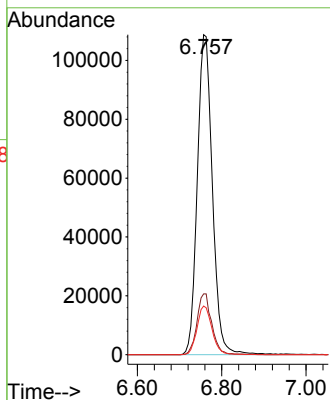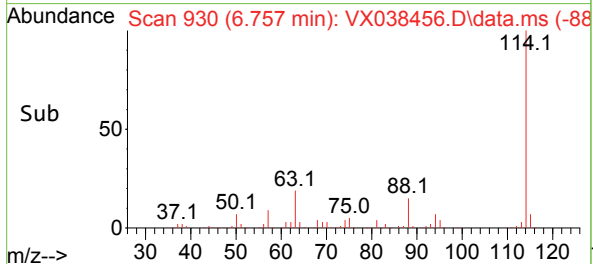

#35
Dibromofluoromethane
Concen: 42.590 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31


Tgt Ion:113 Resp: 83123
Ion Ratio Lower Upper
113 100
111 101.7 82.9 124.3
192 18.7 13.3 19.9

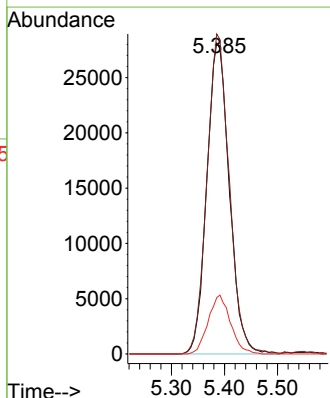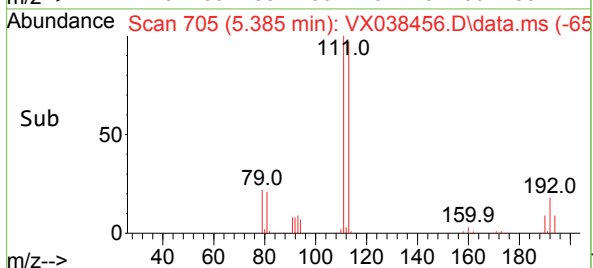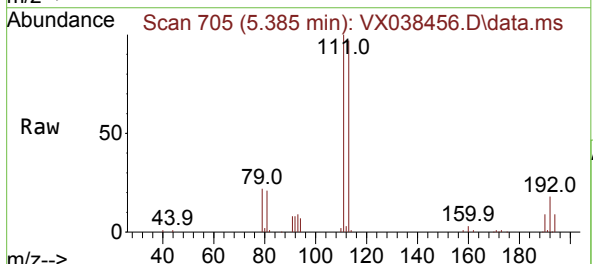






#36
1,1-Dichloropropene
Concen: 4.284 ug/l
RT: 5.544 min Scan# 711
Delta R.T. -0.146 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 75 Resp: 11531
Ion Ratio Lower Upper
75 100
110 9.7 17.0 50.9#
77 0.0 24.7 37.1#



#38
Carbon Tetrachloride
Concen: 6.019 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.128 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31


Tgt Ion: 117 Resp: 15935
Ion Ratio Lower Upper
117 100
119 4.6 78.2 117.2#
121 0.0 24.4 36.6#

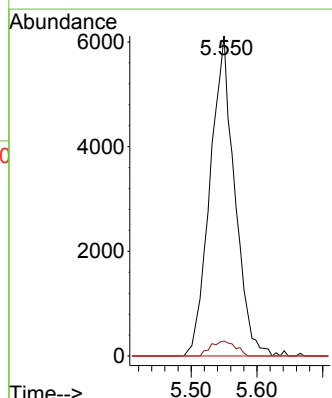






#39
Methylcyclohexane
Concen: 1.041 ug/l
RT: 7.373 min Scan# 1032
Delta R.T. -0.012 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Instrument :
MSVOA_X
ClientSampleId :



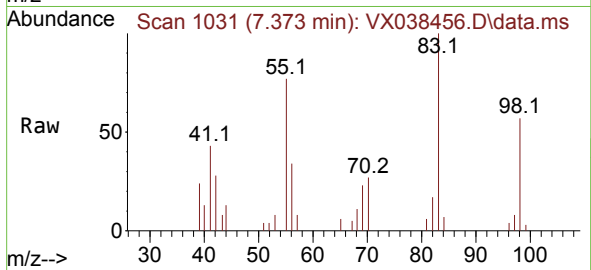



Tgt Ion: 83 Resp: 3281
Ion Ratio Lower Upper
83 100
55 77.3 64.6 97.0
98 56.8 36.7 55.1#



#43
Isopropyl Acetate
Concen: 0.210 ug/l
RT: 6.355 min Scan# 864
Delta R.T. 0.013 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Tgt Ion: 43 Resp: 1001
Ion Ratio Lower Upper
43 100
61 0.0 15.2 22.8#
87 0.0 9.8 14.6#


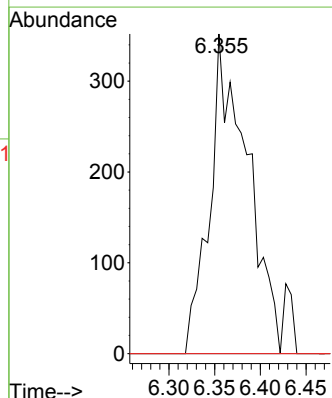

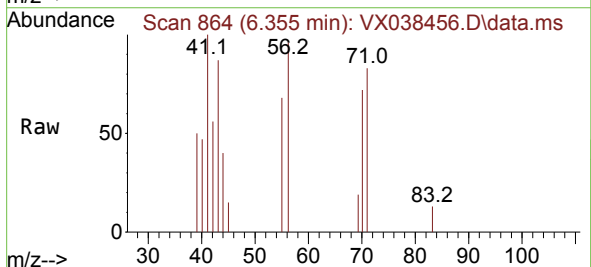




#50
Toluene-d8
Concen: 44.091 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.006 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 328823
Ion Ratio Lower Upper
98 100
100 63.9 53.1 79.7

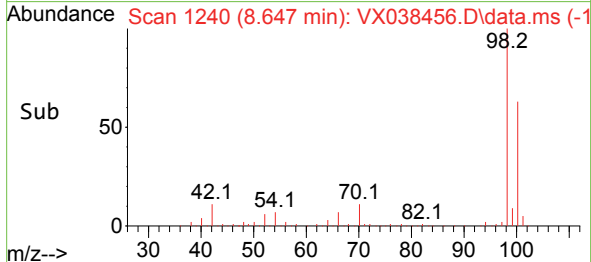

#51
4-Methyl-2-Pentanone
Concen: 0.437 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.079 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Tgt Ion: 43 Resp: 1438
Ion Ratio Lower Upper
43 100
58 179.8 30.4 45.6#


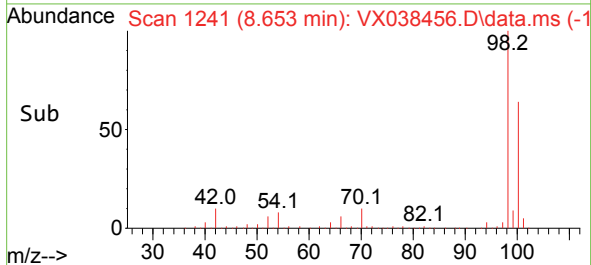

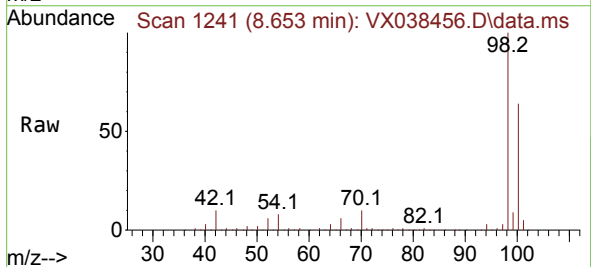




#52
Toluene
Concen: 41.333 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 202674
Ion Ratio Lower Upper
92 100
91 175.9 134.2 201.2

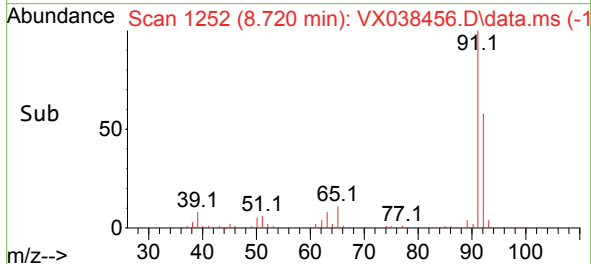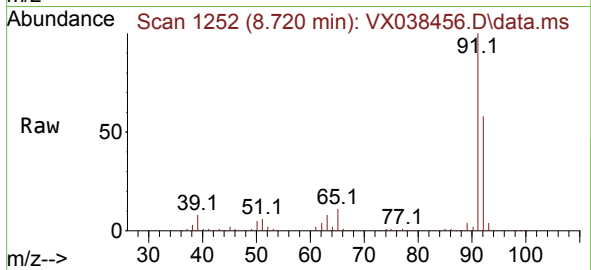

#53
t-1,3-Dichloropropene
Concen: 0.862 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.262 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31


Tgt Ion: 75 Resp: 2488
Ion Ratio Lower Upper
75 100
77 174.9 25.7 38.5#

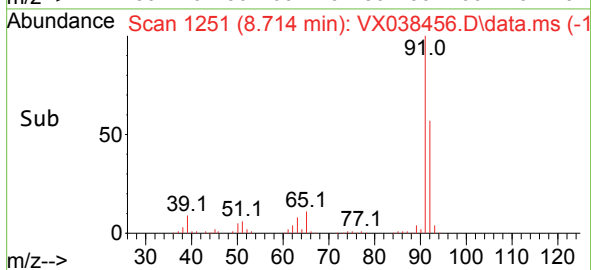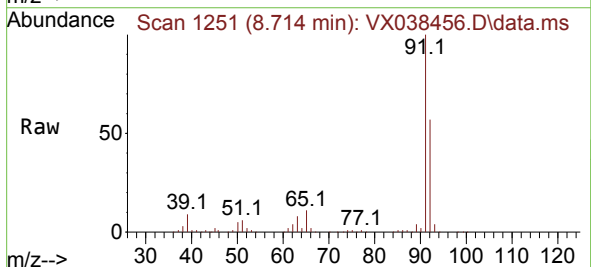






#55
1,1,2-Trichloroethane
Concen: 0.255 ug/l
RT: 9.104 min Scan# 11
Delta R.T. -0.049 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 97	Resp: 535
Ion Ratio	Lower Upper
97 100	
83 0.0	65.8 98.8#
85 25.1	41.6 62.4#
99 0.0	47.8 71.8#

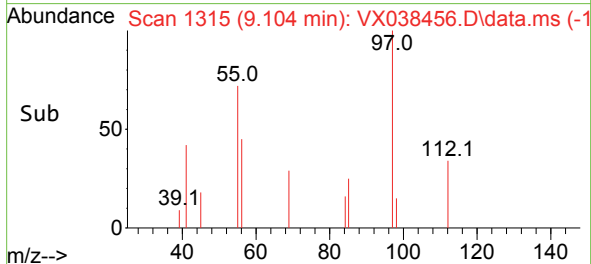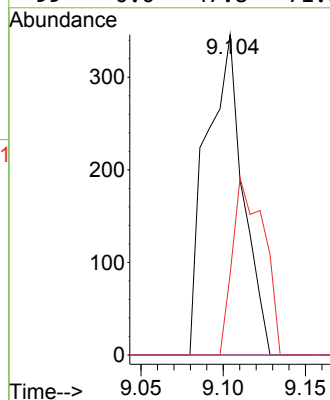

#62
4-Bromofluorobenzene
Concen: 46.707 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Tgt Ion: 95	Resp: 132057
Ion Ratio	Lower Upper
95 100	
174 82.4	0.0 135.6
176 80.0	0.0 131.0


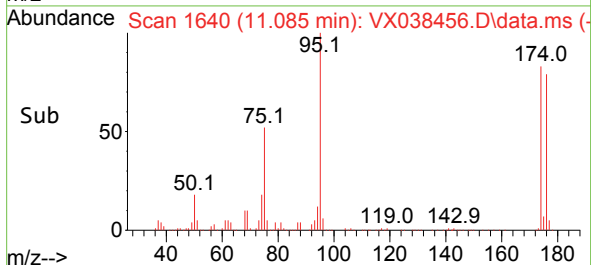
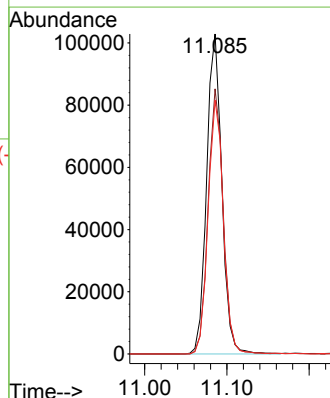
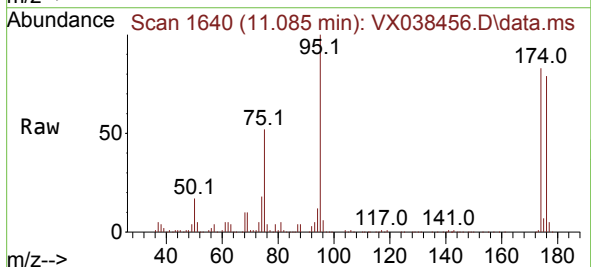




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 269308
Ion Ratio Lower Upper
117 100
82 54.3 46.2 69.4
119 32.0 25.5 38.3

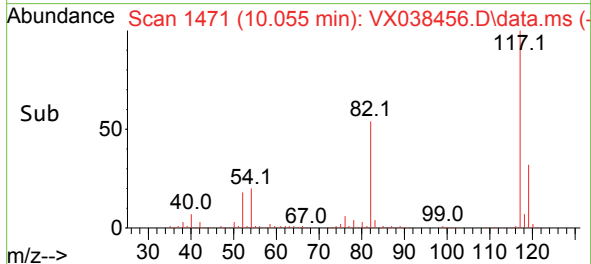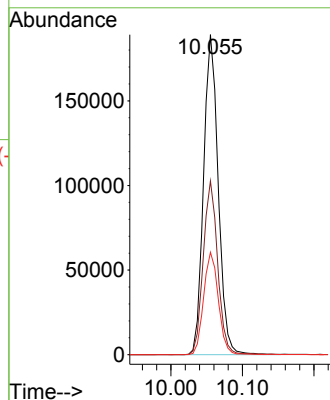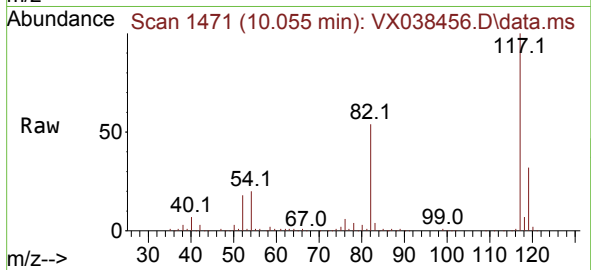

#67
Ethyl Benzene
Concen: 0.306 ug/l
RT: 10.201 min Scan# 1495
Delta R.T. 0.006 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Tgt Ion: 91 Resp: 3083
Ion Ratio Lower Upper
91 100
106 37.8 24.9 37.3#



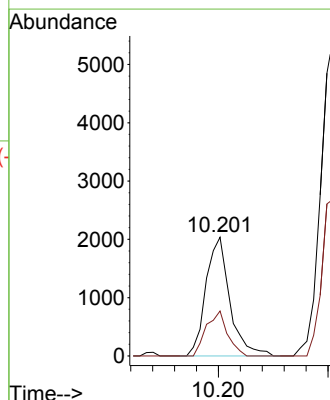
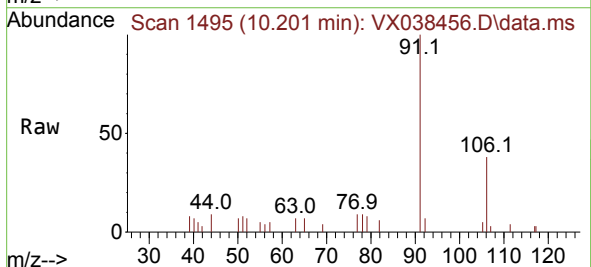




#68
m/p-Xylenes
Concen: 1.001 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 3895
Ion Ratio Lower Upper
106 100
91 217.4 165.5 248.3

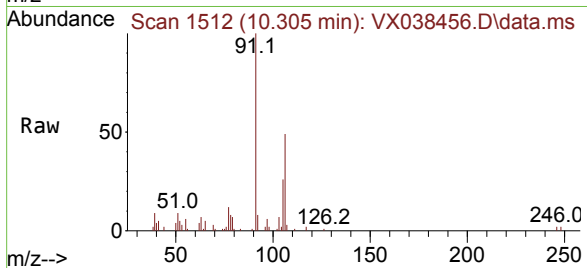

#69
o-Xylene
Concen: 0.466 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. 0.007 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Tgt Ion:106 Resp: 1768
Ion Ratio Lower Upper
106 100
91 229.6 108.9 326.8

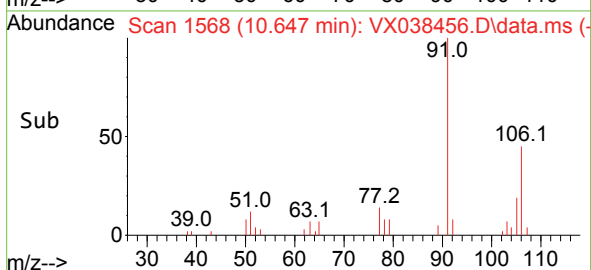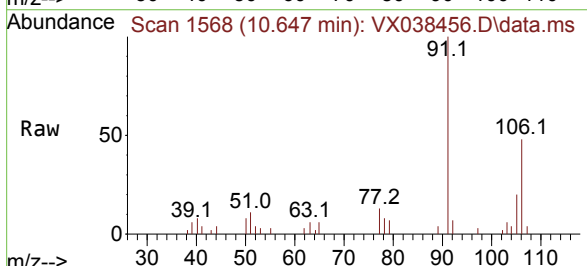



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX038456.D

Acq: 24 Oct 2023 15:31

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:152 Resp: 156222

Ion Ratio Lower Upper

152 100

115 59.4 43.3 129.9

150 156.2 0.0 345.0

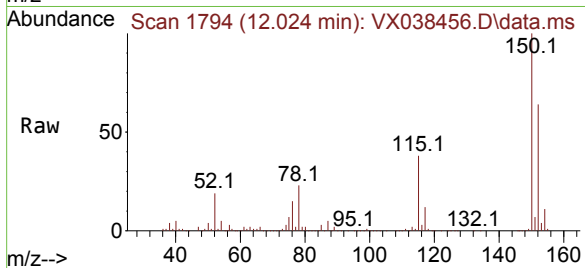

#76

1,2,3-Trichloropropane

Concen: 19.479 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. -0.153 min

Lab File: VX038456.D




Acq: 24 Oct 2023 15:31


Tgt Ion: 75 Resp: 69181

Ion Ratio Lower Upper

75 100

77 1.2 19.1 57.5#


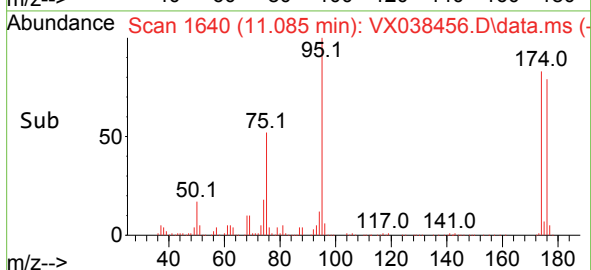

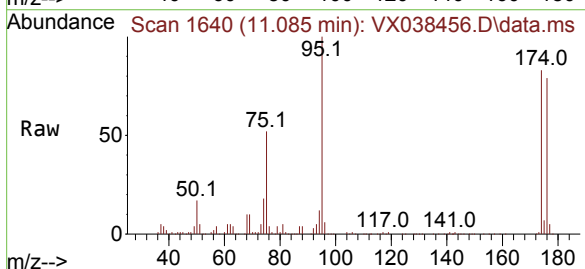




#78
n-propylbenzene
Concen: 0.420 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 5380
Ion Ratio Lower Upper
91 100
120 23.6 11.5 34.4

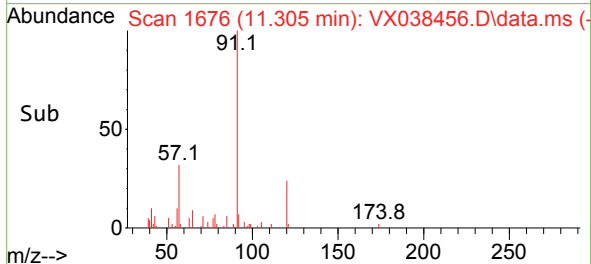

#79
2-Chlorotoluene
Concen: 0.354 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Tgt Ion: 91 Resp: 2690
Ion Ratio Lower Upper
91 100
126 0.7 16.3 48.8#

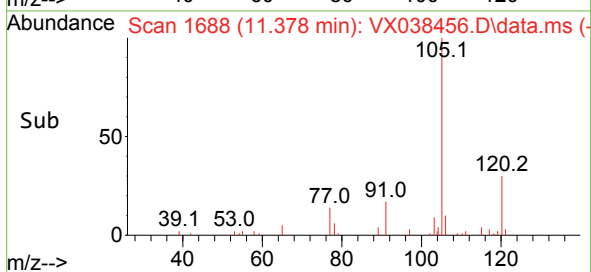



#80

1,3,5-Trimethylbenzene

Concen: 0.547 ug/l

RT: 11.457 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX038456.D

Acq: 24 Oct 2023 15:31

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 4946

Ion Ratio Lower Upper

105 100

120 42.9 24.1 72.3

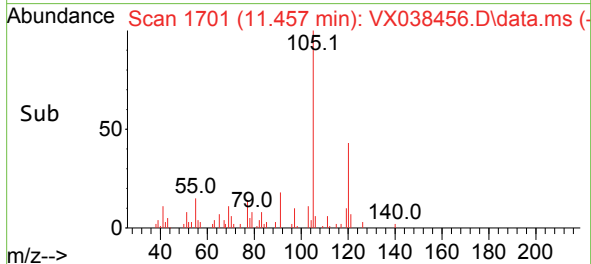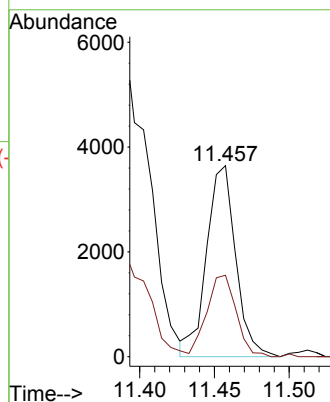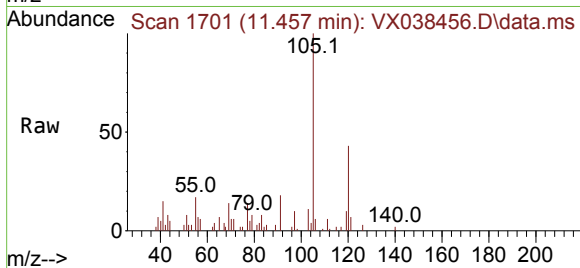

#81

trans-1,4-Dichloro-2-butene

Concen: 56.324 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. 0.067 min

Lab File: VX038456.D

Acq: 24 Oct 2023 15:31




Tgt Ion: 75 Resp: 69181


Ion Ratio Lower Upper

75 100

53 0.2 90.5 135.7#

89 0.1 36.9 55.3#

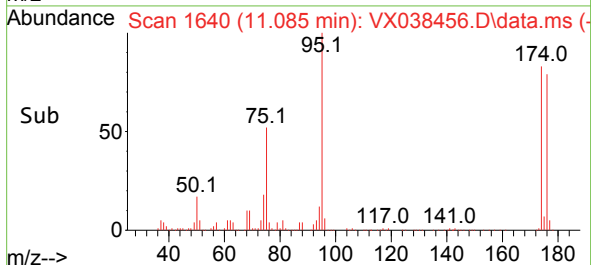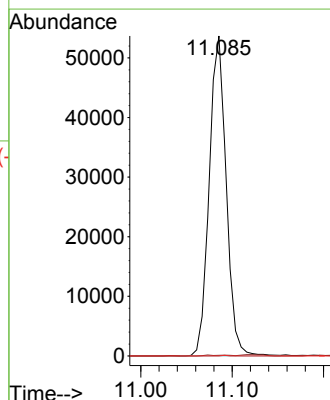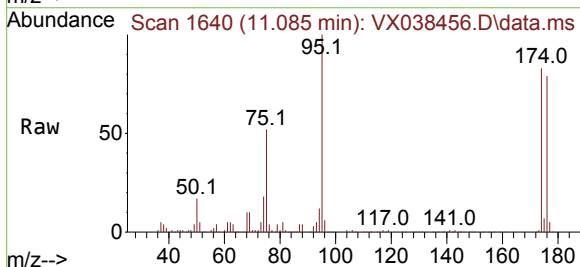



#84

1,2,4-Trimethylbenzene

Concen: 2.048 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. 0.006 min

Lab File: VX038456.D

Acq: 24 Oct 2023 15:31

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 18455

Ion Ratio Lower Upper

105 100

120 44.0 21.2 63.6

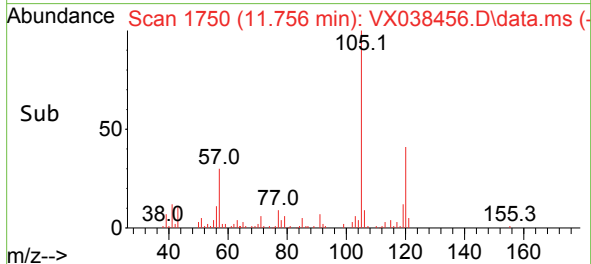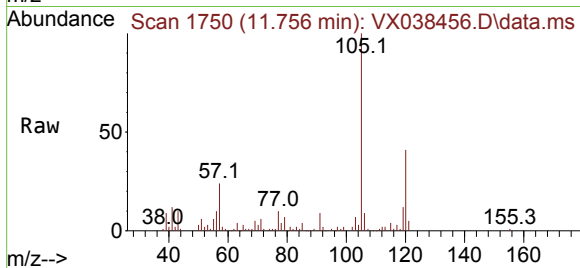

#85

sec-Butylbenzene

Concen: 0.245 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. 0.000 min

Lab File: VX038456.D




Acq: 24 Oct 2023 15:31


Tgt Ion:105 Resp: 2806

Ion Ratio Lower Upper

105 100

134 23.4 9.8 29.4




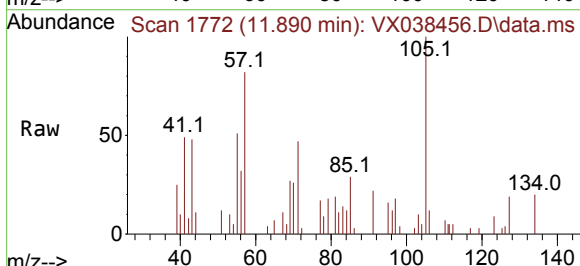


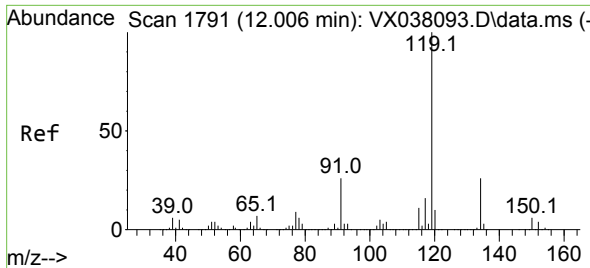

#86
p-Isopropyltoluene
Concen: 0.306 ug/l
RT: 11.976 min Scan# 1786
Delta R.T. -0.030 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:119 Resp: 2886
Ion Ratio Lower Upper
119 100
134 25.8 12.8 38.3
91 26.5 13.1 39.3

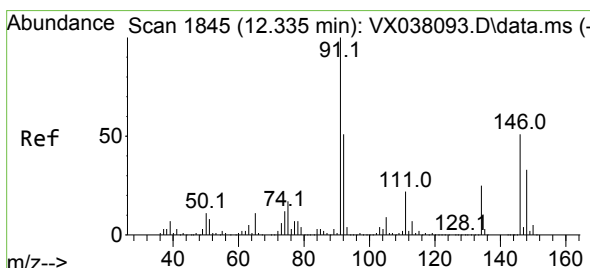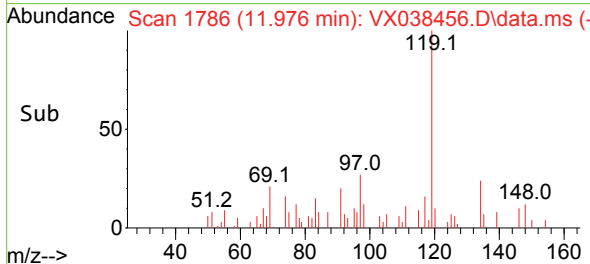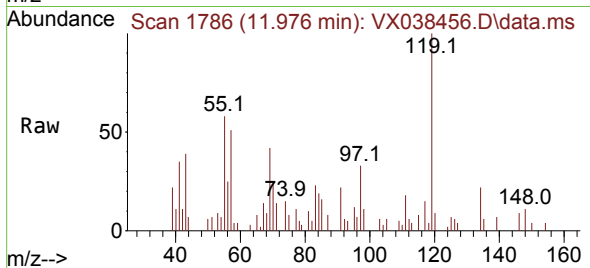

#89
n-Butylbenzene
Concen: 0.858 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX038456.D
Acq: 24 Oct 2023 15:31

Tgt Ion: 91 Resp: 8065
Ion Ratio Lower Upper
91 100
92 38.1 27.4 82.0
134 75.0 12.6 37.8#

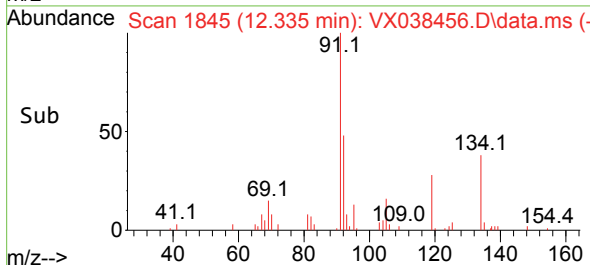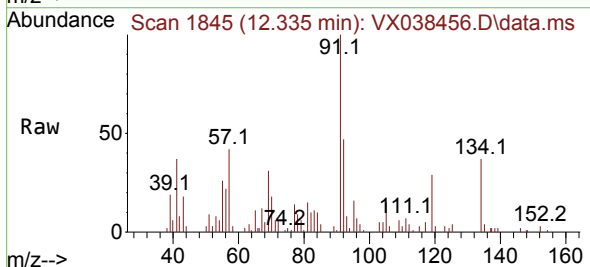



#90

Hexachloroethane

Concen: 0.367 ug/l

RT: 12.530 min Scan# 117

Delta R.T. -0.006 min

Lab File: VX038456.D

Acq: 24 Oct 2023 15:31

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:117 Resp: 574

Ion Ratio Lower Upper

117 100

201 0.0 32.9 98.6#

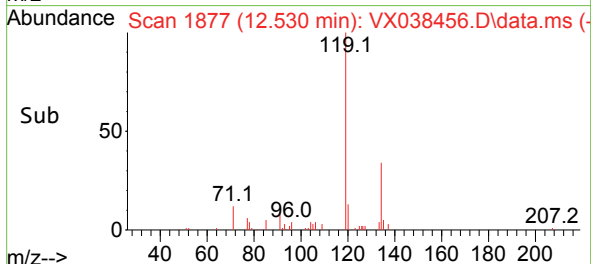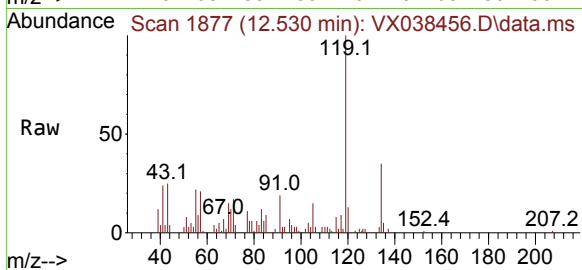

#93

1,2,4-Trichlorobenzene

Concen: 0.590 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX038456.D

Acq: 24 Oct 2023 15:31




Tgt Ion:180 Resp: 1953


Ion Ratio Lower Upper

180 100

182 99.0 48.3 144.8

145 80.1 18.0 54.0#

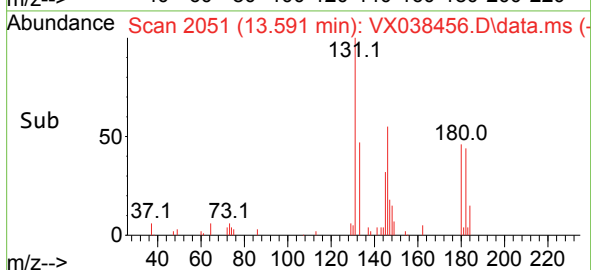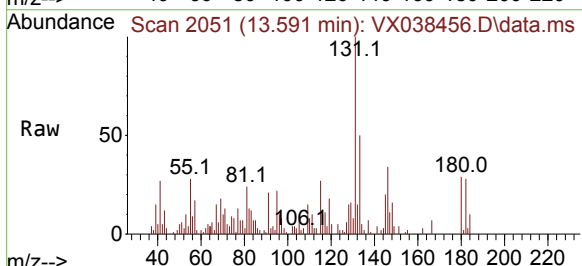



#95

Naphthalene

Concen: 0.452 ug/l

RT: 13.774 min Scan# 2081

Delta R.T. 0.000 min

Lab File: VX038456.D





Acq: 24 Oct 2023 15:31

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:	128	Resp:	5216
Ion Ratio	Lower	Upper	
128	100		
127	17.8	10.3	15.5#
129	15.8	8.8	13.2#

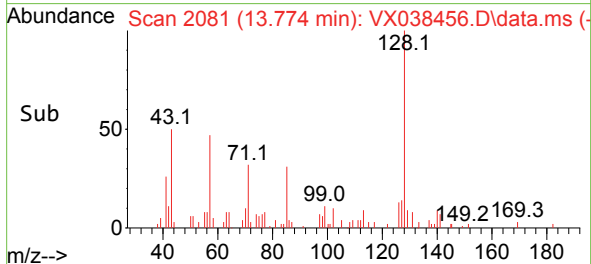

#96

1,2,3-Trichlorobenzene

Concen: 0.228 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. 0.000 min

Lab File: VX038456.D

Acq: 24 Oct 2023 15:31

Tgt Ion:	180	Resp:	732
Ion Ratio	Lower	Upper	
180	100		
182	96.3	46.9	140.6
145	229.1	17.8	53.5#

