

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102423\
 Data File : VX038449.D
 Acq On : 24 Oct 2023 12:16
 Operator : JC/MD
 Sample : VX1024MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1024MBL01

Quant Time: Oct 25 06:06:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 05 15:27:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	150429	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	264046	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	260415	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	137014	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	97540	40.313	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	80.620%
35) Dibromofluoromethane	5.385	113	85951	45.175	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.360%
50) Toluene-d8	8.647	98	317351	43.650	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	87.300%#
62) 4-Bromofluorobenzene	11.079	95	121101	43.936	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	87.880%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102423\
Data File : VX038449.D
Acq On : 24 Oct 2023 12:16
Operator : JC/MD
Sample : VX1024MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1024MBL01

Quant Time: Oct 25 06:06:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 05 15:27:13 2023
Response via : Initial Calibration




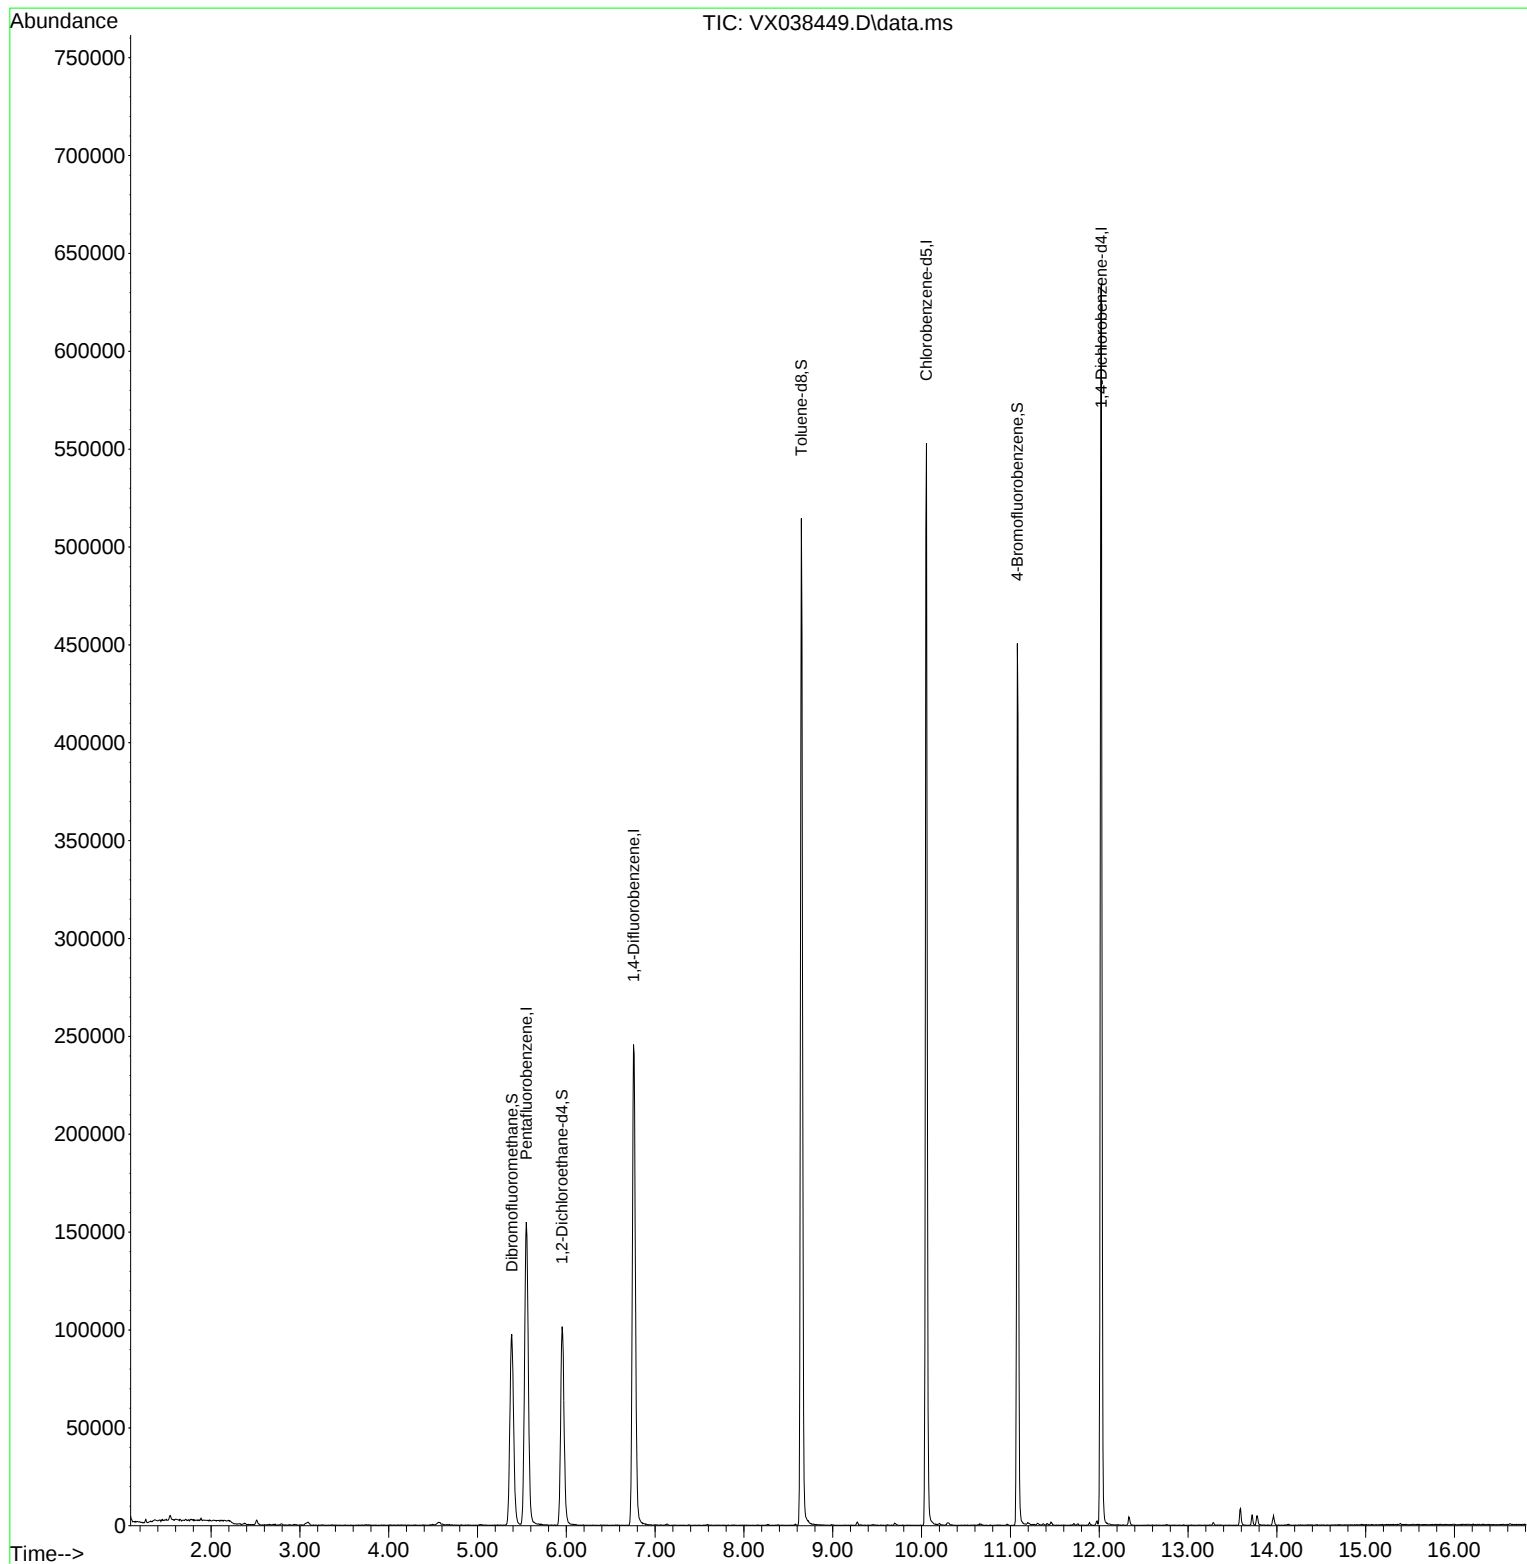




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX038449.D
Acq: 24 Oct 2023 12:16




Instrument :
MSVOA_X
ClientSampleId :
VX1024MBL01


Tgt Ion:168 Resp: 150429
Ion Ratio Lower Upper
168 100
99 57.4 56.6 85.0

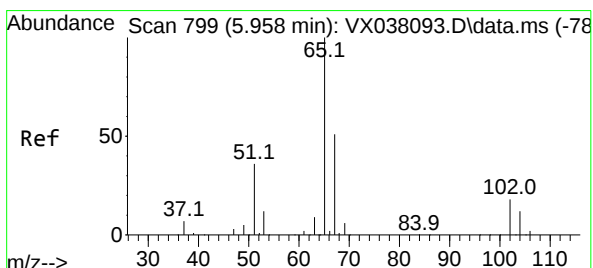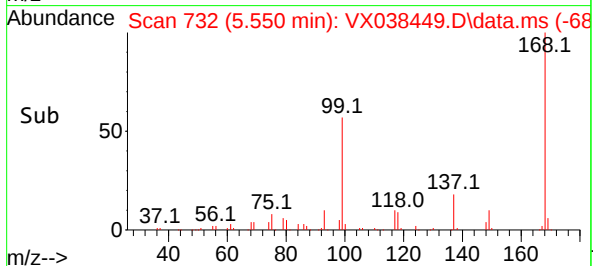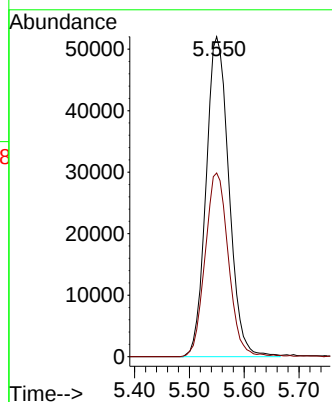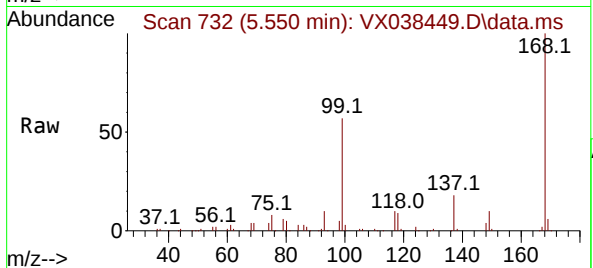

#33
1,2-Dichloroethane-d4
Concen: 40.313 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX038449.D
Acq: 24 Oct 2023 12:16

Tgt Ion: 65 Resp: 97540
Ion Ratio Lower Upper
65 100
67 52.0 0.0 100.2


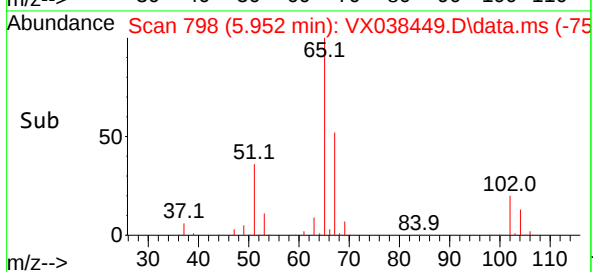
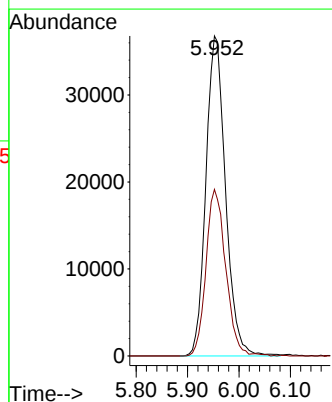
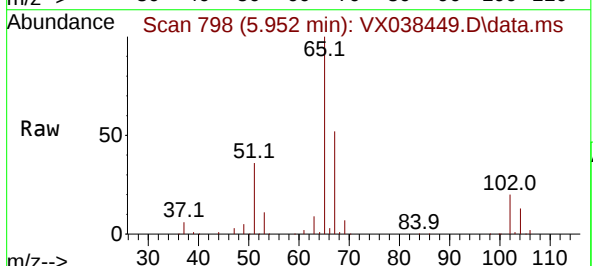


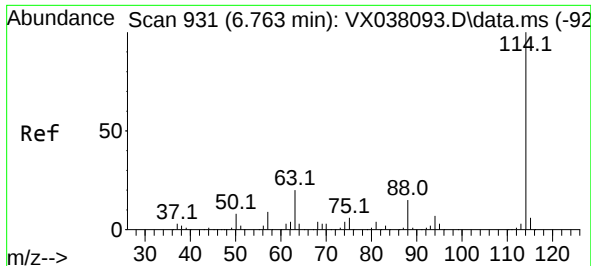

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 911
Delta R.T. -0.006 min
Lab File: VX038449.D
Acq: 24 Oct 2023 12:16




Instrument :
MSVOA_X
ClientSampleId :
VX1024MBL01


Tgt Ion:114 Resp: 264046
Ion Ratio Lower Upper
114 100
63 19.2 0.0 45.0
88 15.1 0.0 36.6

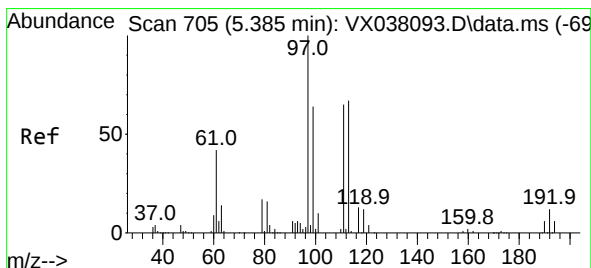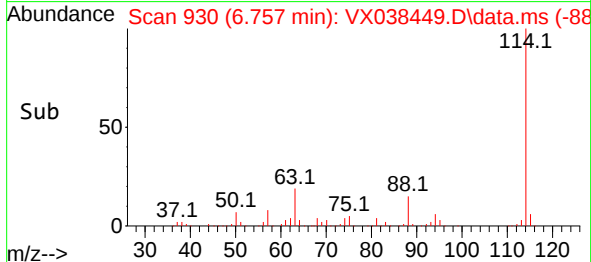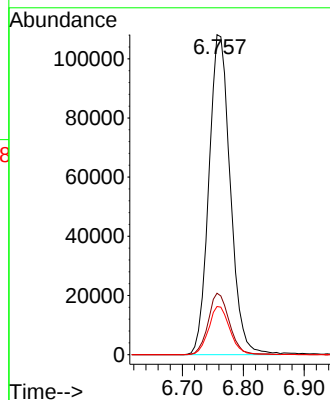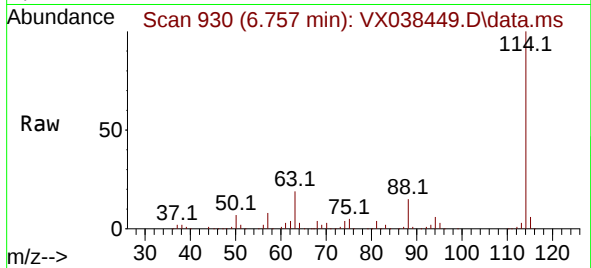

#35
Dibromofluoromethane
Concen: 45.175 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX038449.D
Acq: 24 Oct 2023 12:16

Tgt Ion:113 Resp: 85951
Ion Ratio Lower Upper
113 100
111 102.9 82.9 124.3
192 19.1 13.3 19.9


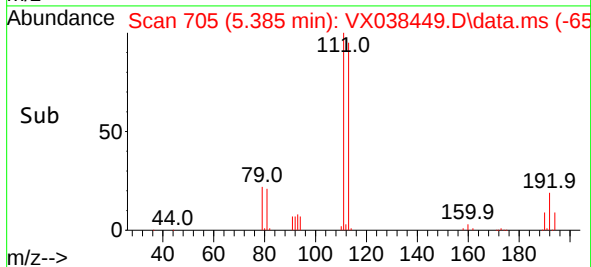
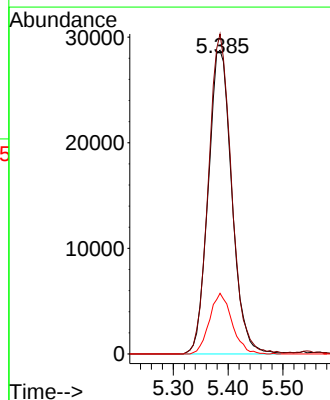
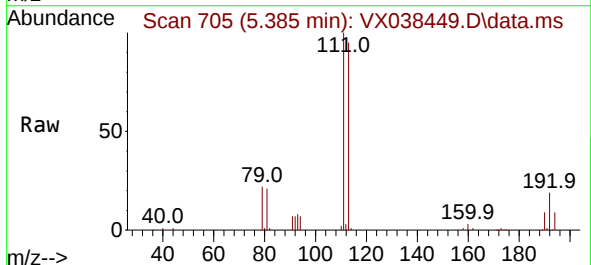


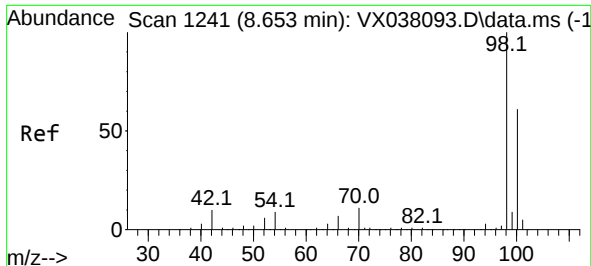

#50
Toluene-d8
Concen: 43.650 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX038449.D
Acq: 24 Oct 2023 12:16




Instrument :
MSVOA_X
ClientSampleId :
VX1024MBL01


Tgt Ion: 98 Resp: 317351
Ion Ratio Lower Upper
98 100
100 64.3 53.1 79.7

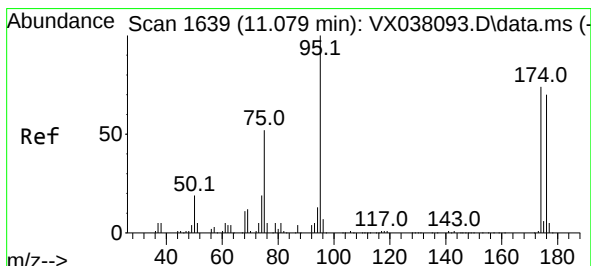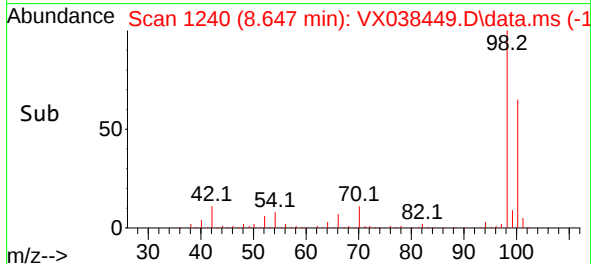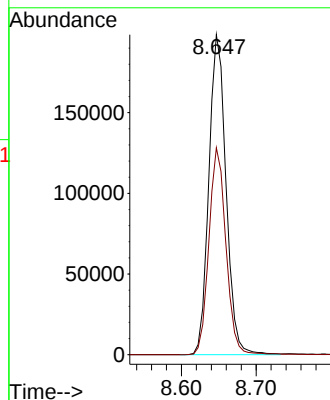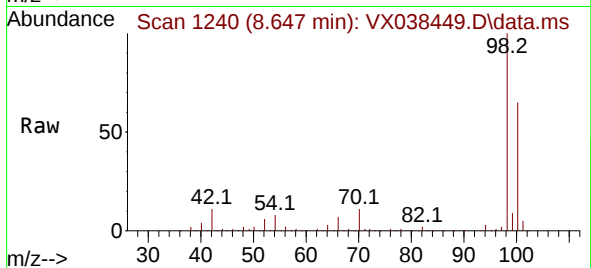

#62
4-Bromofluorobenzene
Concen: 43.936 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX038449.D
Acq: 24 Oct 2023 12:16

Tgt Ion: 95 Resp: 121101
Ion Ratio Lower Upper
95 100
174 82.6 0.0 135.6
176 79.0 0.0 131.0

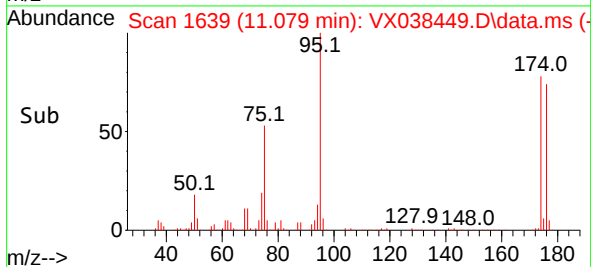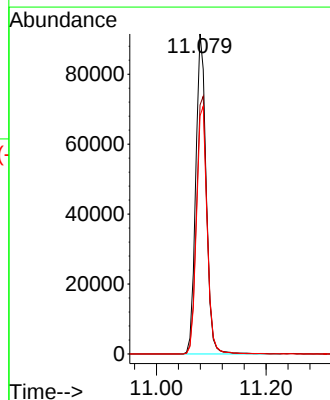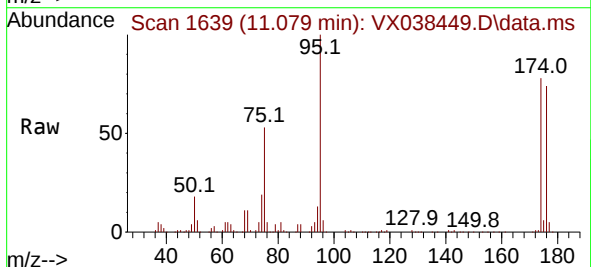

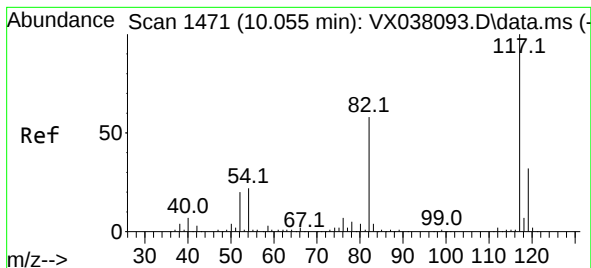

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX038449.D

Acq: 24 Oct 2023 12:16

Instrument :

MSVOA_X

ClientSampleId :

VX1024MBL01





Tgt Ion:117 Resp: 260415

Ion Ratio Lower Upper

117 100

82 52.9 46.2 69.4

119 32.0 25.5 38.3

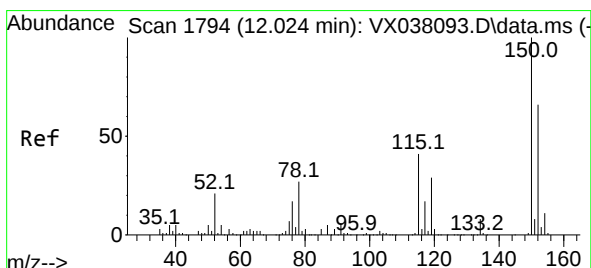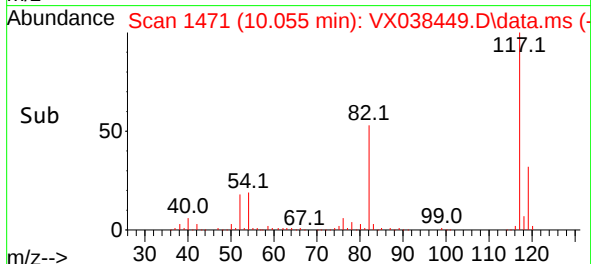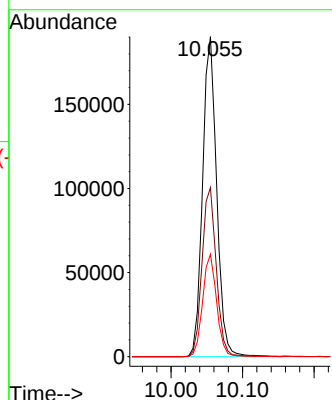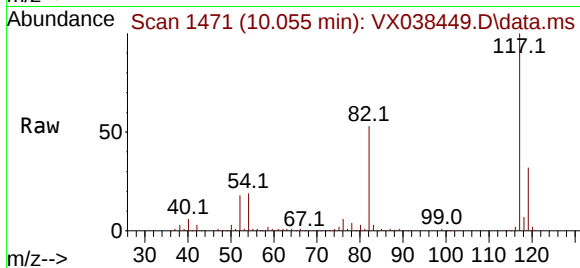

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX038449.D

Acq: 24 Oct 2023 12:16

Tgt Ion:152 Resp: 137014

Ion Ratio Lower Upper

152 100

115 59.3 43.3 129.9

150 156.6 0.0 345.0

