

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102423\  
 Data File : VX038449.D  
 Acq On : 24 Oct 2023 12:16  
 Operator : JC/MD  
 Sample : VX1024MBL01  
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX1024MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038449.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 694           | 705         | 722          | rBV      | 97420          | 286225        | 34.30%          | 6.156%        |
| 2         | 5.550       | 722           | 732         | 753          | rVV      | 154439         | 446796        | 53.55%          | 9.609%        |
| 3         | 5.952       | 786           | 798         | 816          | rBV      | 101466         | 273806        | 32.82%          | 5.889%        |
| 4         | 6.757       | 921           | 930         | 947          | rBV      | 245639         | 598943        | 71.78%          | 12.881%       |
| 5         | 8.647       | 1234          | 1240        | 1252         | rBV      | 514287         | 820928        | 98.39%          | 17.655%       |
| 6         | 10.055      | 1465          | 1471        | 1487         | rBV      | 552733         | 771091        | 92.41%          | 16.583%       |
| 7         | 11.079      | 1634          | 1639        | 1655         | rBV      | 450433         | 606079        | 72.64%          | 13.035%       |
| 8         | 12.024      | 1788          | 1794        | 1807         | rVB      | 633836         | 834386        | 100.00%         | 17.945%       |
| 9         | 13.591      | 2046          | 2051        | 2058         | rBV2     | 8567           | 11511         | 1.38%           | 0.248%        |




Sum of corrected areas: 4649765

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102423\  
Data File : VX038449.D  
Acq On : 24 Oct 2023 12:16  
Operator : JC/MD  
Sample : VX1024MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1024MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

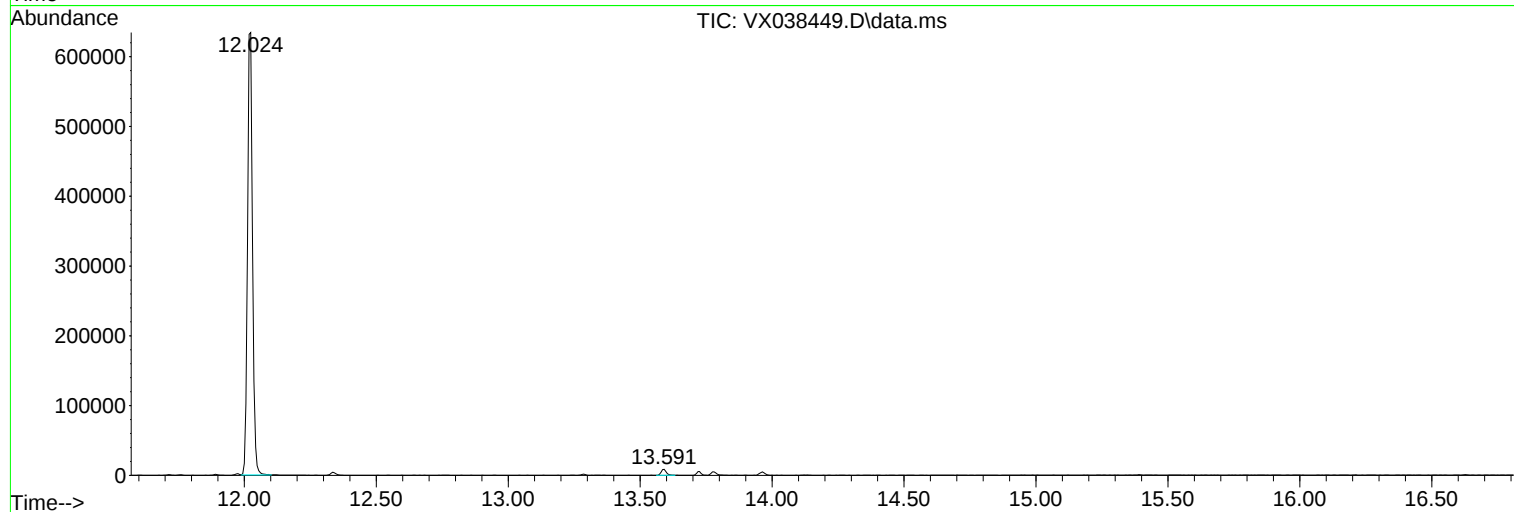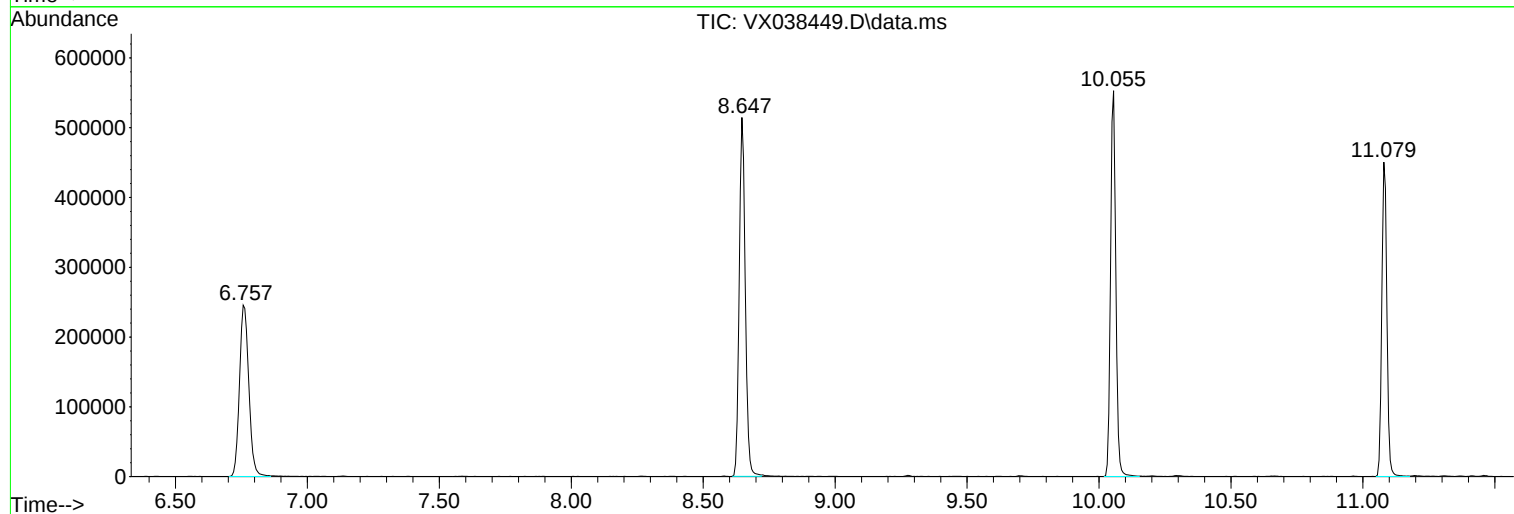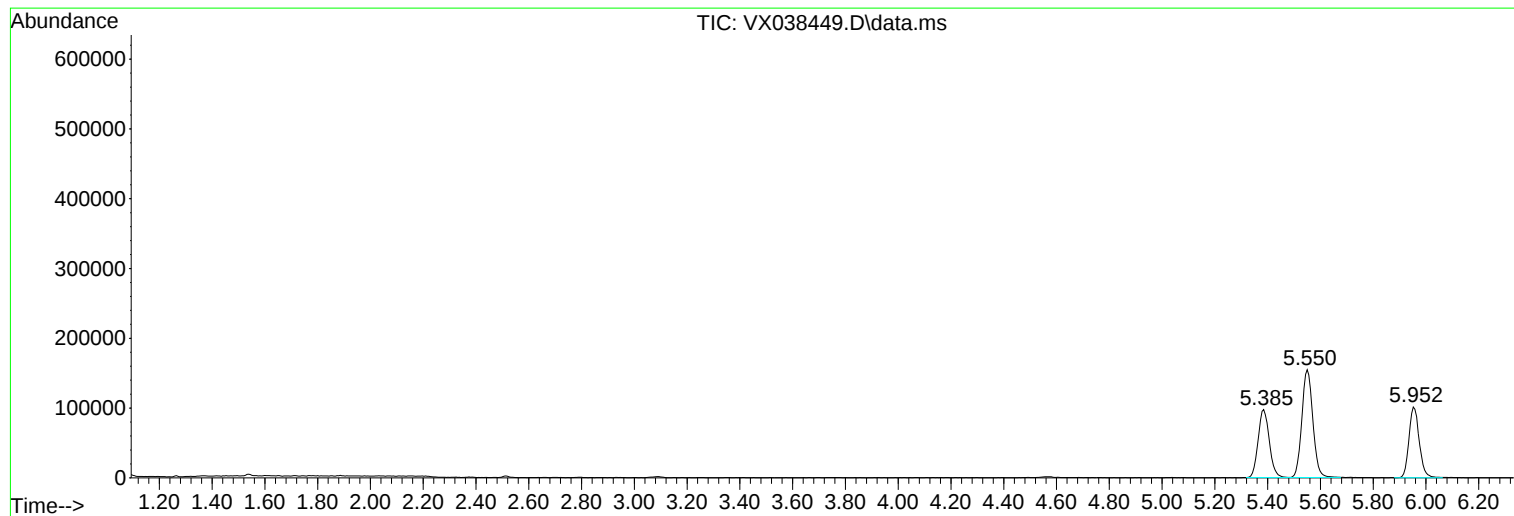

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102423\  
Data File : VX038449.D  
Acq On : 24 Oct 2023 12:16  
Operator : JC/MD  
Sample : VX1024MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1024MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102423\  
Data File : VX038449.D  
Acq On : 24 Oct 2023 12:16  
Operator : JC/MD  
Sample : VX1024MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1024MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|