

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102423\
 Data File : VX038453.D
 Acq On : 24 Oct 2023 13:54
 Operator : JC/MD
 Sample : 04936-07ME
 Misc : 5.07g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1084ME

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Title : SW846 8260

Signal : TIC: VX038453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	68	79	81	rBV4	14475	41407	4.46%	0.767%
2	2.422	213	219	238	rBV	16738	43371	4.67%	0.804%
3	2.946	297	305	315	rBV	9412	20399	2.20%	0.378%
4	5.391	694	706	720	rBV	88944	265365	28.55%	4.918%
5	5.550	720	732	747	rVV	156790	454673	48.92%	8.426%
6	5.952	788	798	813	rBV	106288	277814	29.89%	5.149%
7	6.757	921	930	947	rBV	250016	609680	65.60%	11.299%
8	8.647	1233	1240	1247	rBV	530701	846791	91.12%	15.693%
9	8.720	1247	1252	1268	rVB	71241	124502	13.40%	2.307%
10	10.055	1465	1471	1487	rBV	535487	797781	85.84%	14.785%
11	11.085	1634	1640	1653	rBV	484808	651601	70.11%	12.076%
12	12.024	1789	1794	1800	rBV	754276	929334	100.00%	17.223%
13	12.420	1855	1859	1864	rBV2	30684	36643	3.94%	0.679%
14	12.475	1864	1868	1874	rVB6	4998	9730	1.05%	0.180%
15	12.579	1882	1885	1891	rVB2	6294	9405	1.01%	0.174%
16	12.817	1920	1924	1929	rVB4	8752	12572	1.35%	0.233%
17	12.896	1929	1937	1942	rBV5	12732	32762	3.53%	0.607%
18	12.975	1947	1950	1954	rVV5	14610	20813	2.24%	0.386%
19	13.042	1958	1961	1964	rVB	11760	12459	1.34%	0.231%
20	13.268	1994	1998	2001	rBV	49916	61628	6.63%	1.142%
21	13.384	2013	2017	2020	rBV	13428	17136	1.84%	0.318%
22	13.414	2020	2022	2032	rVB9	8998	22369	2.41%	0.415%
23	13.591	2046	2051	2055	rBV3	11211	17383	1.87%	0.322%
24	13.841	2088	2092	2099	rVB7	5288	9438	1.02%	0.175%
25	14.036	2120	2124	2127	rVB2	9474	10247	1.10%	0.190%
26	14.615	2215	2219	2221	rBV5	7956	9946	1.07%	0.184%
27	14.755	2234	2242	2244	rBV3	11318	16041	1.73%	0.297%
28	15.487	2357	2362	2366	rBV6	11141	17050	1.83%	0.316%
29	16.090	2456	2461	2469	rBV5	9580	17491	1.88%	0.324%




Sum of corrected areas: 5395831

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102423\
Data File : VX038453.D
Acq On : 24 Oct 2023 13:54
Operator : JC/MD
Sample : 04936-07ME
Misc : 5.07g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1084ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

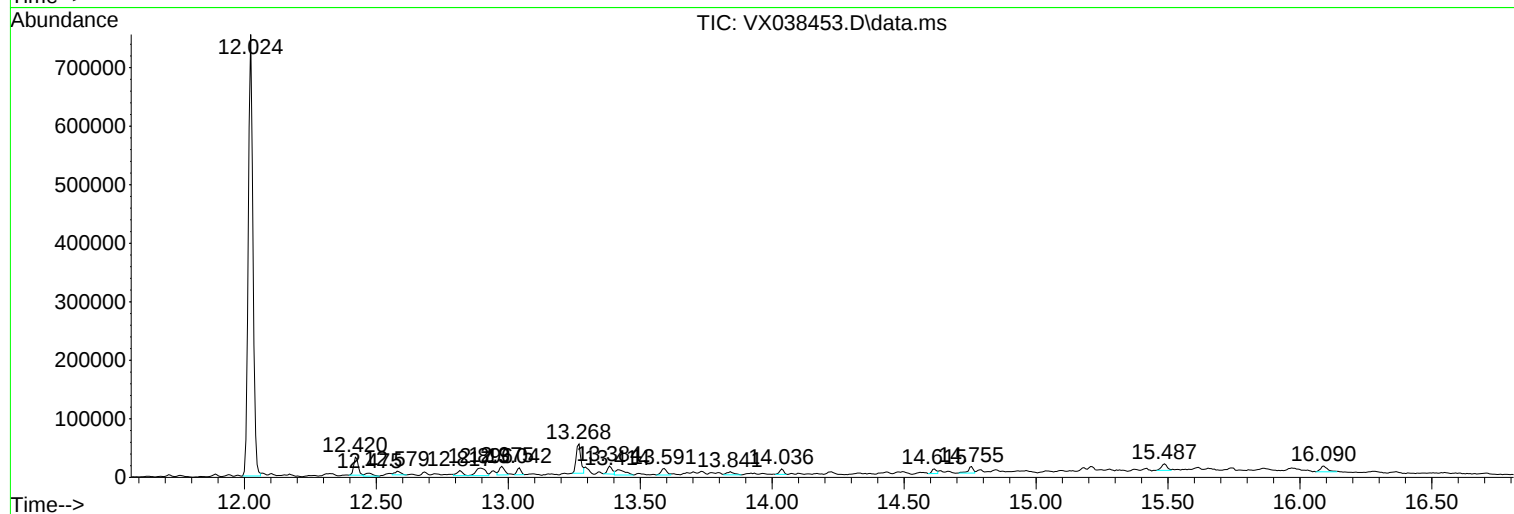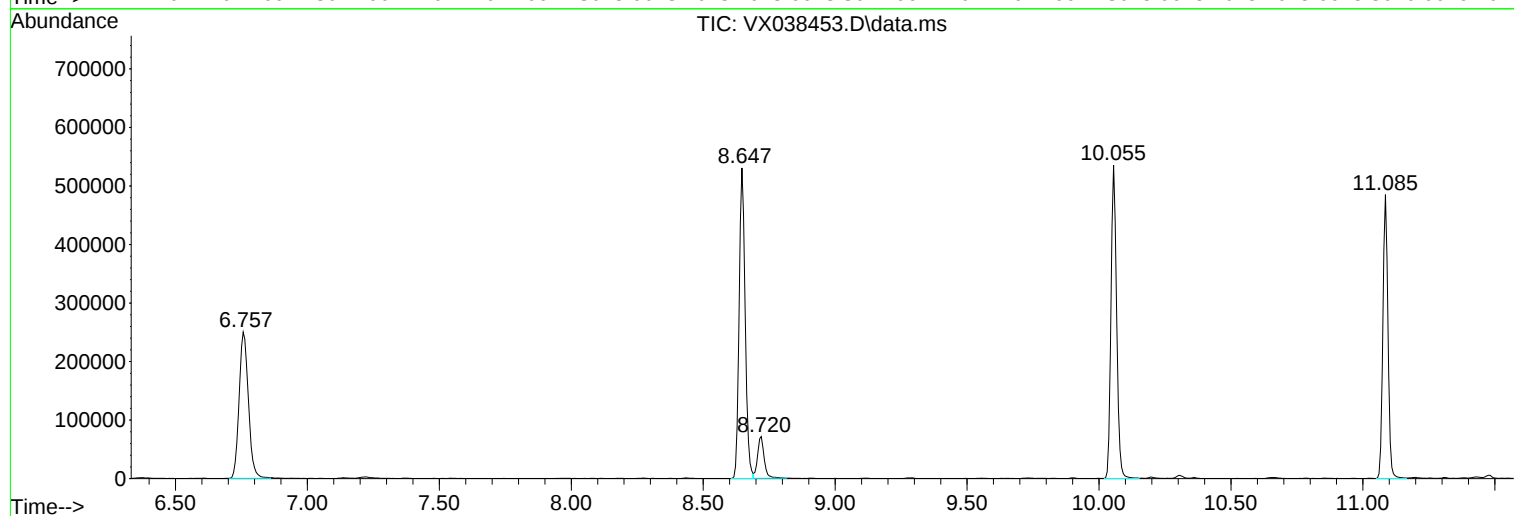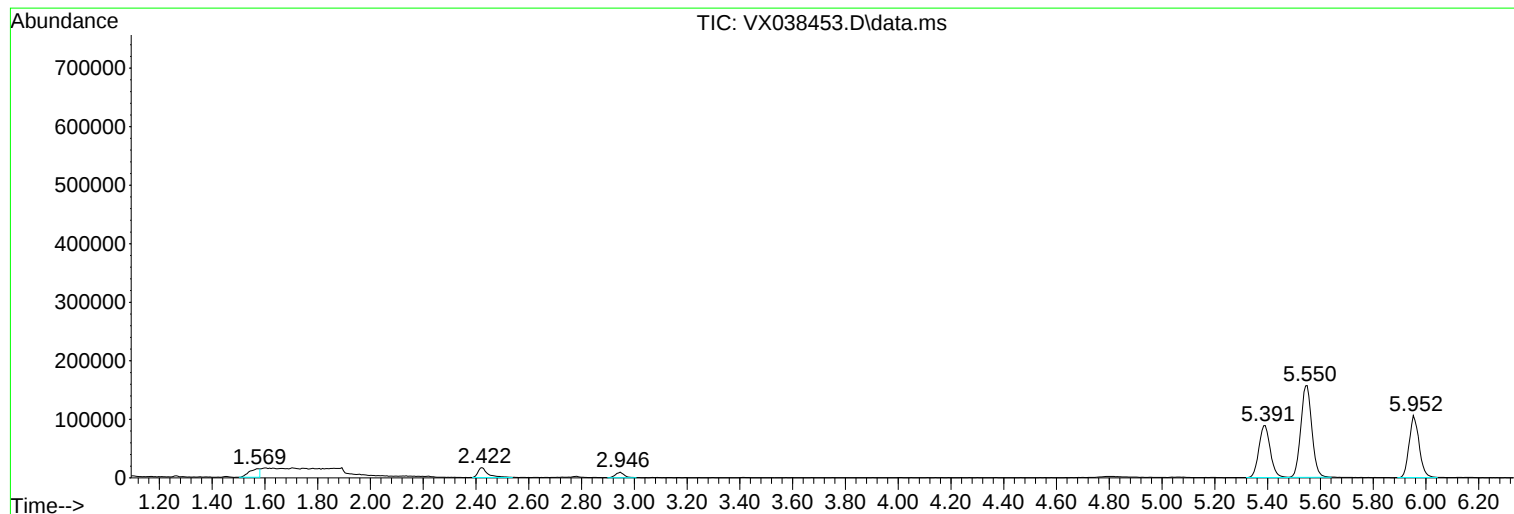

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102423\
Data File : VX038453.D
Acq On : 24 Oct 2023 13:54
Operator : JC/MD
Sample : 04936-07ME
Misc : 5.07g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1084ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102423\
Data File : VX038453.D
Acq On : 24 Oct 2023 13:54
Operator : JC/MD
Sample : 04936-07ME
Misc : 5.07g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1084ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------