

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102425\
 Data File : VX048340.D
 Acq On : 24 Oct 2025 09:48
 Operator : JC/MD
 Sample : VX1024WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1024WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M

Title : SW846 8260

Signal : TIC: VX048340.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	73	84	85	rBV3	7945	23672	4.48%	0.798%
2	2.386	207	213	219	rBV	13773	25455	4.82%	0.858%
3	2.459	219	225	242	rVB	14752	37066	7.02%	1.249%
4	5.367	691	702	719	rBV2	45859	154358	29.23%	5.202%
5	5.531	719	729	750	rVB2	87307	281722	53.34%	9.494%
6	5.934	783	795	823	rBV	56930	178943	33.88%	6.030%
7	6.738	916	927	945	rBV	156914	425627	80.59%	14.343%
8	8.628	1228	1237	1255	rBV	286200	505891	95.79%	17.048%
9	10.037	1462	1468	1485	rBV	354043	528140	100.00%	17.798%
10	11.061	1631	1636	1647	rBV	246099	337695	63.94%	11.380%
11	12.006	1785	1791	1801	rBV	343298	468901	88.78%	15.801%




Sum of corrected areas: 2967470

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102425\
Data File : VX048340.D
Acq On : 24 Oct 2025 09:48
Operator : JC/MD
Sample : VX1024WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1024WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

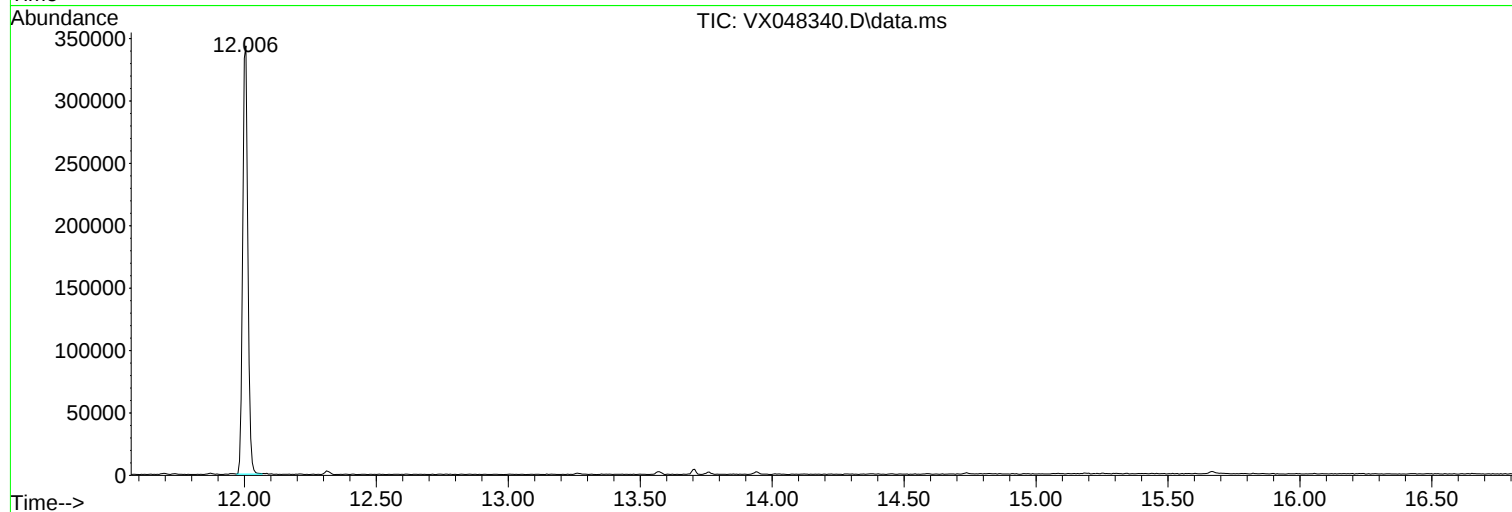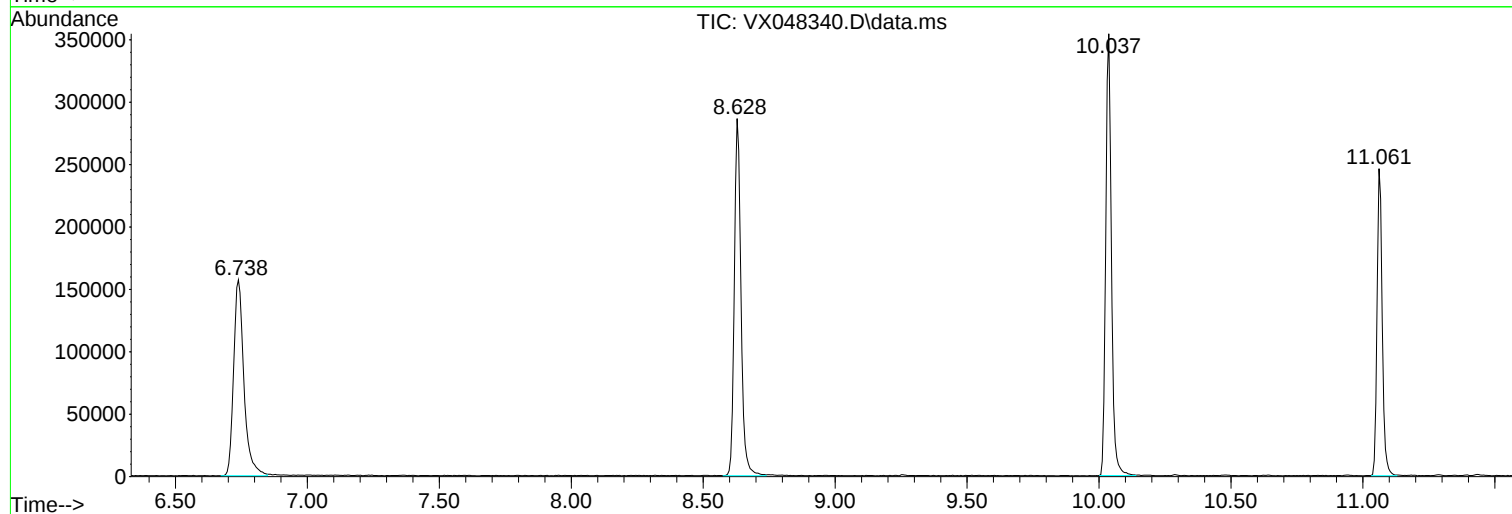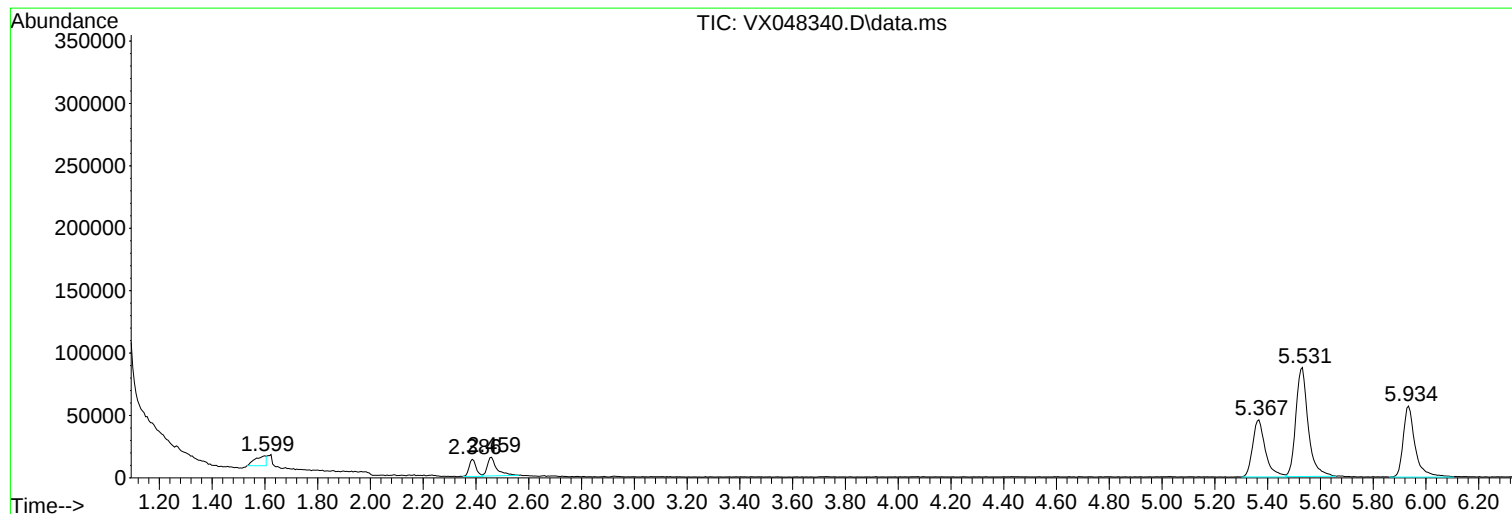

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102425\
Data File : VX048340.D
Acq On : 24 Oct 2025 09:48
Operator : JC/MD
Sample : VX1024WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1024WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102425\
Data File : VX048340.D
Acq On : 24 Oct 2025 09:48
Operator : JC/MD
Sample : VX1024WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1024WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc