

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102519\
 Data File : VX013206.D
 Acq On : 24 Oct 2019 12:50
 Operator : JC/SP
 Sample : K5531-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-MW203D1-GW-20191022

Quant Time: Oct 25 01:19:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 24 03:56:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	79507	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	119420	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	120389	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	75751	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.05	65	88934	53.48	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.96%	
35) Dibromofluoromethane	5.48	113	68023	51.08	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.16%	
50) Toluene-d8	8.71	98	246585	49.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.92%	
62) 4-Bromofluorobenzene	11.14	95	91894	47.04	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.08%	

Target Compounds


					Qvalue	
3) Chloromethane	1.32	50	963	1.692	ug/l	100
5) Bromomethane	1.65	94	214	0.280	ug/l #	38
6) Chloroethane	1.72	64	546	Below Cal	#	43
10) Methyl Iodide	2.50	142	257	3.675	ug/l #	88
11) Tert butyl alcohol	3.00	59	586	0.564	ug/l #	72
12) 1,1-Dichloroethene	2.37	96	7993	5.902	ug/l	95
16) Acetone	2.43	43	1661	2.120	ug/l	100
18) Methyl Acetate	2.59	43	7444	5.236	ug/l #	49
20) Methylene Chloride	2.85	84	337	0.517	ug/l #	67
21) trans-1,2-Dichloroethene	3.16	96	74	0.528	ug/l #	45
24) 1,1-Dichloroethane	3.69	63	48227	18.806	ug/l	97
27) cis-1,2-Dichloroethene	4.59	96	2850	1.718	ug/l	82
30) Chloroform	5.19	83	2536	0.929	ug/l #	74
31) Cyclohexane	5.65	56	1519	0.706	ug/l #	1
32) 1,1,1-Trichloroethane	5.48	97	6201	2.554	ug/l	97
36) 1,1-Dichloropropene	5.65	75	6075	2.967	ug/l #	51
38) Carbon Tetrachloride	5.65	117	8937	4.049	ug/l #	14
44) Trichloroethene	7.21	130	10209	5.997	ug/l	95
49) 1,4-Dioxane	7.75	88	227	5.462	ug/l #	86
51) 4-Methyl-2-Pentanone	8.71	43	988	0.491	ug/l #	1
60) Dibromochloromethane	9.33	129	1570	0.953	ug/l #	11
64) Tetrachloroethene	9.33	164	1652	Below Cal		93
76) 1,2,3-Trichloropropane	11.13	75	46025	25.209	ug/l #	38
81) trans-1,4-Dichloro-2-buten	11.13	75	46025	69.273	ug/l #	10


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102519\
Data File : VX013206.D
Acq On : 24 Oct 2019 12:50
Operator : JC/SP
Sample : K5531-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW203D1-GW-20191022

Quant Time: Oct 25 01:19:20 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 24 03:56:38 2019
Response via : Initial Calibration




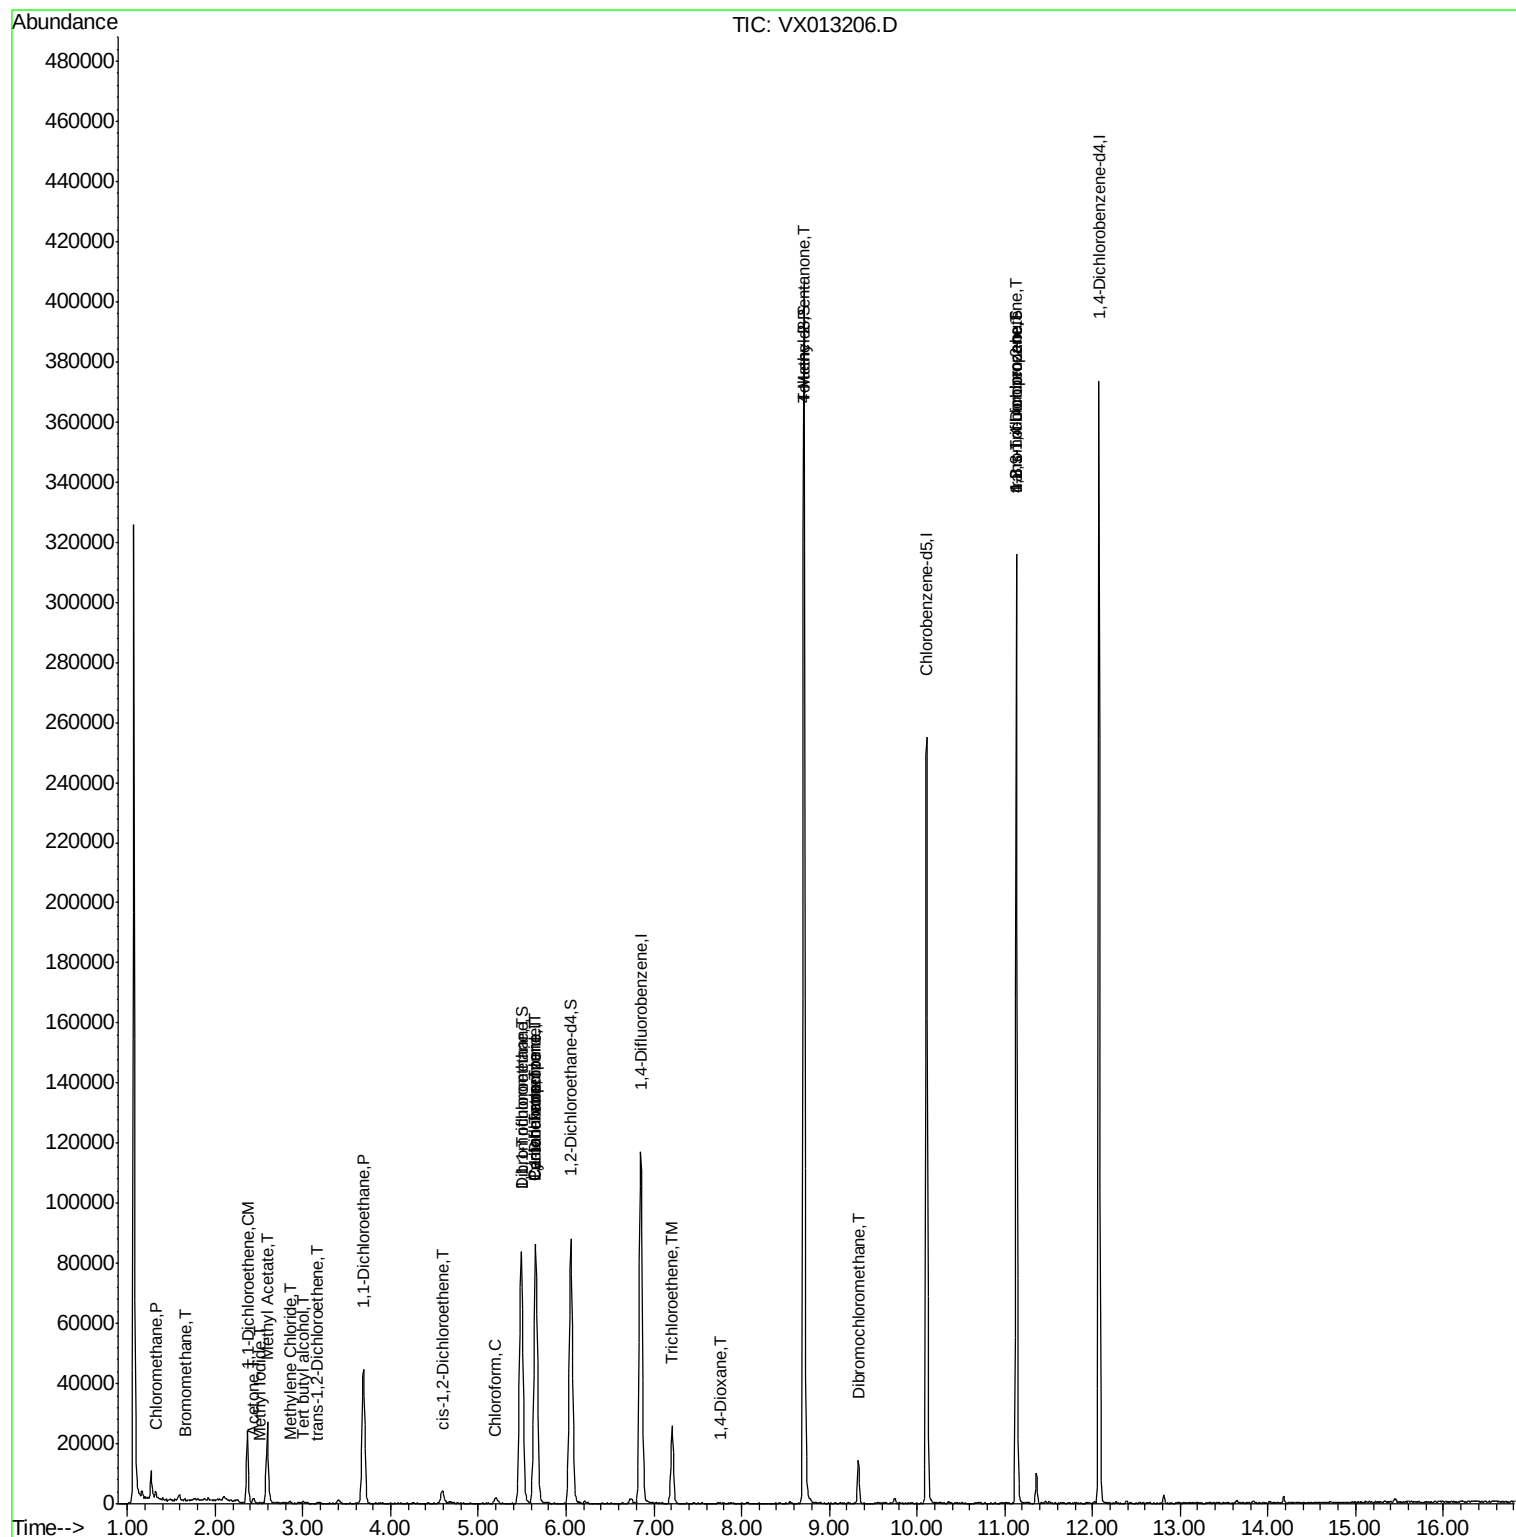


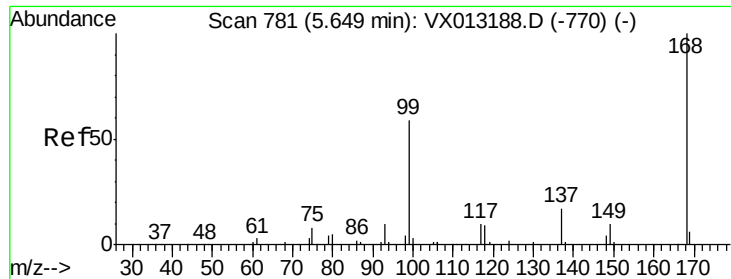

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.65 min Scan# 781
Delta R.T. 0.00 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW203D1-GW-20191022


Tot Ion:168 Resp: 79507
Ion Ratio Lower Upper
168 100
99 61.6 47.0 70.4

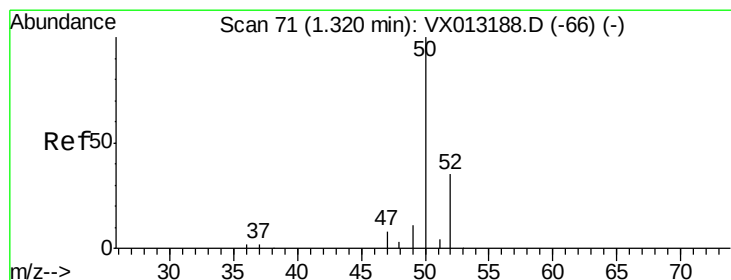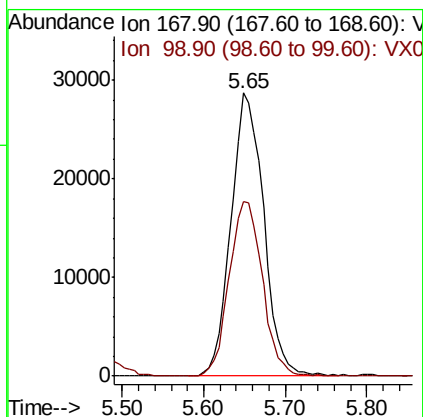

#3
Chloromethane
Concen: 1.692 ug/l
RT: 1.32 min Scan# 71
Delta R.T. 0.00 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50

Tgt Ion: 50 Resp: 963
Ion Ratio Lower Upper
50 100
52 34.6 27.8 41.6



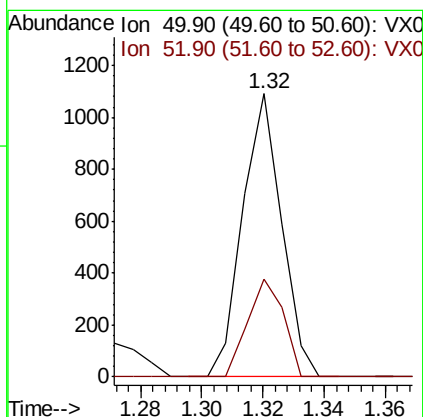



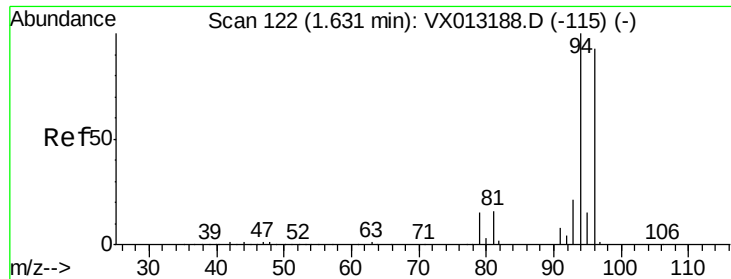

#5
Bromomethane
Concen: 0.280 ug/l
RT: 1.65 min Scan# 125
Delta R.T. 0.02 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW203D1-GW-20191022


Tot Ion: 94 Resp: 214
Ion Ratio Lower Upper
94 100
96 33.2 74.2 111.2#

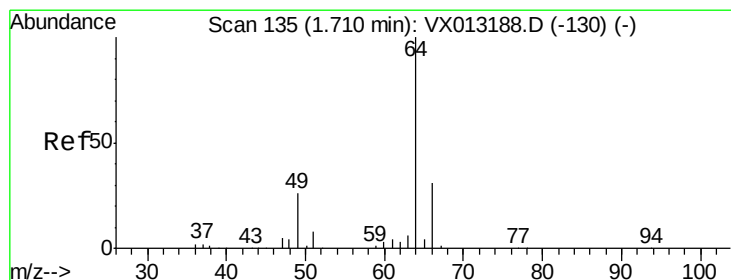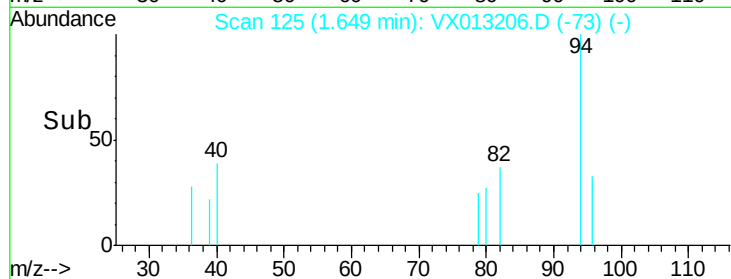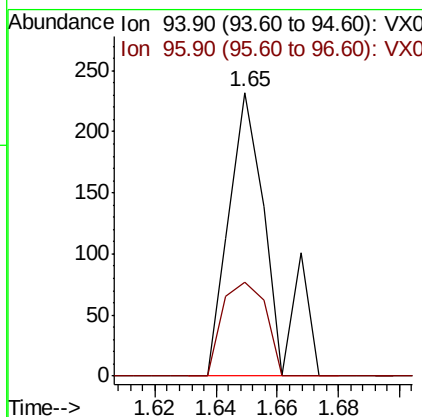

#6
Chloroethane
Concen: Below Cal
RT: 1.72 min Scan# 136
Delta R.T. 0.01 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50

Tgt Ion: 64 Resp: 546
Ion Ratio Lower Upper
64 100
66 0.0 25.0 37.6#


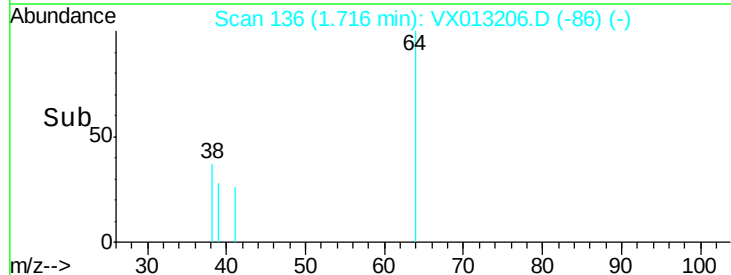
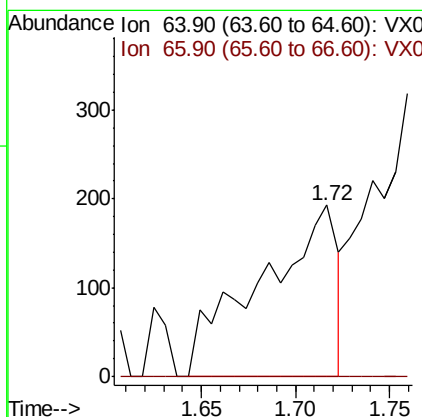



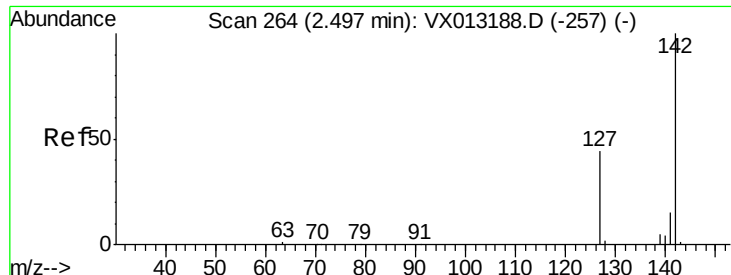

#10
Methvl Iodide
Concen: 3.675 ug/l
RT: 2.50 min Scan# 264
Delta R.T. 0.00 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW203D1-GW-20191022


Tot Ion:142 Resp: 257
Ion Ratio Lower Upper
142 100
127 41.6 35.6 53.4
141 0.0 11.6 17.4#

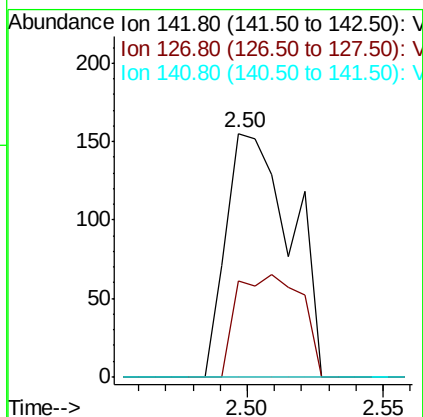

#11
Tert butyl alcohol
Concen: 0.564 ug/l
RT: 3.00 min Scan# 347
Delta R.T. -0.03 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50

Tgt Ion: 59 Resp: 586
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#



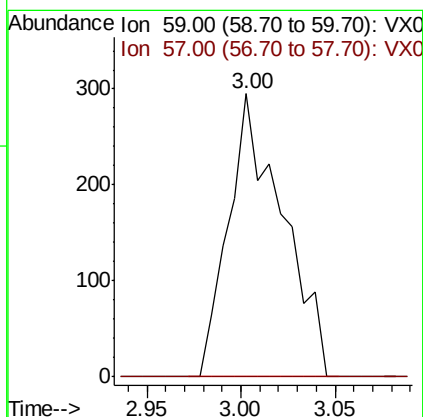





#12
 1,1-Dichloroethene
 Concen: 5.902 ug/l
 RT: 2.37 min Scan# 243
 Delta R.T. 0.01 min
 Lab File: VX013206.D
 Acq: 24 Oct 2019 12:50




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-MW203D1-GW-20191022


Tot Ion: 96 Resp: 7993
 Ion Ratio Lower Upper
 96 100
 61 148.4 123.8 185.8
 98 60.3 51.6 77.4

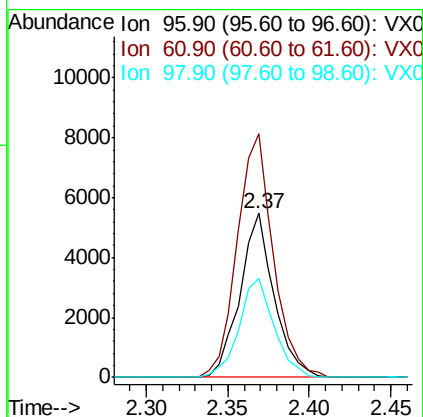

#16
 Acetone
 Concen: 2.120 ug/l
 RT: 2.43 min Scan# 253
 Delta R.T. -0.01 min
 Lab File: VX013206.D
 Acq: 24 Oct 2019 12:50

Tgt Ion: 43 Resp: 1661
 Ion Ratio Lower Upper
 43 100
 58 29.6 23.8 35.6



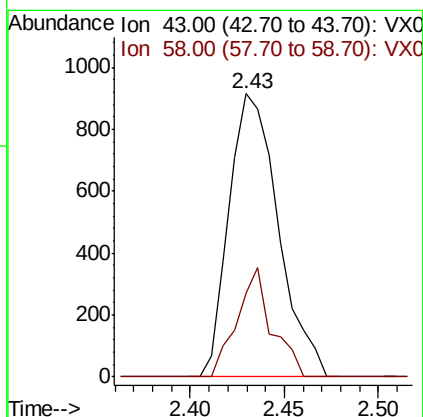





#18
Methvl Acetate
Concen: 5.236 ug/l
RT: 2.59 min Scan# 280
Delta R.T. -0.17 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW203D1-GW-20191022


Tot Ion: 43 Resp: 7444
Ion Ratio Lower Upper
43 100
74 0.0 20.9 31.3#

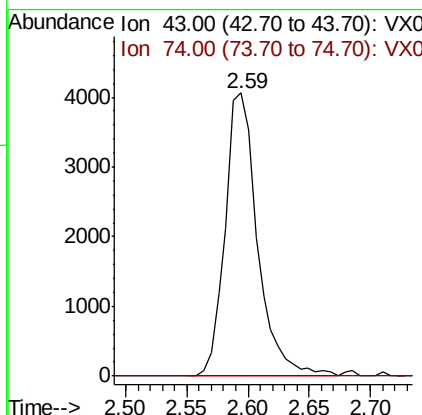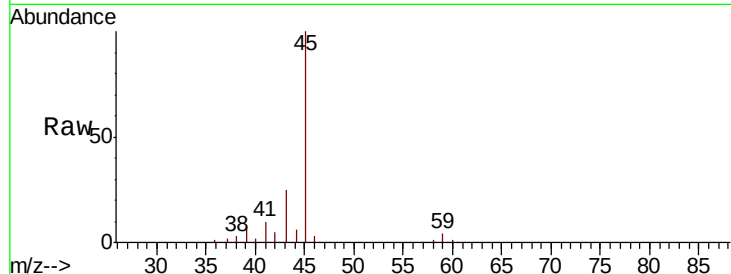

#20
Methylene Chloride
Concen: 0.517 ug/l
RT: 2.85 min Scan# 322
Delta R.T. 0.01 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50

Tgt Ion: 84 Resp: 337
Ion Ratio Lower Upper
84 100
49 74.4 89.2 133.8#
51 0.0 28.8 43.2#
86 53.1 51.2 76.8

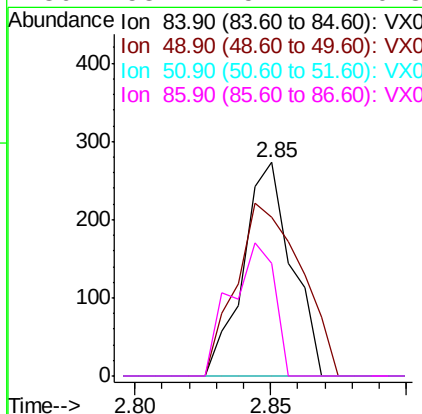

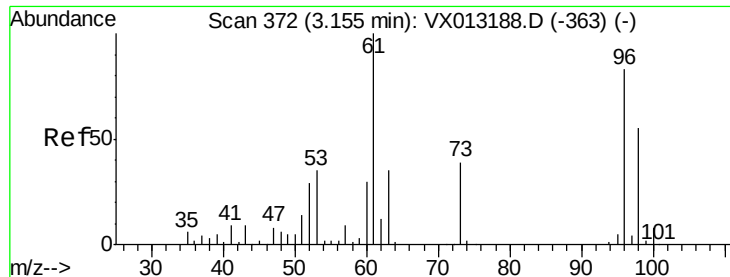

#21

trans-1,2-Dichloroethene

Concen: 0.528 ug/l

RT: 3.16 min Scan# 373

Delta R.T. 0.01 min

Lab File: VX013206.D

Acq: 24 Oct 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :

BP-TT-MW203D1-GW-20191022


Tot Ion: 96 Resp: 74

Ion Ratio Lower Upper

96 100

61 165.3 96.9 145.3#




98 0.0 53.0 79.4#

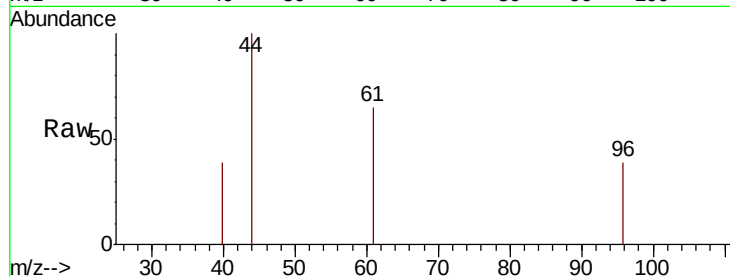

Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

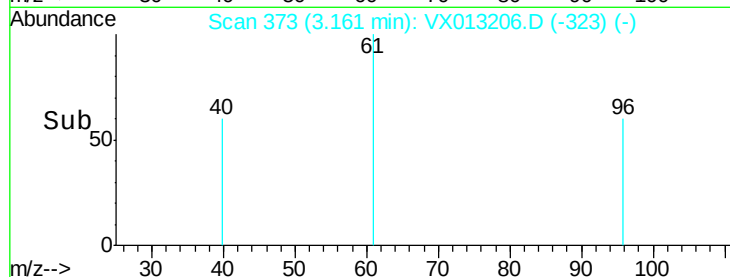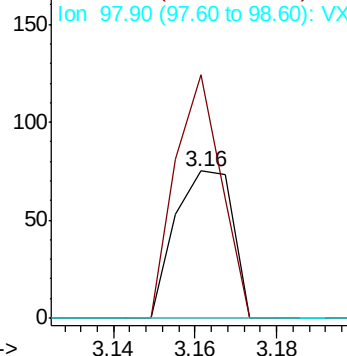

#24

1,1-Dichloroethane

Concen: 18.806 ug/l

RT: 3.69 min Scan# 460

Delta R.T. 0.01 min

Lab File: VX013206.D

Acq: 24 Oct 2019 12:50


Tgt Ion: 63 Resp: 48227

Ion Ratio Lower Upper

63 100

98 8.7 3.8 11.2



100 5.3 2.2 6.6




Abundance Ion 62.90 (62.60 to 63.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

Ion 99.90 (99.60 to 100.60): VX0

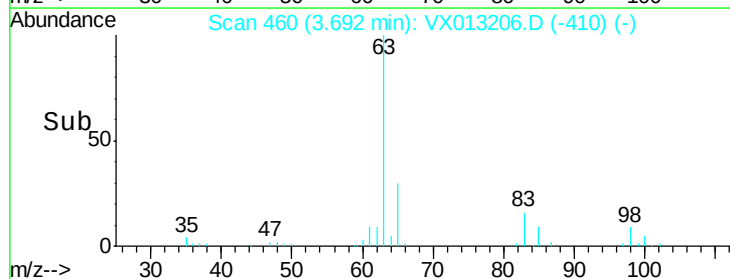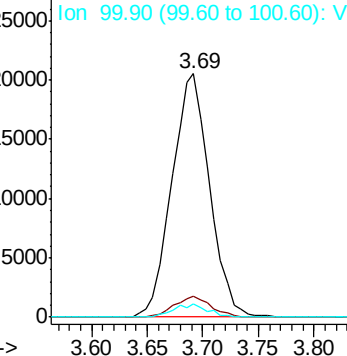


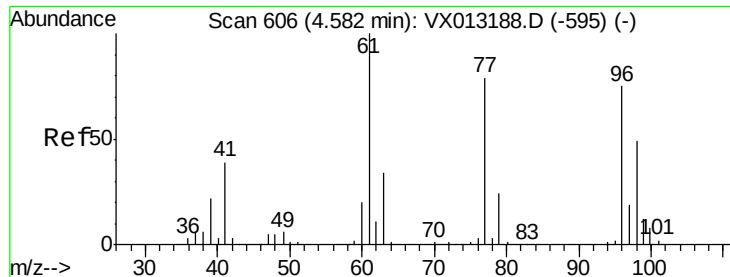




#27
 cis-1,2-Dichloroethene
 Concen: 1.718 ug/l
 RT: 4.59 min Scan# 607
 Delta R.T. 0.01 min
 Lab File: VX013206.D
 Acq: 24 Oct 2019 12:50

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-MW203D1-GW-20191022

Tot Ion: 96 Resp: 2850
 Ion Ratio Lower Upper
 96 100
 61 116.1 0.0 290.4
 98 59.3 0.0 130.4

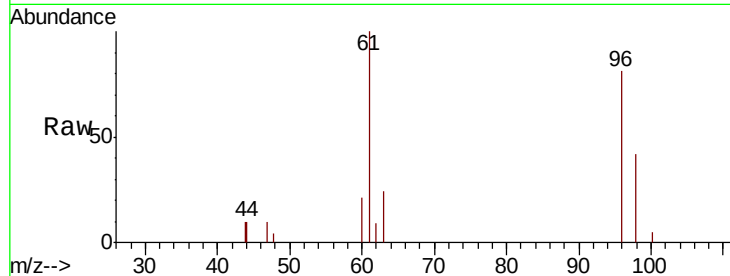


Abundance Ion 95.90 (95.60 to 96.60): VX0
 Ion 60.90 (60.60 to 61.60): VX0
 Ion 97.90 (97.60 to 98.60): VX0

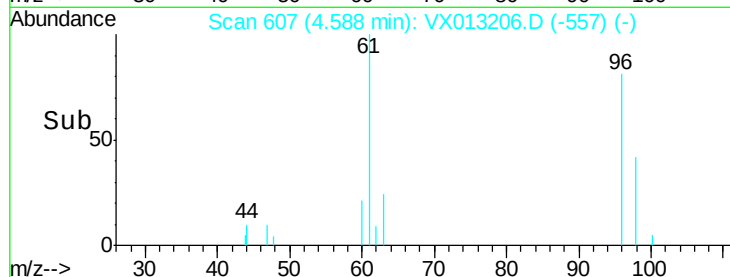
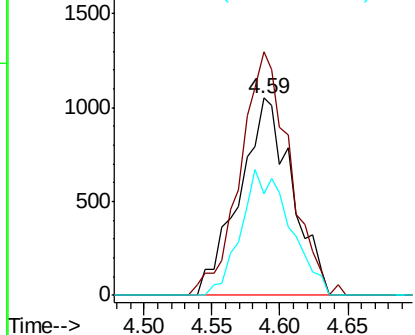



#30
 Chloroform
 Concen: 0.929 ug/l
 RT: 5.19 min Scan# 705
 Delta R.T. -0.01 min
 Lab File: VX013206.D
 Acq: 24 Oct 2019 12:50

Tgt Ion: 83 Resp: 2536
 Ion Ratio Lower Upper
 83 100
 85 42.5 50.1 75.1#



Abundance Ion 82.90 (82.60 to 83.60): VX0
 Ion 84.90 (84.60 to 85.60): VX0

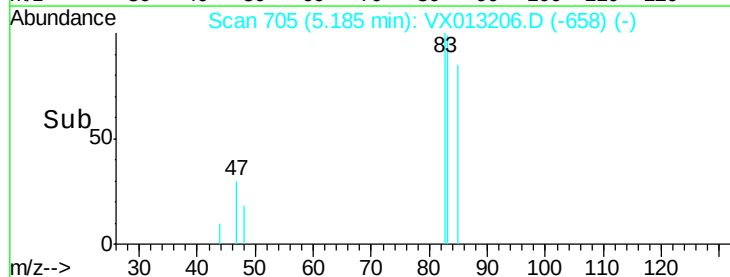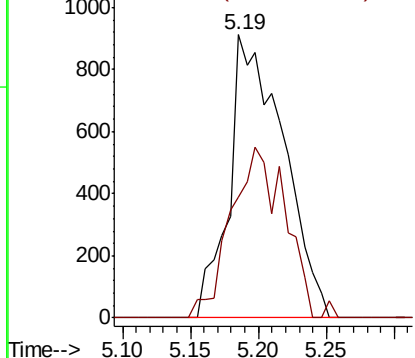


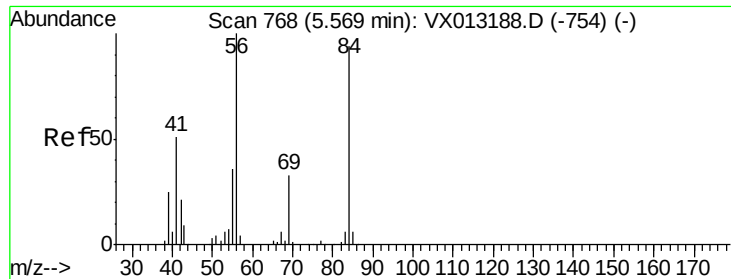




#31
Cyclohexane
Concen: 0.706 ug/l
RT: 5.65 min Scan# 781
Delta R.T. 0.08 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW203D1-GW-20191022

Tot Ion: 56 Resp: 1519
Ion Ratio Lower Upper
56 100
69 189.5 26.3 39.5#
84 156.7 73.8 110.6#




Abundance Ion 56.00 (55.70 to 56.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 84.00 (83.70 to 84.70): VX0

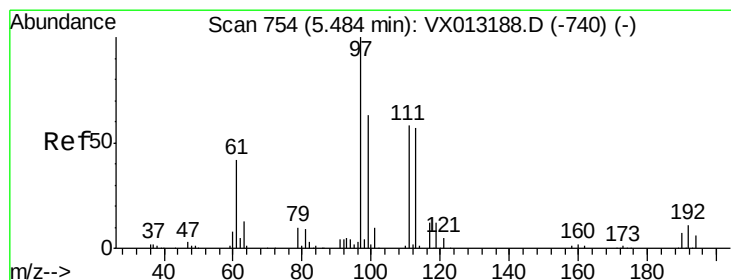
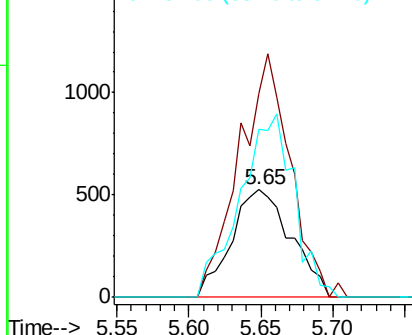



#32
1,1,1-Trichloroethane
Concen: 2.554 ug/l
RT: 5.48 min Scan# 754
Delta R.T. 0.00 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50

Tgt Ion: 97 Resp: 6201
Ion Ratio Lower Upper
97 100
99 65.3 50.8 76.2
61 44.1 32.8 49.2



Abundance Ion 96.90 (96.60 to 97.60): VX0
Ion 98.90 (98.60 to 99.60): VX0
Ion 60.90 (60.60 to 61.60): VX0

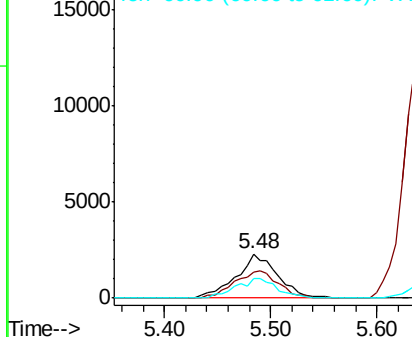

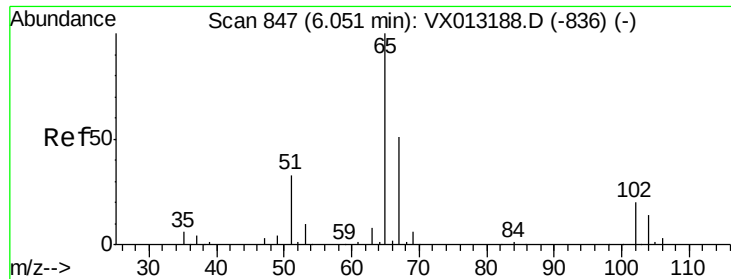

#33

1,2-Dichloroethane-d4

Concen: 53.480 ug/l

RT: 6.05 min Scan# 847

Delta R.T. 0.00 min

Lab File: VX013206.D

Acq: 24 Oct 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :


BP-TT-MW203D1-GW-20191022

Tot Ion: 65 Resp: 88934

Ion Ratio Lower Upper

65 100

67 50.6 0.0 102.6



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.05

40000

30000



20000

10000

0

Time-->

5.90 6.00 6.10 6.20

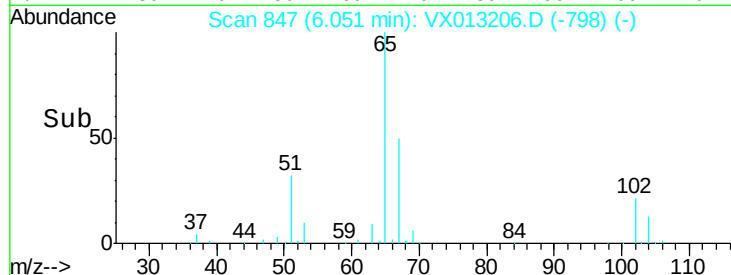

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. 0.00 min

Lab File: VX013206.D

Acq: 24 Oct 2019 12:50


Tgt Ion: 114 Resp: 119420

Ion Ratio Lower Upper

114 100

63 19.8 0.0 39.0

88 16.3 0.0 32.0



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

6.85

60000


40000


20000

0

Time-->

6.80 6.90 7.00





#35

Dibromofluoromethane

Concen: 51.080 ug/l

RT: 5.48 min Scan# 754

Delta R.T. 0.00 min

Lab File: VX013206.D

Acq: 24 Oct 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :

BP-TT-MW203D1-GW-20191022


Tot Ion:113 Resp: 68023

Ion Ratio Lower Upper

113 100

111 103.0 80.3 120.5




192 20.3 15.9 23.9

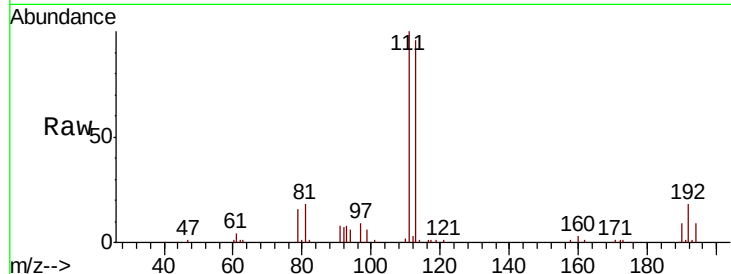

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

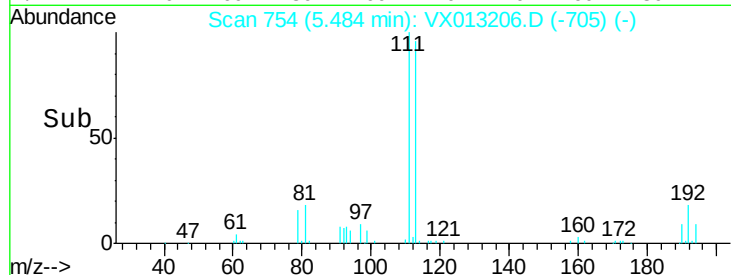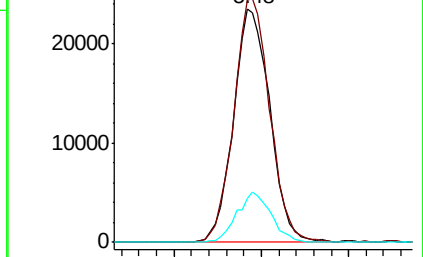

#36

1,1-Dichloropropene

Concen: 2.967 ug/l

RT: 5.65 min Scan# 781

Delta R.T. -0.14 min

Lab File: VX013206.D

Acq: 24 Oct 2019 12:50


Tgt Ion: 75 Resp: 6075

Ion Ratio Lower Upper

75 100

110 10.0 17.6 52.9#



77 0.0 24.7 37.1#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

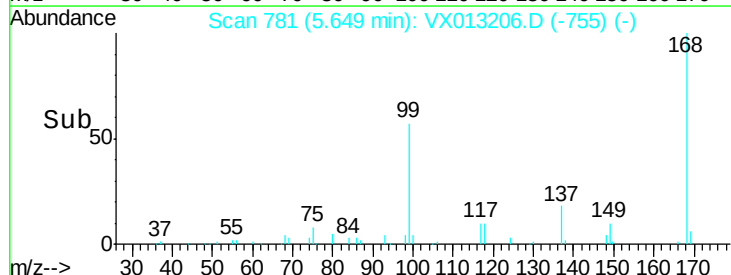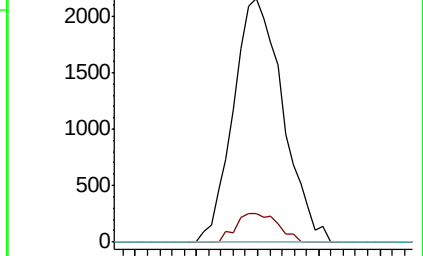

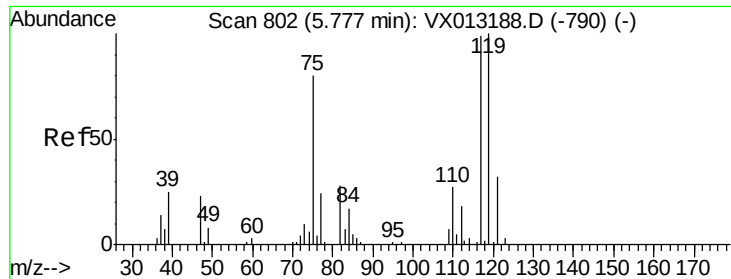

#38

Carbon Tetrachloride

Concen: 4.049 ug/l

RT: 5.65 min Scan# 781

Delta R.T. -0.13 min

Lab File: VX013206.D

Acq: 24 Oct 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :

BP-TT-MW203D1-GW-20191022


Tot Ion:117 Resp: 8937

Ion Ratio Lower Upper

117 100

119 4.3 80.1 120.1#




121 0.0 25.5 38.3#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

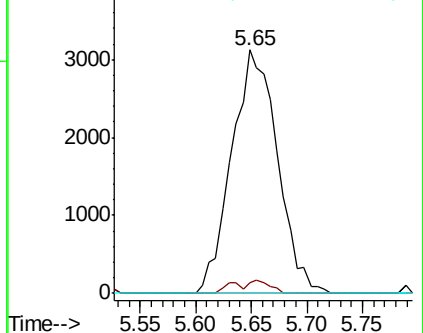

#44

Trichloroethene

Concen: 5.997 ug/l

RT: 7.21 min Scan# 1037

Delta R.T. 0.01 min

Lab File: VX013206.D


Acq: 24 Oct 2019 12:50

Tgt Ion:130 Resp: 10209

Ion Ratio Lower Upper



130 100


95 101.5 0.0 193.6



Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0




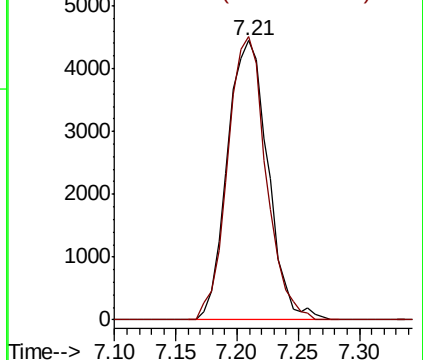


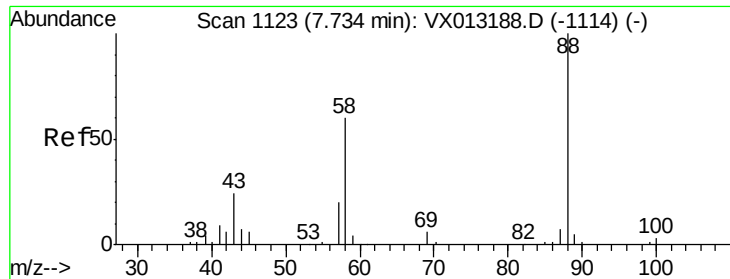

#49
1,4-Dioxane
Concen: 5.462 ug/l
RT: 7.75 min Scan# 1126
Delta R.T. 0.02 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW203D1-GW-20191022


Tot Ion: 88 Resp: 227
Ion Ratio Lower Upper
88 100
43 11.0 24.5 36.7#
58 64.8 54.1 81.1

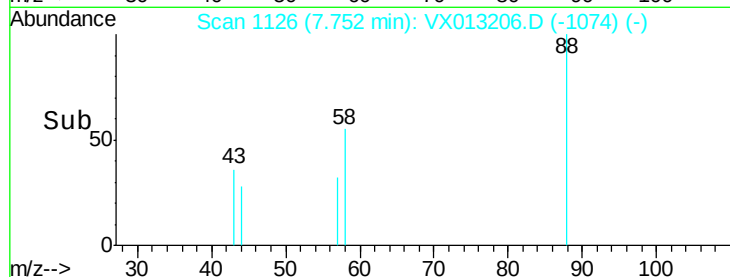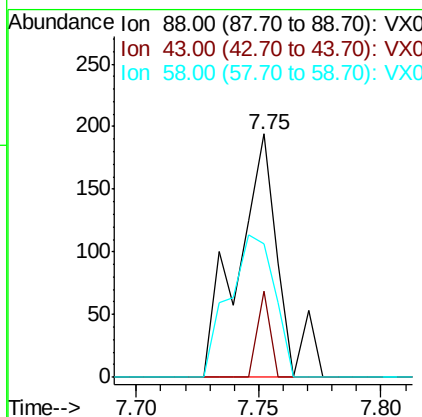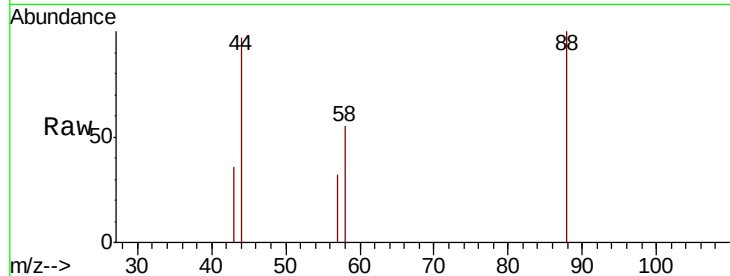

#50
Toluene-d8
Concen: 49.965 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. 0.00 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50

Tgt Ion: 98 Resp: 246585
Ion Ratio Lower Upper
98 100
100 66.4 53.3 79.9

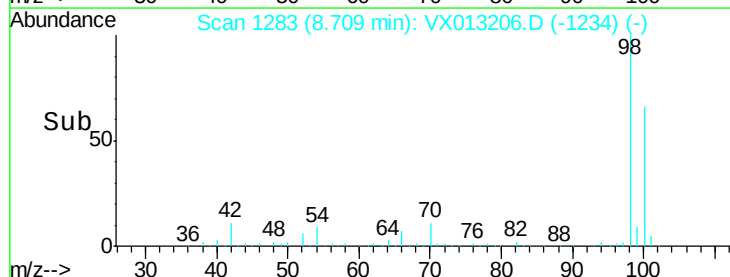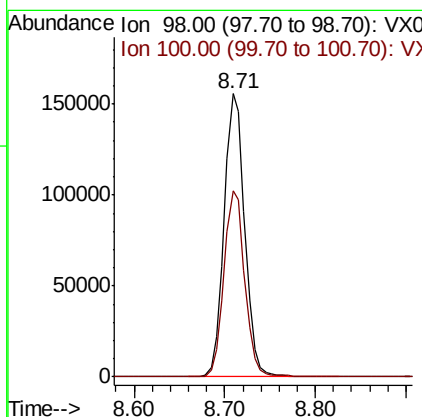

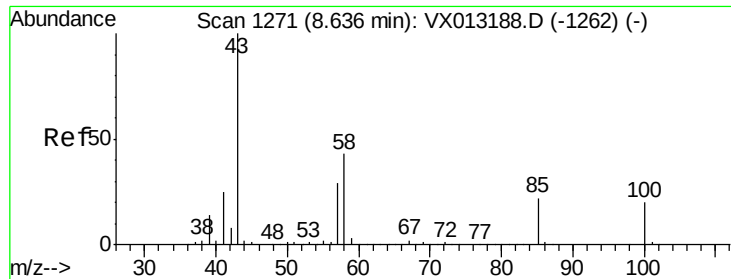

#51

4-Methyl-2-Pentanone

Concen: 0.491 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. 0.07 min

Lab File: VX013206.D

Acq: 24 Oct 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :


BP-TT-MW203D1-GW-20191022

Tot Ion: 43 Resp: 988

Ion Ratio Lower Upper




43 100

58 211.9 33.9 50.9#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

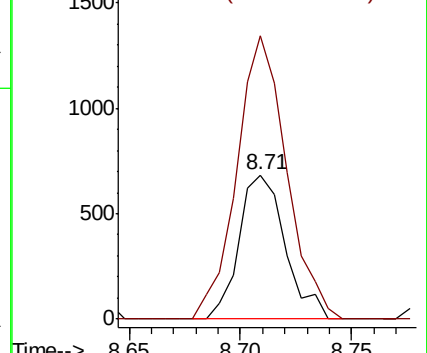

#60

Dibromochloromethane

Concen: 0.953 ug/l

RT: 9.33 min Scan# 1385

Delta R.T. -0.24 min

Lab File: VX013206.D


Acq: 24 Oct 2019 12:50

Tgt Ion:129 Resp: 1570

Ion Ratio Lower Upper



129 100


127 0.0 38.2 114.6#



Abundance Ion 128.80 (128.50 to 129.50): V

Ion 126.80 (126.50 to 127.50): V

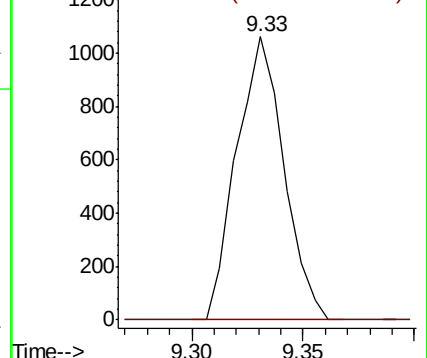

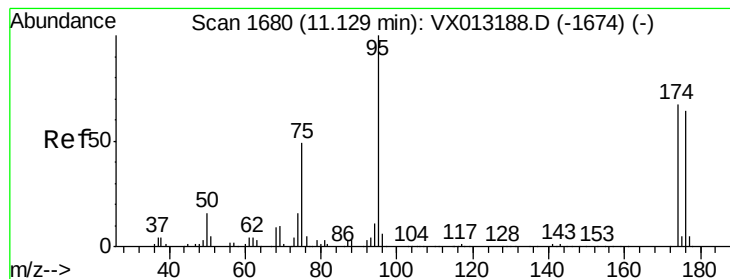

#62

4-Bromofluorobenzene

Concen: 47.044 ug/l

RT: 11.14 min Scan# 1681

Delta R.T. 0.01 min

Lab File: VX013206.D

Acq: 24 Oct 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :

BP-TT-MW203D1-GW-20191022


Tot Ion: 95 Resp: 91894

Ion Ratio Lower Upper

95 100

174 76.4 0.0 152.4




176 74.3 0.0 146.0



Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

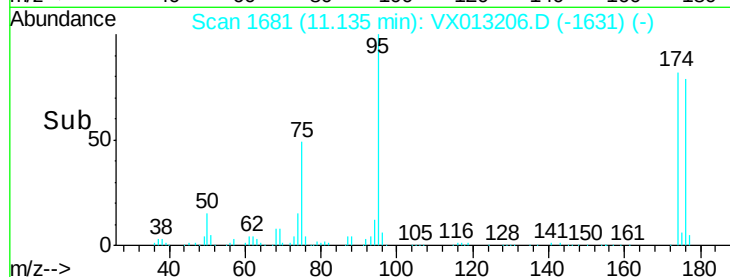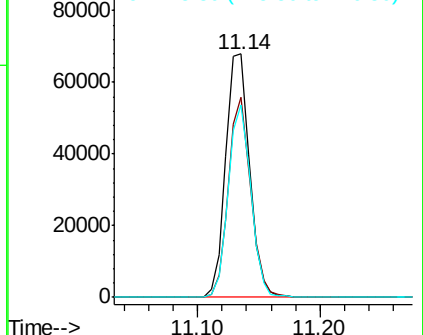

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1513

Delta R.T. 0.00 min

Lab File: VX013206.D

Acq: 24 Oct 2019 12:50


Tgt Ion: 117 Resp: 120389

Ion Ratio Lower Upper

117 100

82 55.0 46.5 69.7



119 33.9 25.2 37.8




Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V



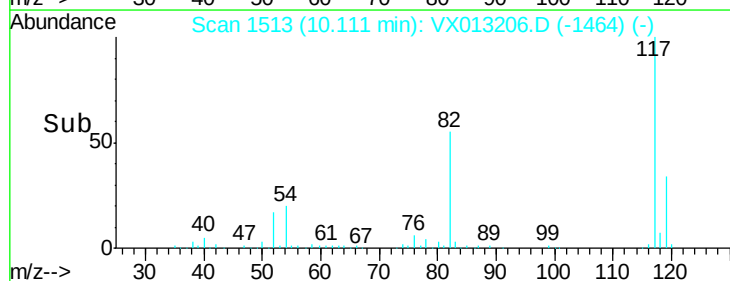
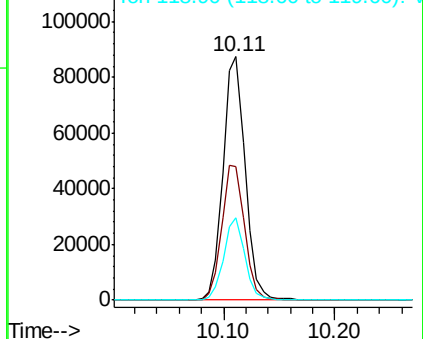




#64
Tetrachloroethene
Concen: Below Cal
RT: 9.33 min Scan# 1385
Delta R.T. 0.00 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW203D1-GW-20191022


Tot Ion	Ratio	Lower	Upper
164	100		
166	117.4	102.2	153.4
129	99.3	79.8	119.8
131	83.7	75.3	112.9

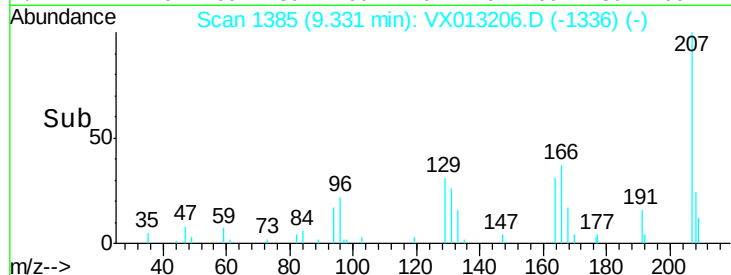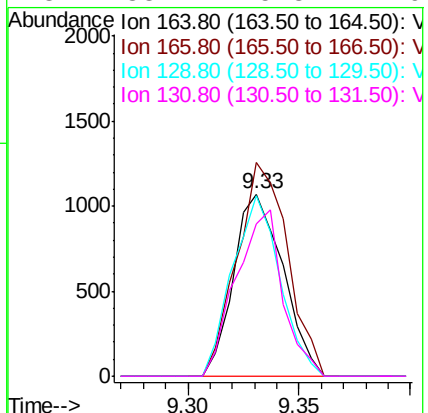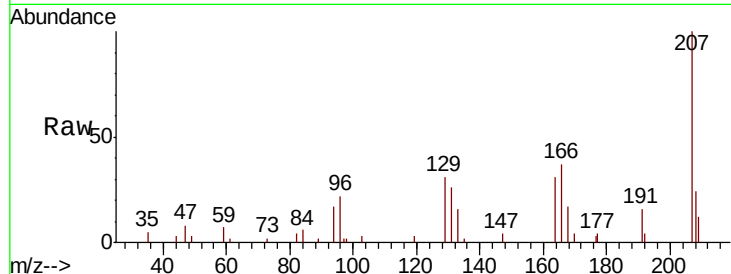

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. 0.00 min
Lab File: VX013206.D
Acq: 24 Oct 2019 12:50

Tgt Ion	Ratio	Lower	Upper
152	100		
115	65.4	46.6	139.8
150	156.2	0.0	354.0

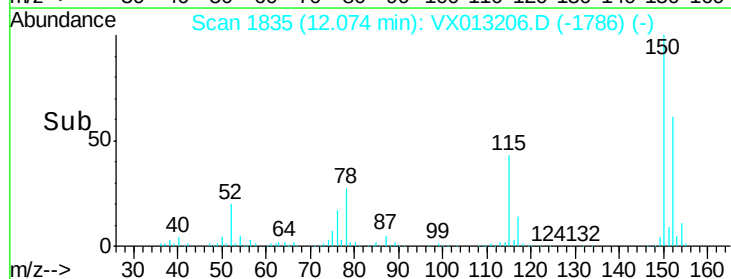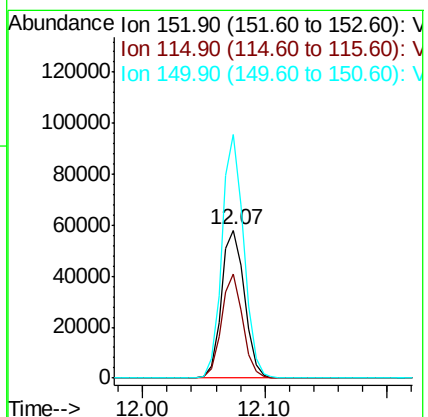

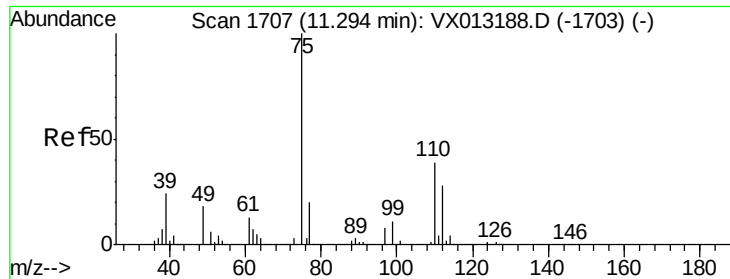

#76

1,2,3-Trichloropropane

Concen: 25.209 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.16 min

Lab File: VX013206.D

Acq: 24 Oct 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :


BP-TT-MW203D1-GW-20191022

Tot Ion: 75 Resp: 46025

Ion Ratio Lower Upper




75 100

77 0.9 19.1 57.5#

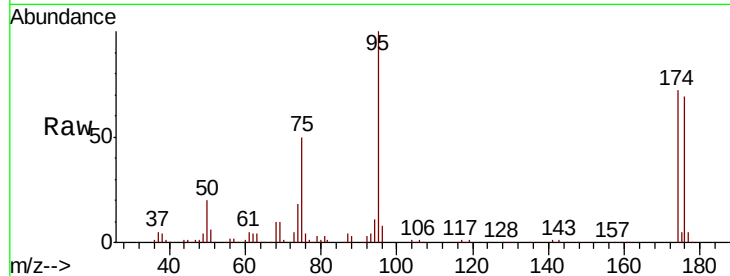

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

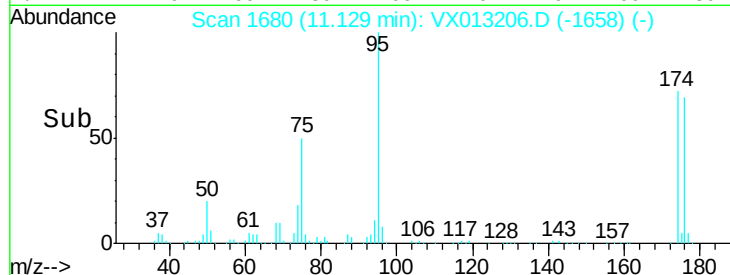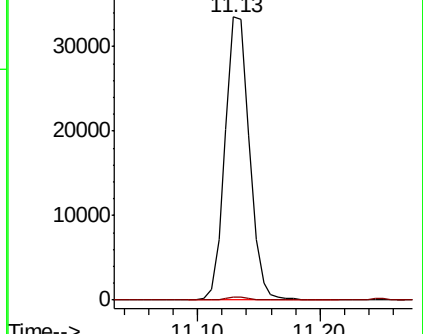

#81

trans-1,4-Dichloro-2-butene

Concen: 69.273 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. 0.06 min

Lab File: VX013206.D

Acq: 24 Oct 2019 12:50


Tgt Ion: 75 Resp: 46025

Ion Ratio Lower Upper

75 100

53 0.0 77.9 116.9#

89 0.0 37.3 55.9#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

