

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102519\
 Data File : VX013223.D
 Acq On : 25 Oct 2019 12:11
 Operator : JC/SP
 Sample : K5547-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	41	rBV	200294	262723	44.03%	8.960%
2	1.265	59	62	76	rVB	13434	20610	3.45%	0.703%
3	2.594	272	280	290	rBV	38149	68358	11.46%	2.331%
4	5.490	743	755	768	rBV2	69174	205227	34.40%	6.999%
5	5.655	771	782	796	rVV	78959	218304	36.59%	7.445%
6	6.051	836	847	866	rBV	82205	215300	36.08%	7.343%
7	6.850	966	978	990	rBV	108397	250507	41.98%	8.544%
8	8.709	1276	1283	1302	rBV	375717	596661	100.00%	20.350%
9	10.105	1507	1512	1526	rBV	222607	317871	53.27%	10.841%
10	11.129	1675	1680	1691	rBV	281517	378591	63.45%	12.912%
11	12.074	1829	1835	1848	rVB	303059	390436	65.44%	13.316%
12	14.178	2175	2180	2186	rBV	5671	7478	1.25%	0.255%


Sum of corrected areas: 2932066

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102519\
Data File : VX013223.D
Acq On : 25 Oct 2019 12:11
Operator : JC/SP
Sample : K5547-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

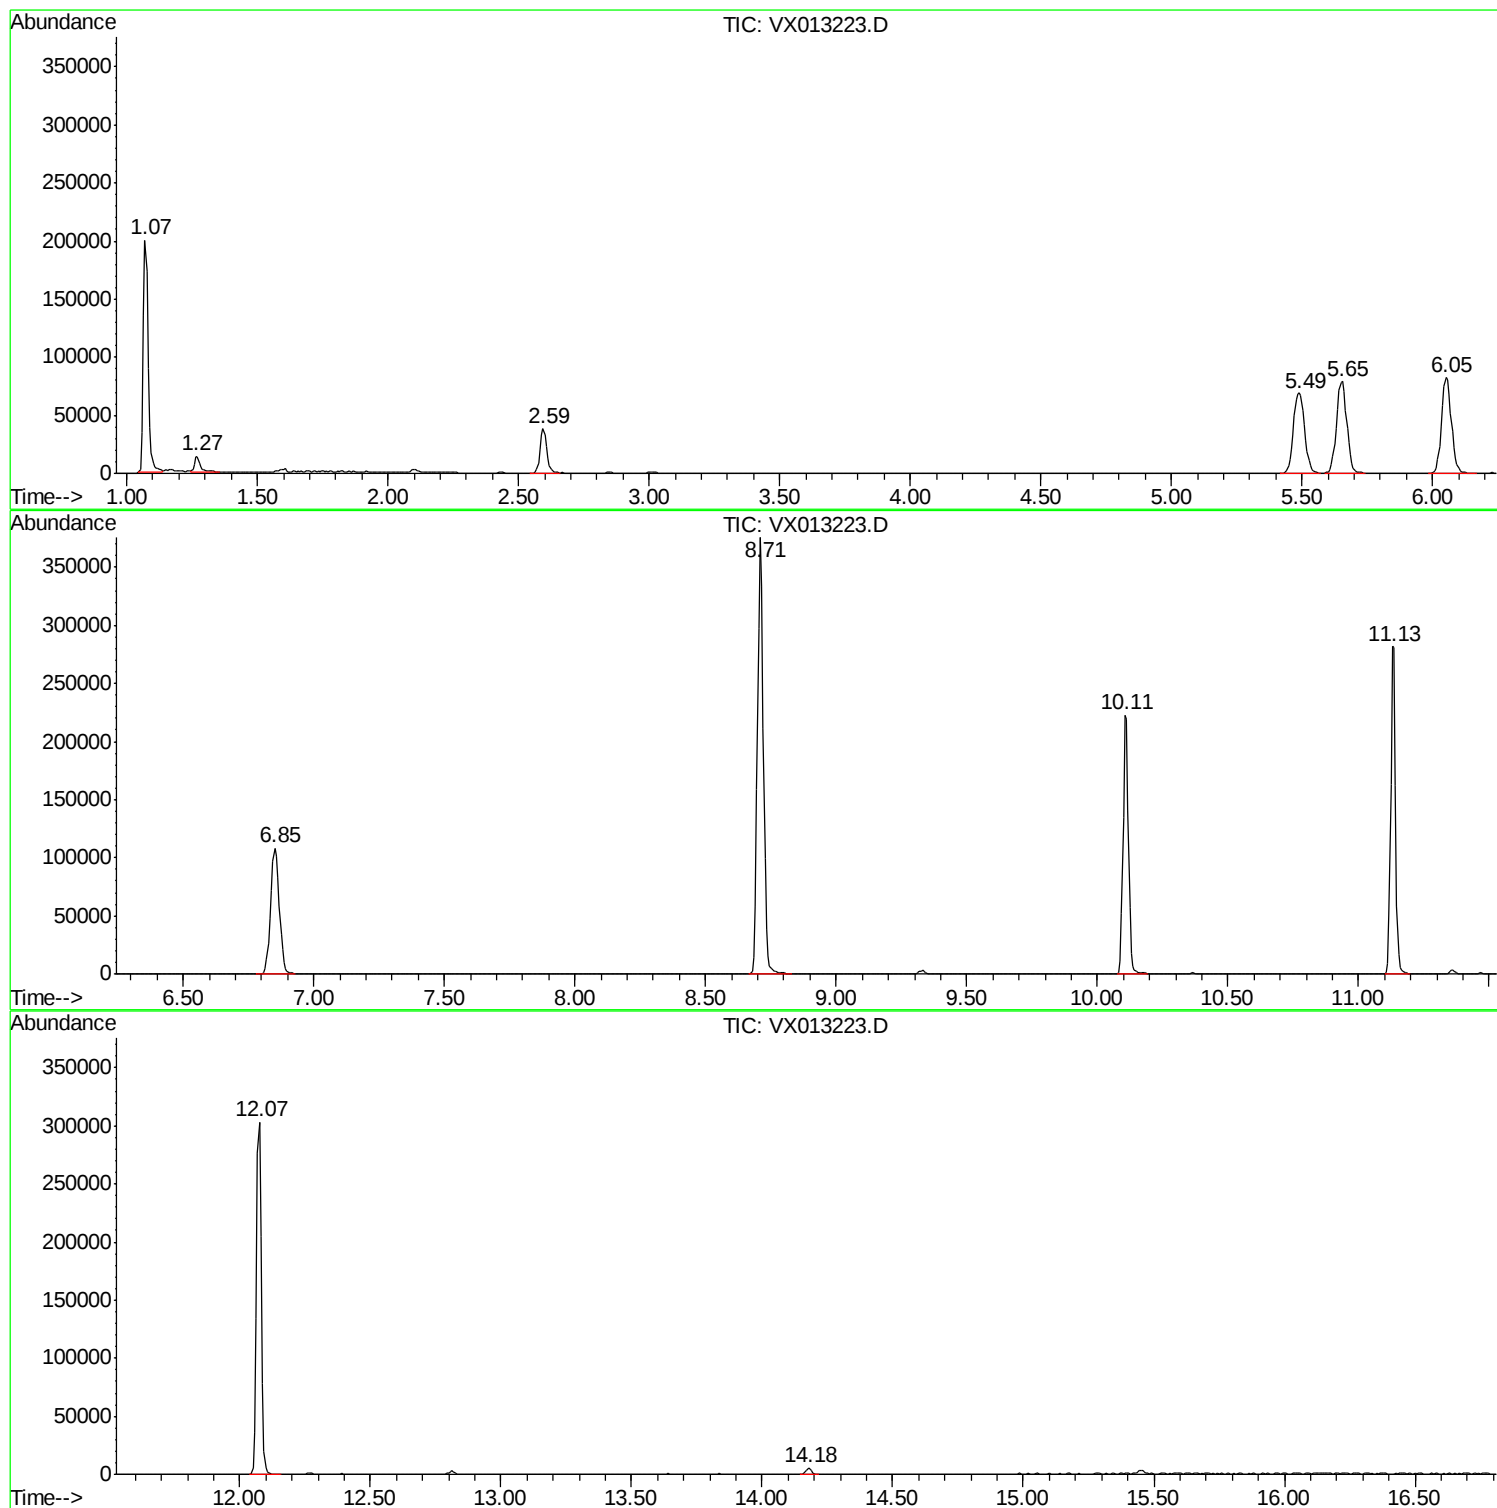

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102519\
Data File : VX013223.D
Acq On : 25 Oct 2019 12:11
Operator : JC/SP
Sample : K5547-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	15.66 ug/l	68358	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	90
2		Hvdrazine, ethyl-	60	C2H8N2	000624-80-6	40
3		Hvdrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4		Formamide	45	CH3NO	000075-12-7	5
5		Ethylamine	45	C2H7N	000075-04-7	5

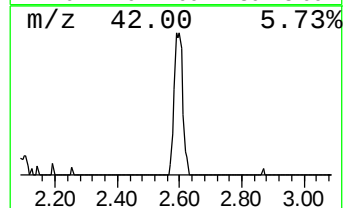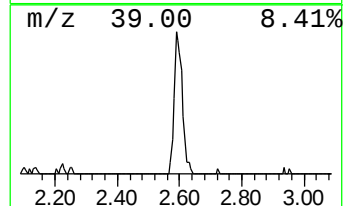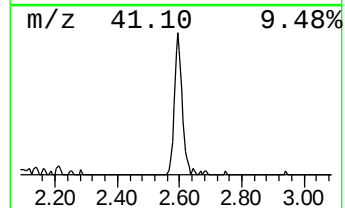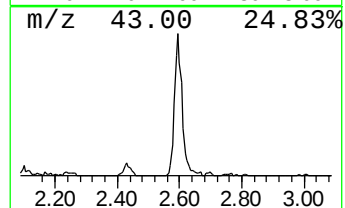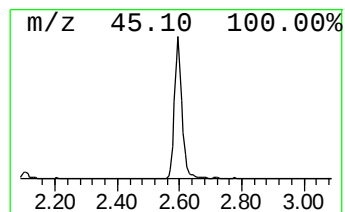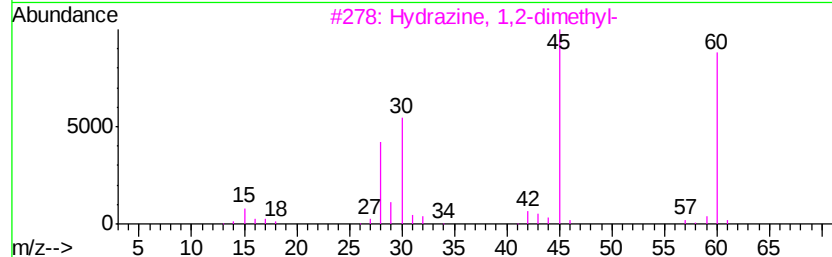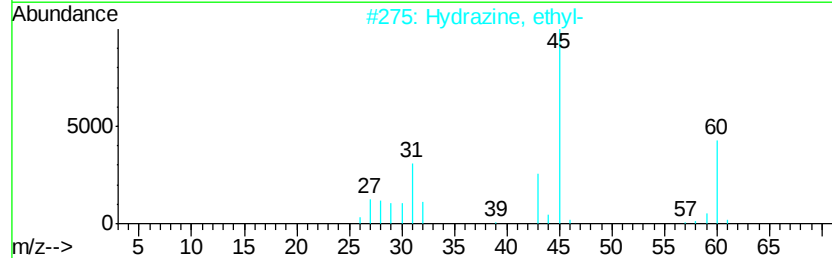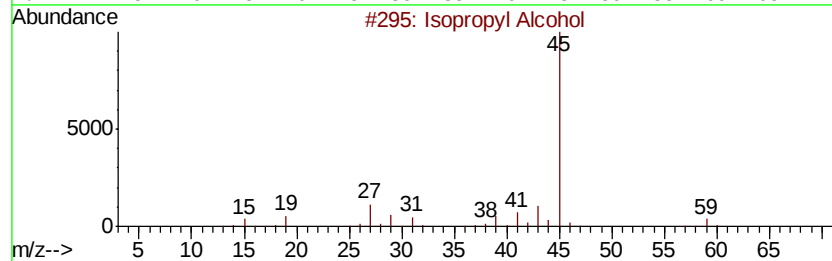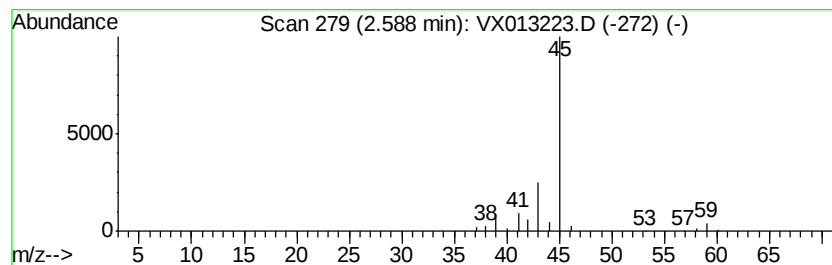

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX102519\
Data File : VX013223.D
Acq On : 25 Oct 2019 12:11
Operator : JC/SP
Sample : K5547-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	15.7	ug/l	68358	1	5.65	218304	50.0