


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX102519\
Data File : VX013199.D
Acq On : 24 Oct 2019 09:28
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Title : SW846 8260
Last Update : Thu Oct 24 03:56:38 2019

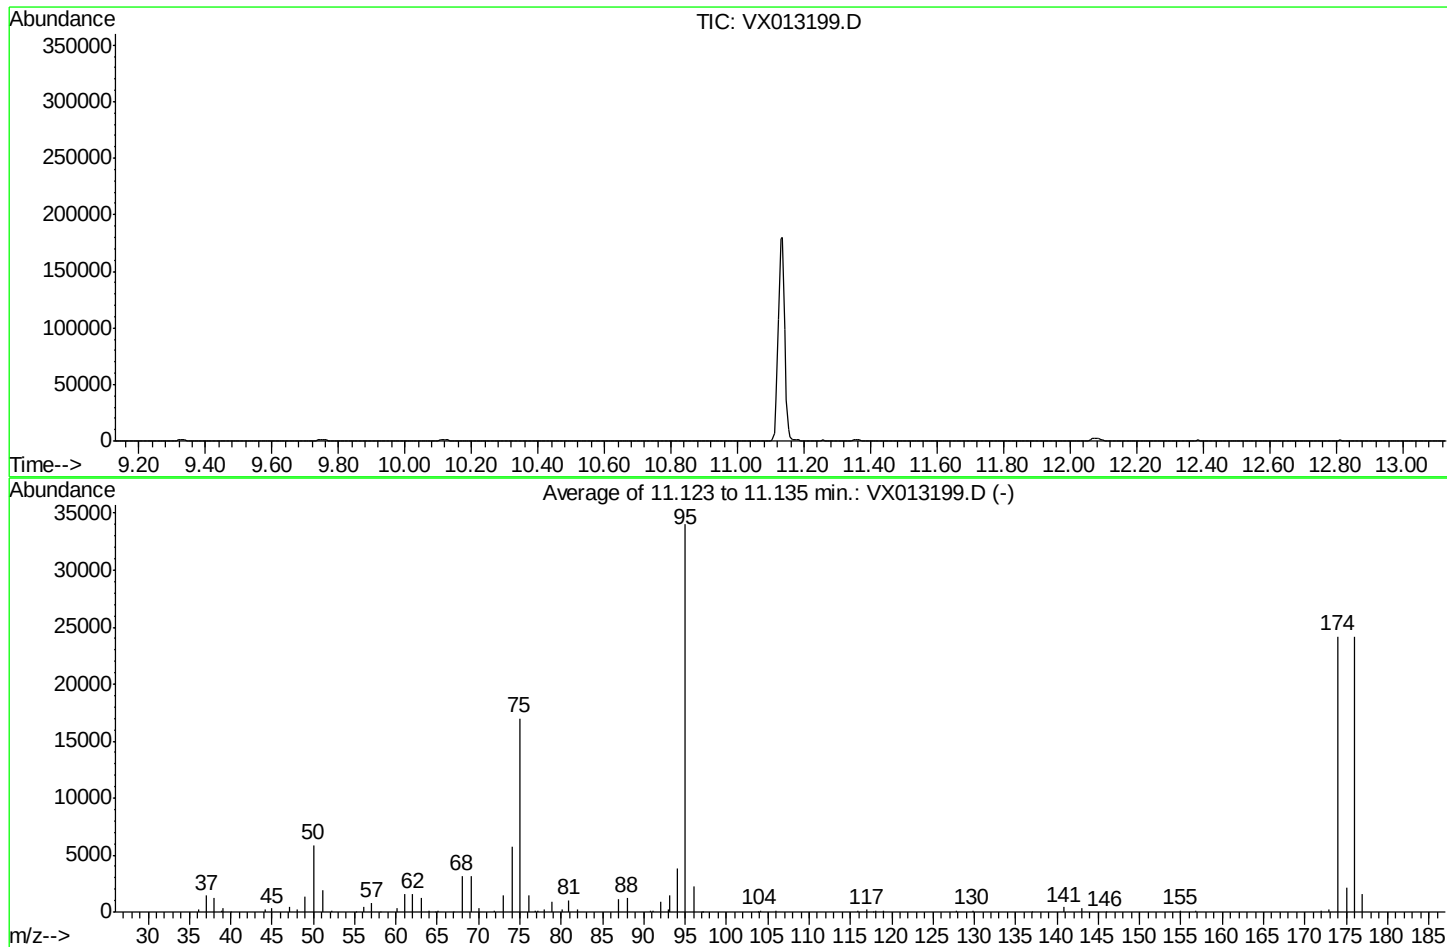

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	5868	PASS
75	95	30	60	49.9	16970	PASS
95	95	100	100	100.0	34026	PASS
96	95	5	9	6.5	2211	PASS
173	174	0.00	2	1.1	259	PASS
174	95	50	100	71.2	24212	PASS
175	174	5	9	8.7	2116	PASS
176	174	95	101	99.7	24140	PASS
177	176	5	9	6.7	1621	PASS