


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102519\  
Data File : VX013218.D  
Acq On : 25 Oct 2019 09:47  
Operator : JC/SP  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X102419W.M  
Title : SW846 8260  
Last Update : Thu Oct 24 03:56:38 2019

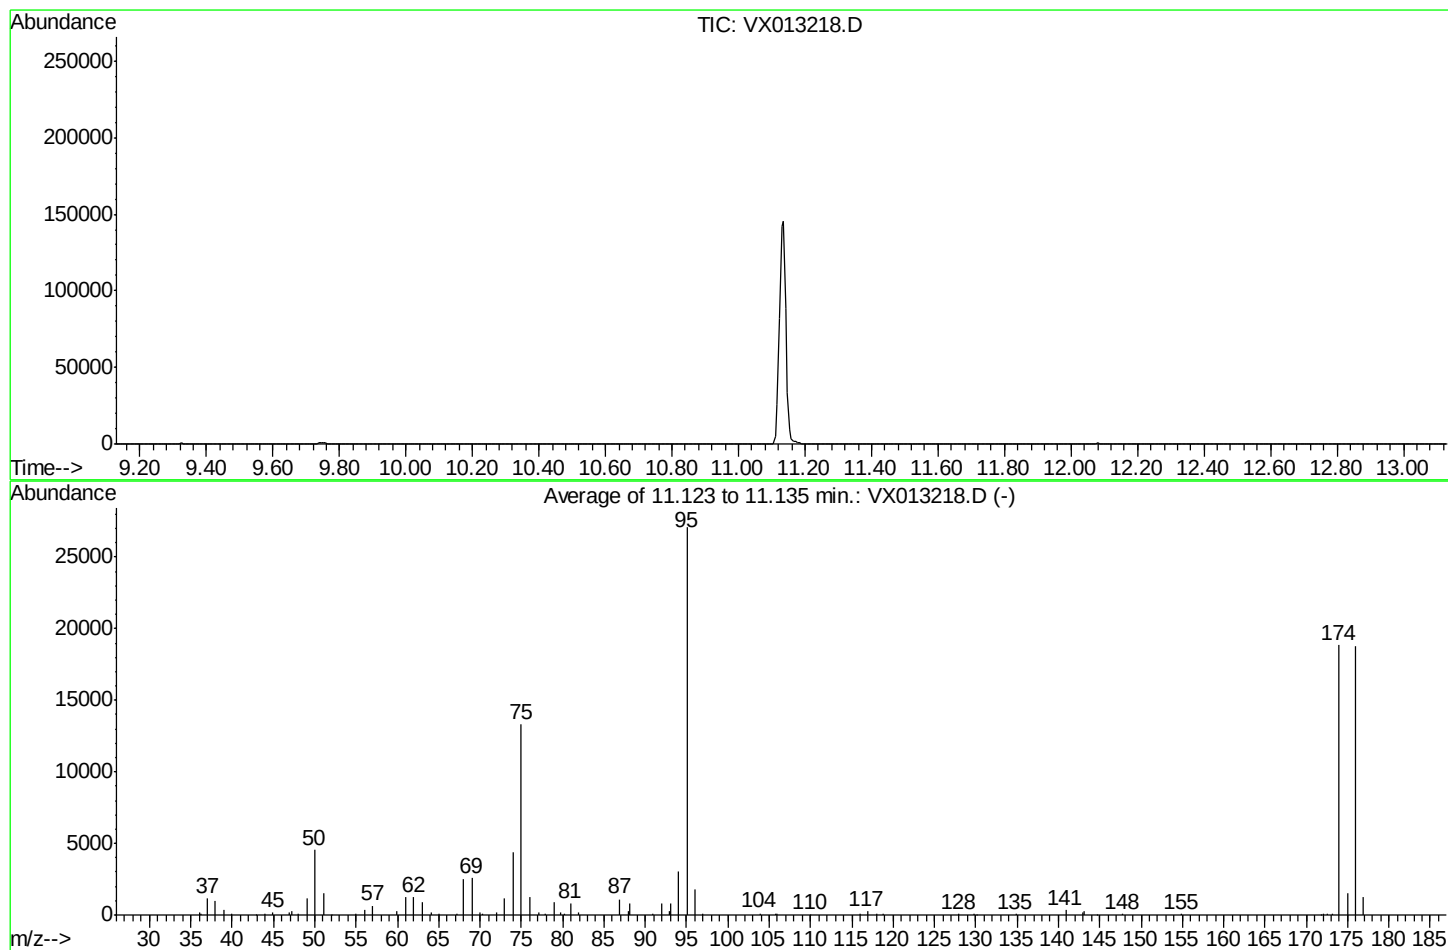

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.8      | 4556    | PASS             |
| 75          | 95           | 30           | 60           | 49.1      | 13301   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 27082   | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 1800    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.3       | 61      | PASS             |
| 174         | 95           | 50           | 100          | 69.6      | 18851   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 1503    | PASS             |
| 176         | 174          | 95           | 101          | 99.6      | 18778   | PASS             |
| 177         | 176          | 5            | 9            | 6.5       | 1216    | PASS             |