
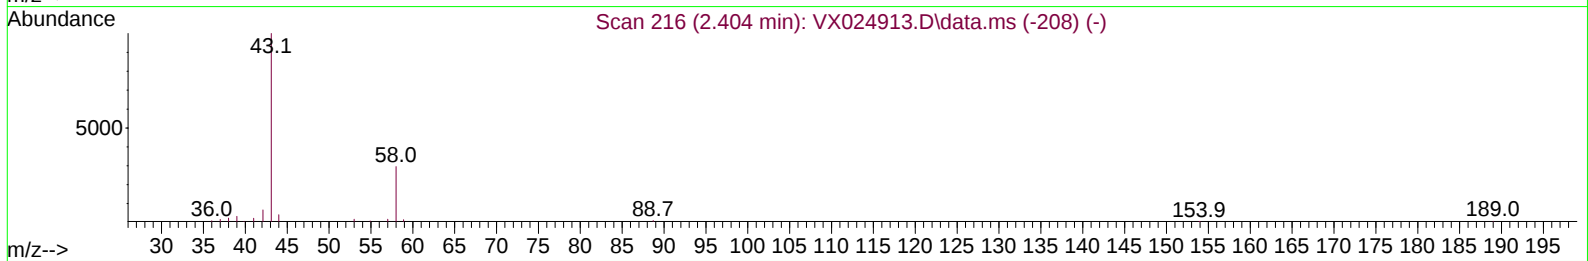
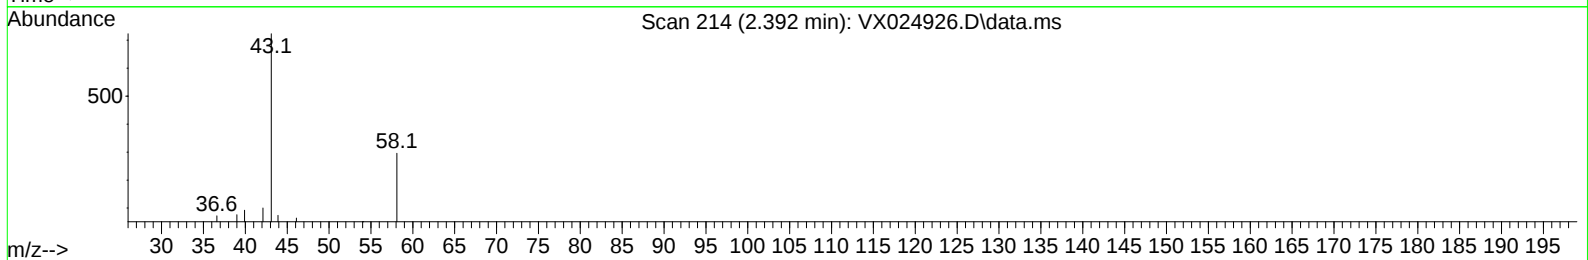


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
 Data File : VX024926.D
 Acq On : 25 Oct 2021 21:46
 Operator : JC/MD
 Sample : M4318-02
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Oct 26 01:27:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 26 01:24:18 2021
 Response via : Initial Calibration

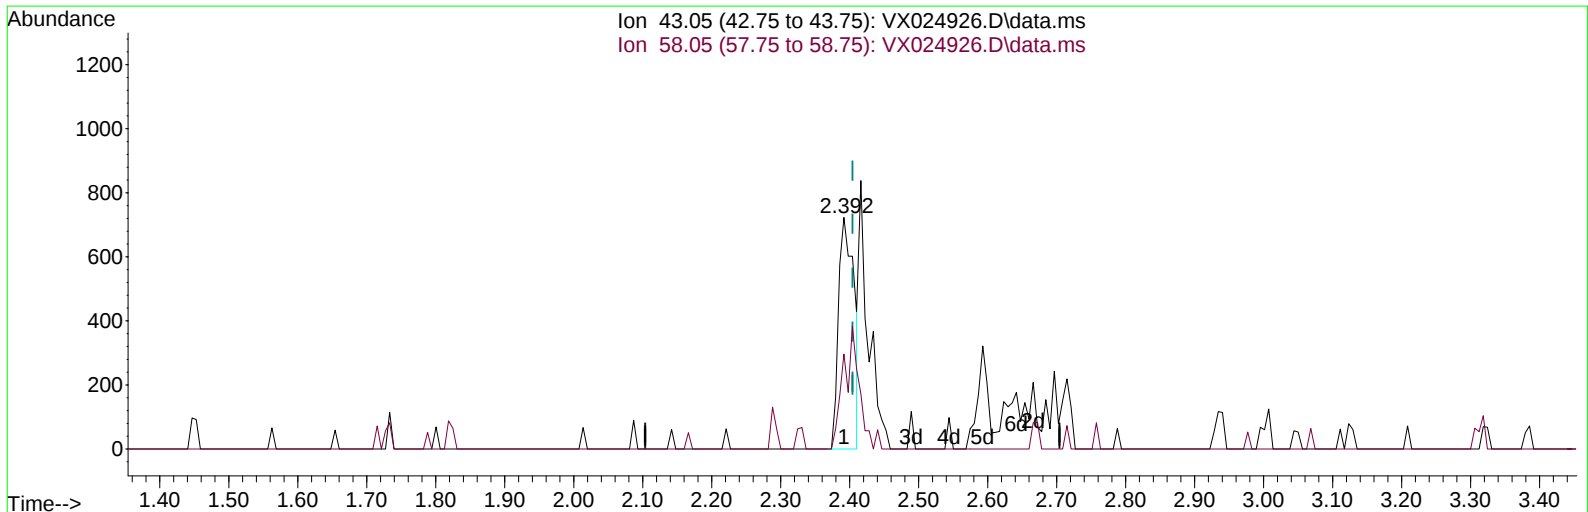

TIC: VX024926.D\data.ms

(13) Acetone (T)

2.392min (-0.012) 1.83 ug/L

response 1130

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.10	54.51
0.00	0.00	0.00
0.00	0.00	0.00