

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
 Data File : VX024923.D
 Acq On : 25 Oct 2021 20:35
 Operator : JC/MD
 Sample : M4303-21
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P055-TW001-01

Quant Time: Oct 26 01:27:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 26 01:24:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	77794	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	74008	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	34493	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	8727	3.821	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.400%
7) Chloroethane-d5	1.672	69	9146	4.445	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.800%
11) 1,1-Dichloroethene-d2	2.313	63	23467	2.756	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.200%#
20) 2-Butanone-d5	4.471	46	43380	51.952	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.900%
24) Chloroform-d	5.068	84	51349	4.670	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
26) 1,2-Dichloroethane-d4	5.958	65	25888	4.308	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.200%
32) Benzene-d6	5.983	84	77168	4.475	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.600%
36) 1,2-Dichloropropane-d6	7.318	67	23434	4.260	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.200%
41) Toluene-d8	8.653	98	72812	4.211	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.200%
43) trans-1,3-Dichloroprop...	8.952	79	9588	3.797	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.000%
46) 2-Hexanone-d5	9.390	63	42365	46.617	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.240%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	19472	4.631	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.600%
66) 1,2-Dichlorobenzene-d4	12.323	152	27097	4.662	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.200%
Target Compounds					Qvalue	
13) Acetone	2.404	43	1858	2.967	ug/L	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024923.D
Acq On : 25 Oct 2021 20:35
Operator : JC/MD
Sample : M4303-21
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P055-TW001-01


Quant Time: Oct 26 01:27:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 26 01:24:18 2021
Response via : Initial Calibration

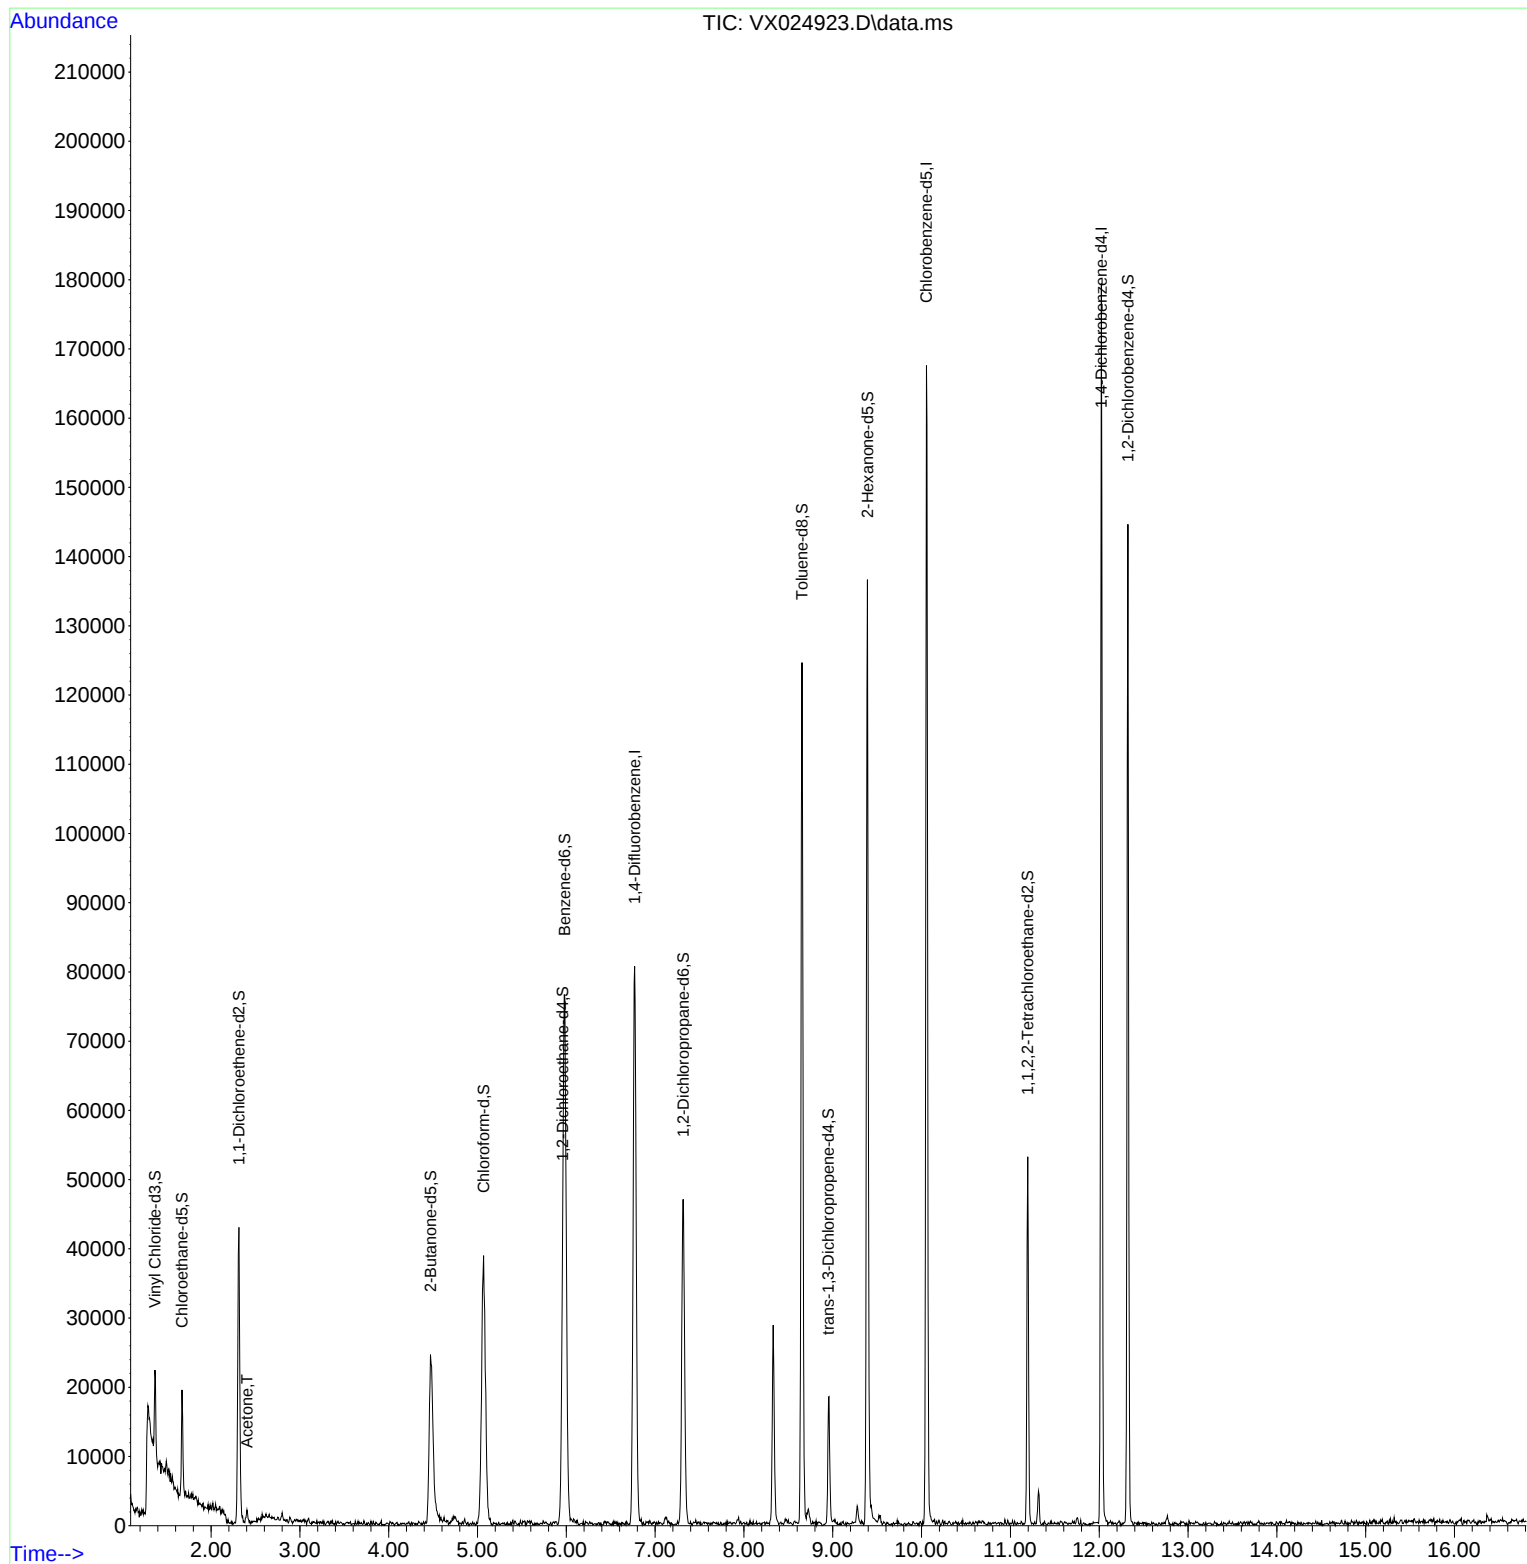

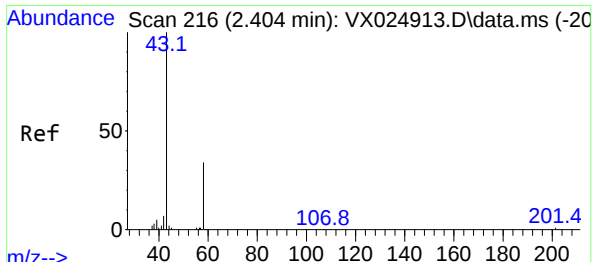

#13
Acetone
Concen: 2.967 ug/L
RT: 2.404 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX024923.D
Acq: 25 Oct 2021 20:35

Instrument :
MSVOA_X
ClientSampleId :
P055-TW001-01

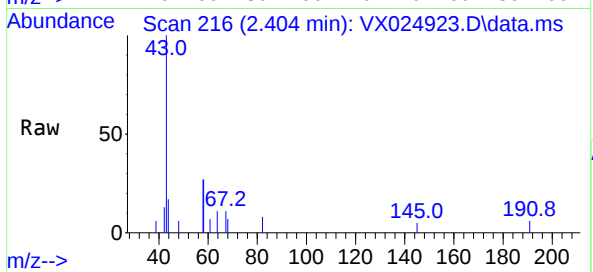

Tgt Ion: 43 Resp: 1858
Ion Ratio Lower Upper
43 100
58 46.2 0.0 64.2

