

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
 Data File : VX024925.D
 Acq On : 25 Oct 2021 21:22
 Operator : JC/MD
 Sample : M4318-01
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P008-TW001-02

Quant Time: Oct 26 01:27:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 26 01:24:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	78769	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	76093	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	33680	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	8923	3.859	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.200%
7) Chloroethane-d5	1.672	69	9110	4.372	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.400%
11) 1,1-Dichloroethene-d2	2.306	63	24118	2.798	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.000%#
20) 2-Butanone-d5	4.471	46	43914	51.940	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.880%
24) Chloroform-d	5.062	84	50391	4.526	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
26) 1,2-Dichloroethane-d4	5.964	65	26368	4.334	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.600%
32) Benzene-d6	5.983	84	76839	4.334	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.600%
36) 1,2-Dichloropropane-d6	7.318	67	24737	4.373	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.400%
41) Toluene-d8	8.653	98	72902	4.101	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.000%
43) trans-1,3-Dichloroprop...	8.952	79	10689	4.117	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.400%
46) 2-Hexanone-d5	9.390	63	42703	45.701	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.400%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	20037	4.635	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.600%
66) 1,2-Dichlorobenzene-d4	12.323	152	25218	4.443	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.800%
Target Compounds						
					Qvalue	
13) Acetone	2.404	43	2060	3.248	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024925.D
Acq On : 25 Oct 2021 21:22
Operator : JC/MD
Sample : M4318-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P008-TW001-02

Quant Time: Oct 26 01:27:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 26 01:24:18 2021
Response via : Initial Calibration

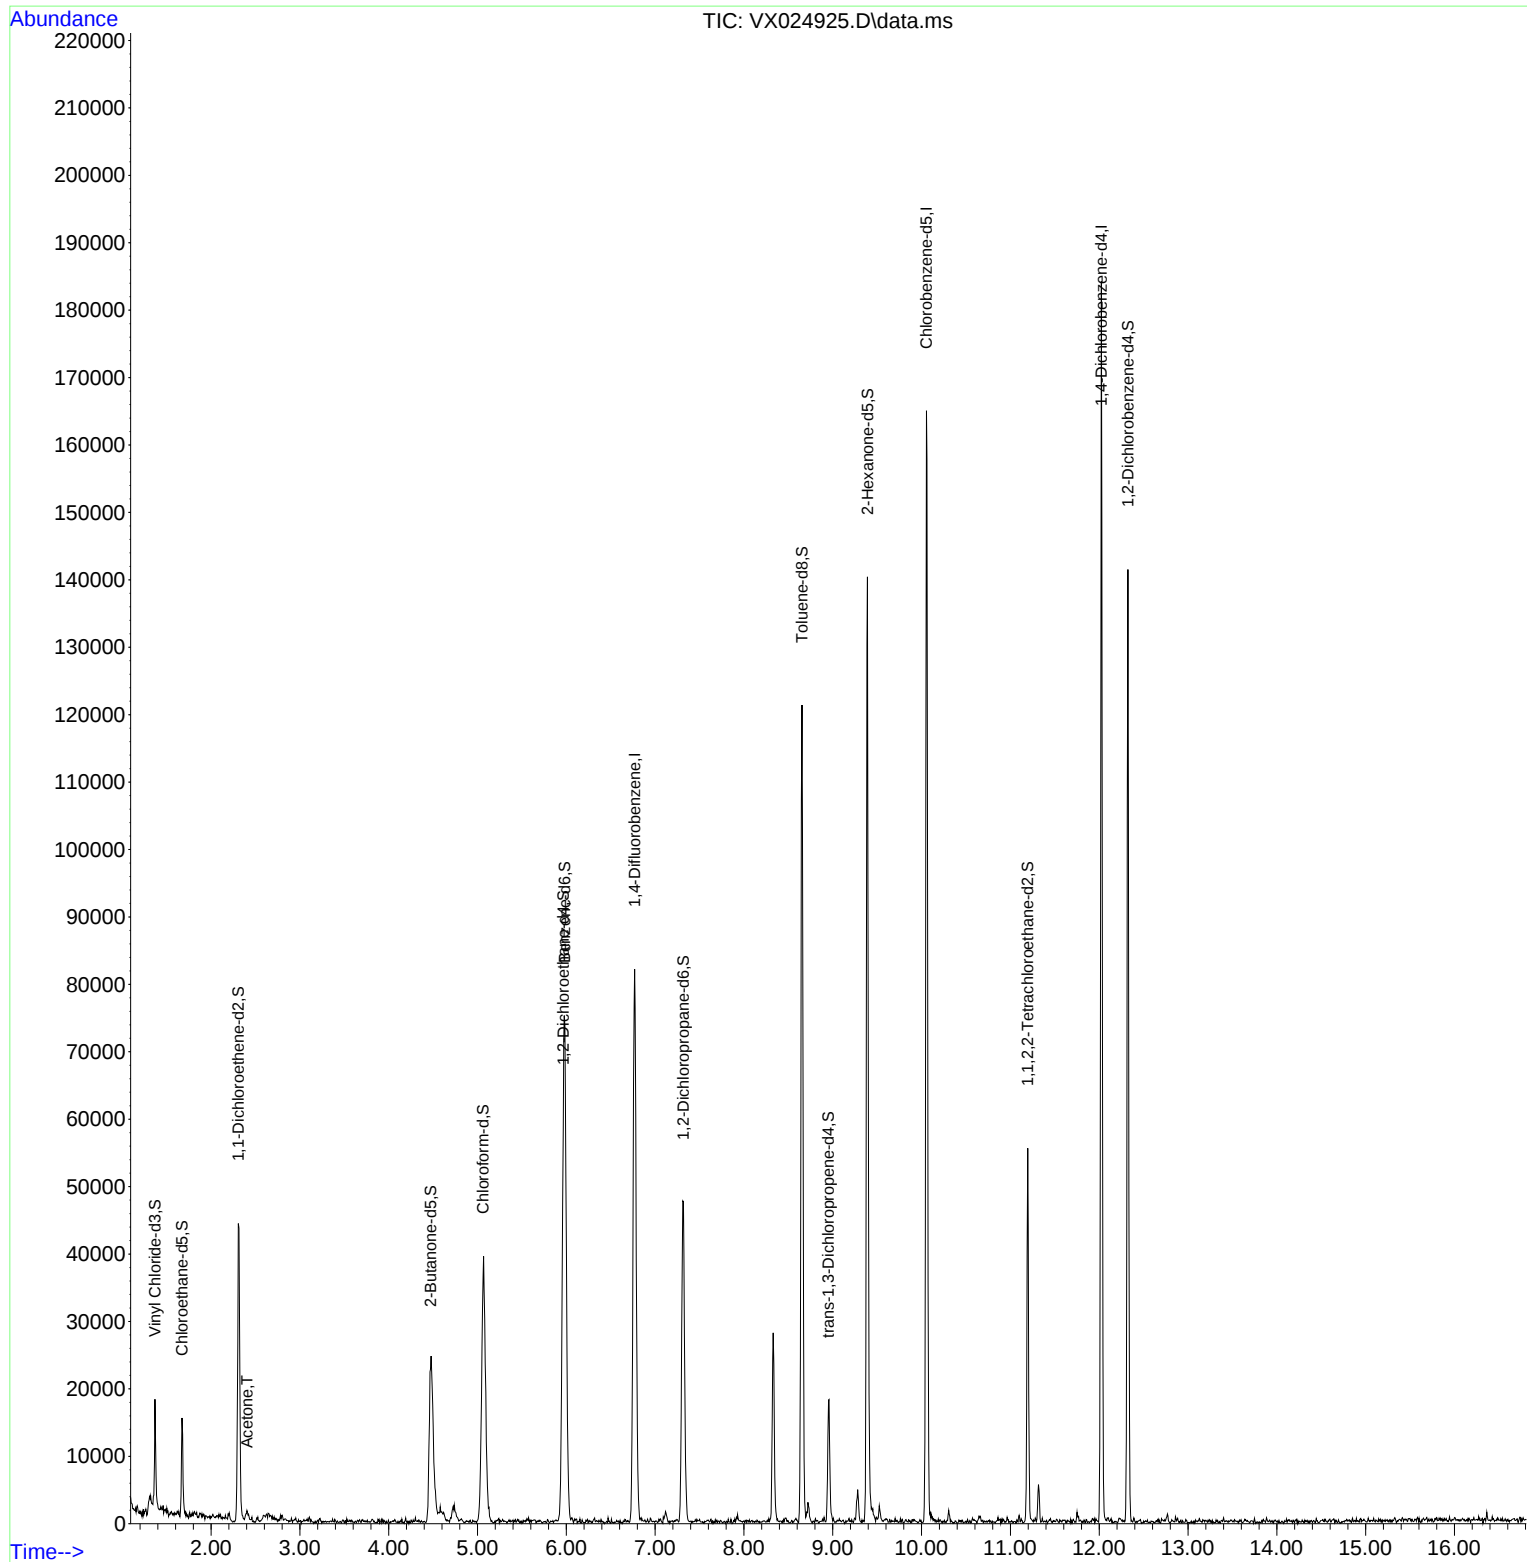

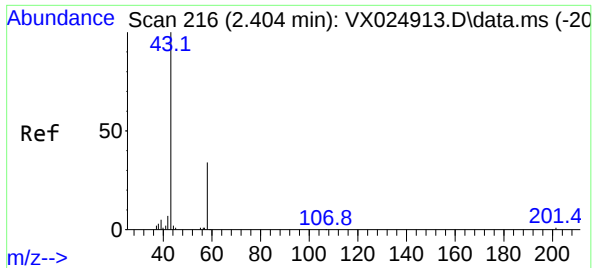

#13
 Acetone
 Concen: 3.248 ug/L
 RT: 2.404 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX024925.D
 Acq: 25 Oct 2021 21:22

Instrument :
 MSVOA_X
 ClientSampleId :
 P008-TW001-02

Tgt Ion: 43 Resp: 2060
 Ion Ratio Lower Upper
 43 100
 58 34.4 0.0 64.2

