

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
 Data File : VX024927.D
 Acq On : 25 Oct 2021 22:10
 Operator : JC/MD
 Sample : M4318-05
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P016-TW001-03

Quant Time: Oct 26 01:27:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 26 01:24:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	79706	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	73021	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	35449	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	7728	3.303	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.000%
7) Chloroethane-d5	1.672	69	8751	4.151	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.000%
11) 1,1-Dichloroethene-d2	2.306	63	24649	2.826	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.600%#
20) 2-Butanone-d5	4.470	46	40984	47.905	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.800%
24) Chloroform-d	5.068	84	50480	4.481	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.600%
26) 1,2-Dichloroethane-d4	5.964	65	26063	4.233	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.600%
32) Benzene-d6	5.982	84	75827	4.457	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%
36) 1,2-Dichloropropane-d6	7.318	67	23926	4.408	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.200%
41) Toluene-d8	8.653	98	71873	4.213	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.200%
43) trans-1,3-Dichloroprop...	8.957	79	10156	4.076	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.600%
46) 2-Hexanone-d5	9.390	63	42133	46.988	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.980%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	19275	4.646	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.000%
66) 1,2-Dichlorobenzene-d4	12.323	152	25308	4.236	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.800%
Target Compounds						
					Qvalue	
13) Acetone	2.404	43	1775	2.766	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024927.D
Acq On : 25 Oct 2021 22:10
Operator : JC/MD
Sample : M4318-05
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P016-TW001-03


Quant Time: Oct 26 01:27:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 26 01:24:18 2021
Response via : Initial Calibration

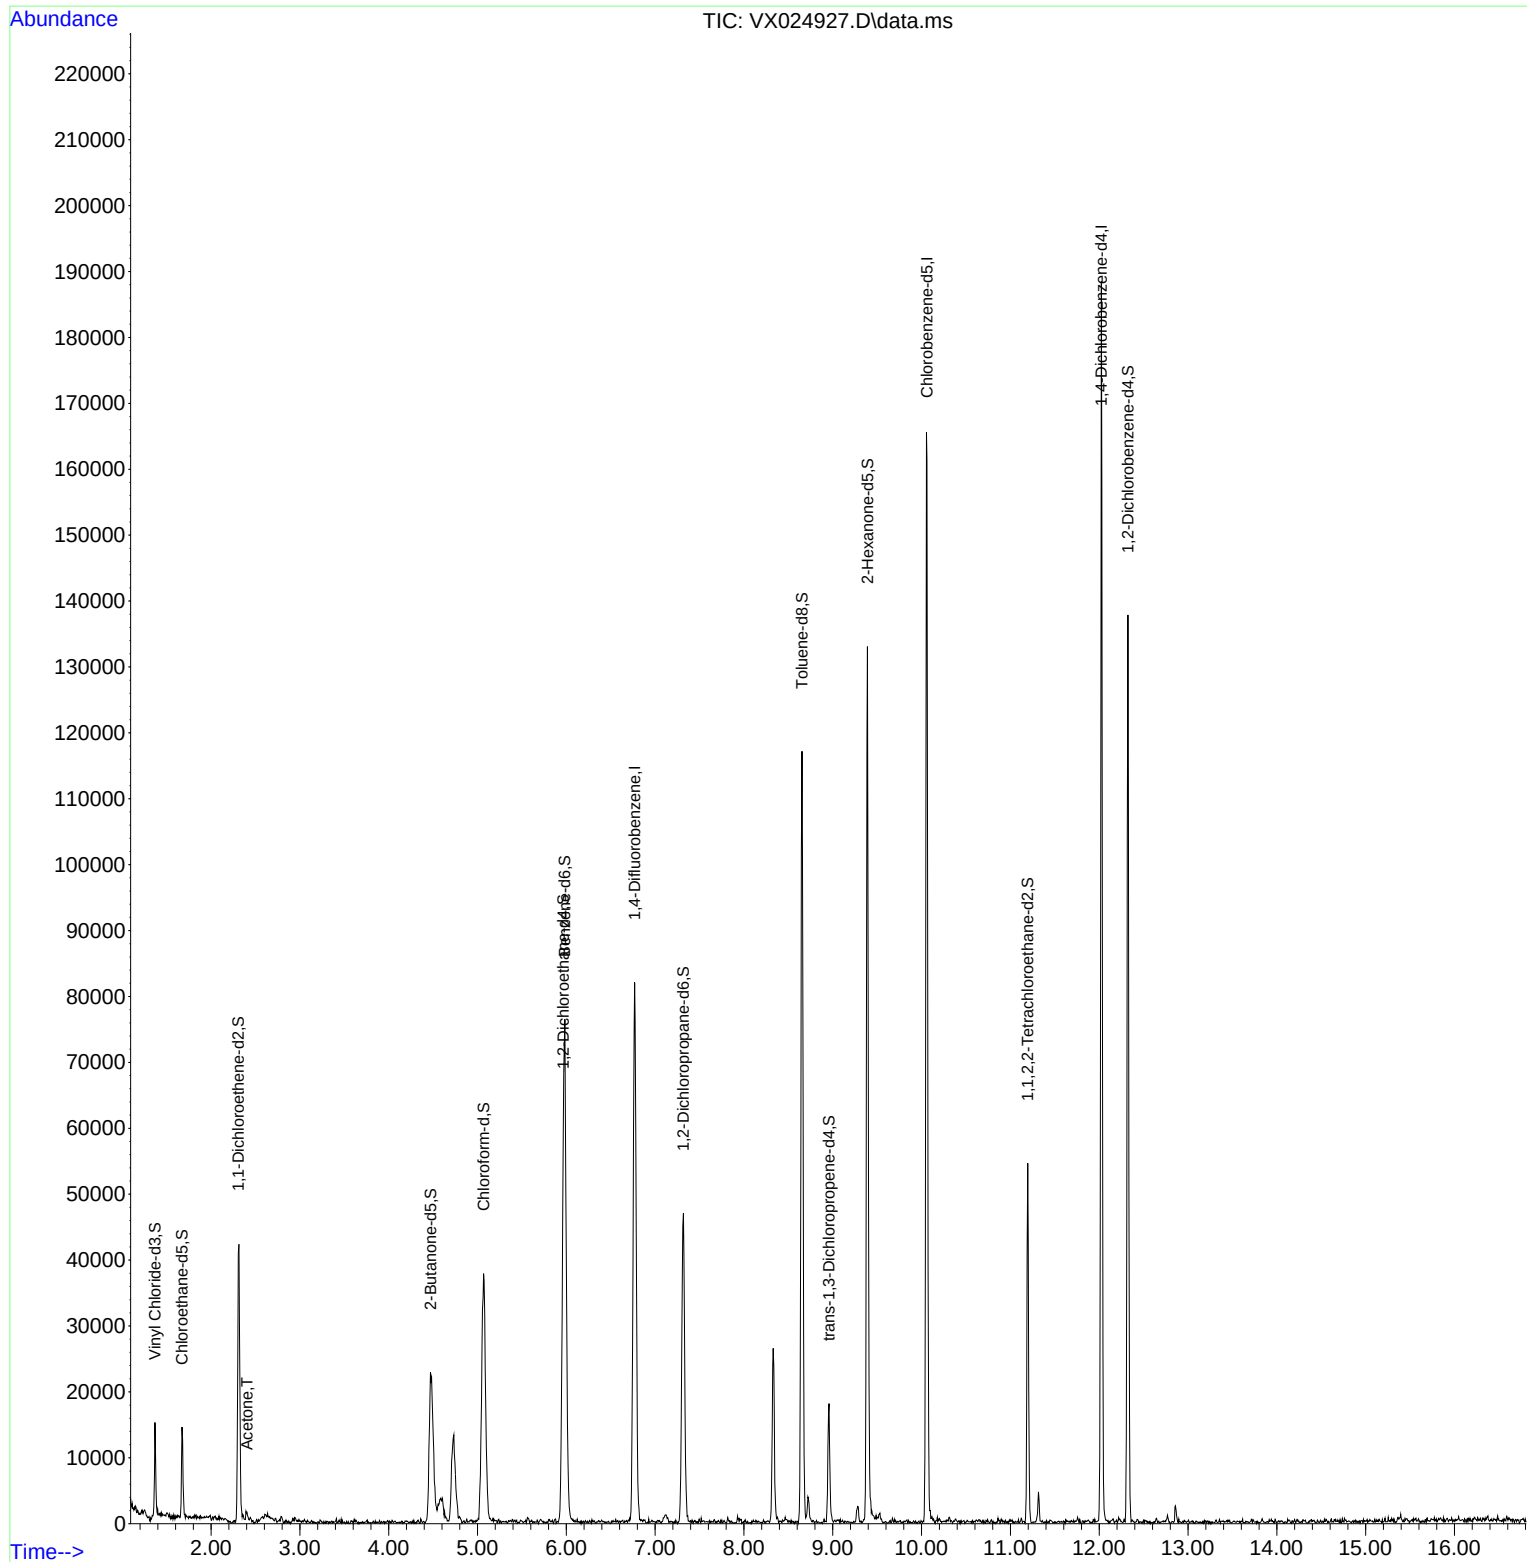

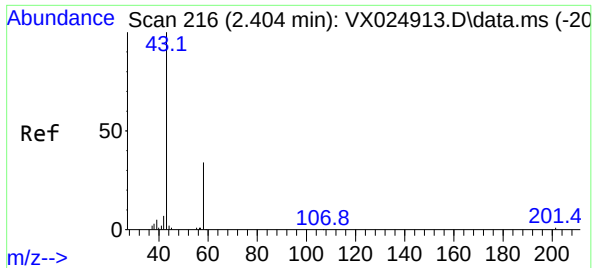

#13
 Acetone
 Concen: 2.766 ug/L
 RT: 2.404 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX024927.D
 Acq: 25 Oct 2021 22:10

Instrument :
 MSVOA_X
 ClientSampleId :
 P016-TW001-03

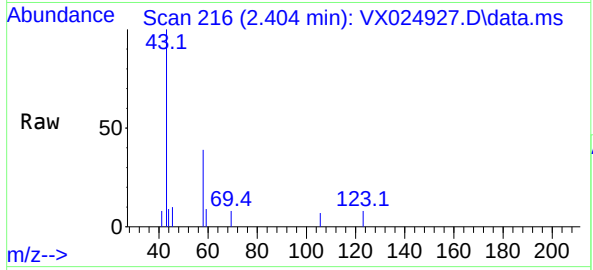

Tgt Ion: 43 Resp: 1775
 Ion Ratio Lower Upper
 43 100
 58 35.2 0.0 64.2

