

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
 Data File : VX024918.D
 Acq On : 25 Oct 2021 18:35
 Operator : JC/MD
 Sample : M4291-24
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P052-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	39	46	51	rBV	13229	16234	6.80%	0.797%
2	1.672	92	96	103	rVB	14644	18139	7.59%	0.890%
3	2.306	194	200	210	rVB	40686	67134	28.11%	3.295%
4	2.514	230	234	241	rVB	2862	4406	1.84%	0.216%
5	4.471	545	555	570	rBV	23494	73847	30.92%	3.625%
6	5.062	641	652	665	rBV3	36102	115405	48.32%	5.665%
7	5.977	790	802	818	rVB3	74539	225790	94.53%	11.083%
8	6.769	922	932	941	rBV	83497	202841	84.92%	9.957%
9	7.318	1013	1022	1032	rVB2	49132	107974	45.21%	5.300%
10	8.330	1182	1188	1200	rBV	27118	46898	19.64%	2.302%
11	8.653	1233	1241	1249	rBV	123140	192619	80.65%	9.455%
12	8.720	1249	1252	1258	rVB	2781	3908	1.64%	0.192%
13	8.958	1285	1291	1299	rVB2	18218	29140	12.20%	1.430%
14	9.281	1338	1344	1350	rBV3	3003	4508	1.89%	0.221%
15	9.391	1356	1362	1374	rBV	133488	195034	81.66%	9.574%
16	10.055	1465	1471	1481	rBV	172573	238848	100.00%	11.724%
17	11.195	1653	1658	1666	rBV	55275	69423	29.07%	3.408%
18	11.317	1672	1678	1683	rBV2	4834	7206	3.02%	0.354%
19	12.024	1789	1794	1804	rVB	195327	234879	98.34%	11.530%
20	12.323	1836	1843	1853	rVB	136918	182962	76.60%	8.981%


Sum of corrected areas: 2037195

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024918.D
Acq On : 25 Oct 2021 18:35
Operator : JC/MD
Sample : M4291-24
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P052-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

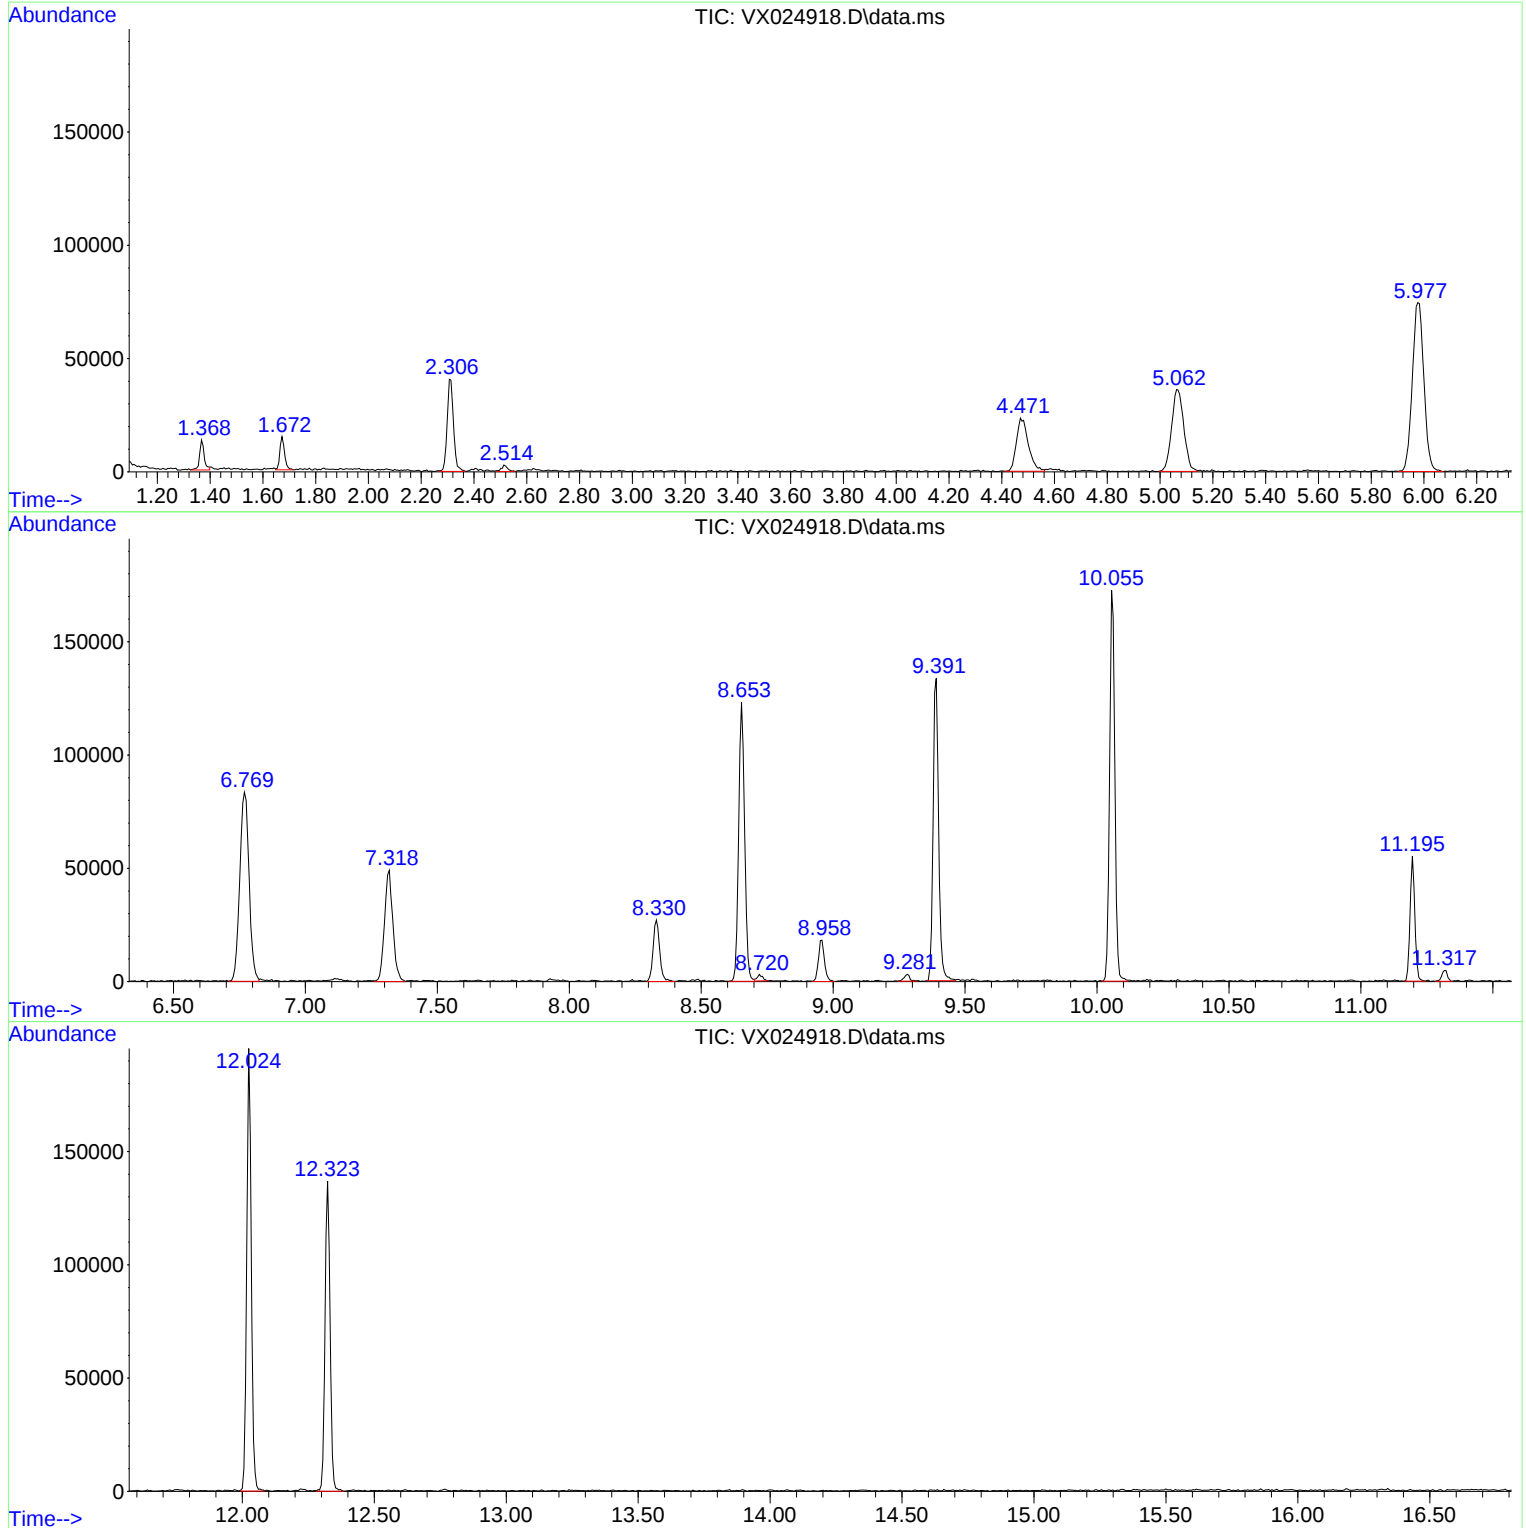

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024918.D
Acq On : 25 Oct 2021 18:35
Operator : JC/MD
Sample : M4291-24
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P052-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024918.D
Acq On : 25 Oct 2021 18:35
Operator : JC/MD
Sample : M4291-24
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P052-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc