

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
 Data File : VX024922.D
 Acq On : 25 Oct 2021 20:11
 Operator : JC/MD
 Sample : M4303-20
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P042-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024922.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rBV	14034	14033	5.87%	0.736%
2	1.672	88	96	101	rBV	12728	17157	7.17%	0.900%
3	2.313	195	201	212	rBV	38108	61628	25.76%	3.232%
4	4.477	545	556	569	rBV2	21991	69619	29.10%	3.651%
5	5.068	642	653	666	rVB2	34447	101491	42.43%	5.323%
6	5.977	790	802	813	rBV4	68246	204679	85.57%	10.735%
7	6.769	920	932	947	rBV2	85909	201699	84.32%	10.578%
8	7.129	985	991	997	rVB4	3476	7403	3.09%	0.388%
9	7.312	1011	1021	1030	rBV	43330	96469	40.33%	5.059%
10	8.330	1183	1188	1194	rBV2	26516	41686	17.43%	2.186%
11	8.653	1233	1241	1248	rBV	108234	174322	72.88%	9.142%
12	8.720	1248	1252	1261	rVB4	2101	4101	1.71%	0.215%
13	8.952	1286	1290	1297	rBV	17384	25079	10.48%	1.315%
14	9.281	1339	1344	1349	rVB2	3038	4523	1.89%	0.237%
15	9.391	1353	1362	1376	rBV	120392	180783	75.58%	9.481%
16	10.055	1466	1471	1479	rBV	174448	239200	100.00%	12.545%
17	11.195	1651	1658	1664	rBV	47985	62127	25.97%	3.258%
18	11.317	1672	1678	1682	rVB2	4510	5557	2.32%	0.291%
19	12.024	1789	1794	1804	rVB	181471	234189	97.91%	12.282%
20	12.323	1837	1843	1852	rVB	125030	160993	67.30%	8.443%




Sum of corrected areas: 1906738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024922.D
Acq On : 25 Oct 2021 20:11
Operator : JC/MD
Sample : M4303-20
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P042-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

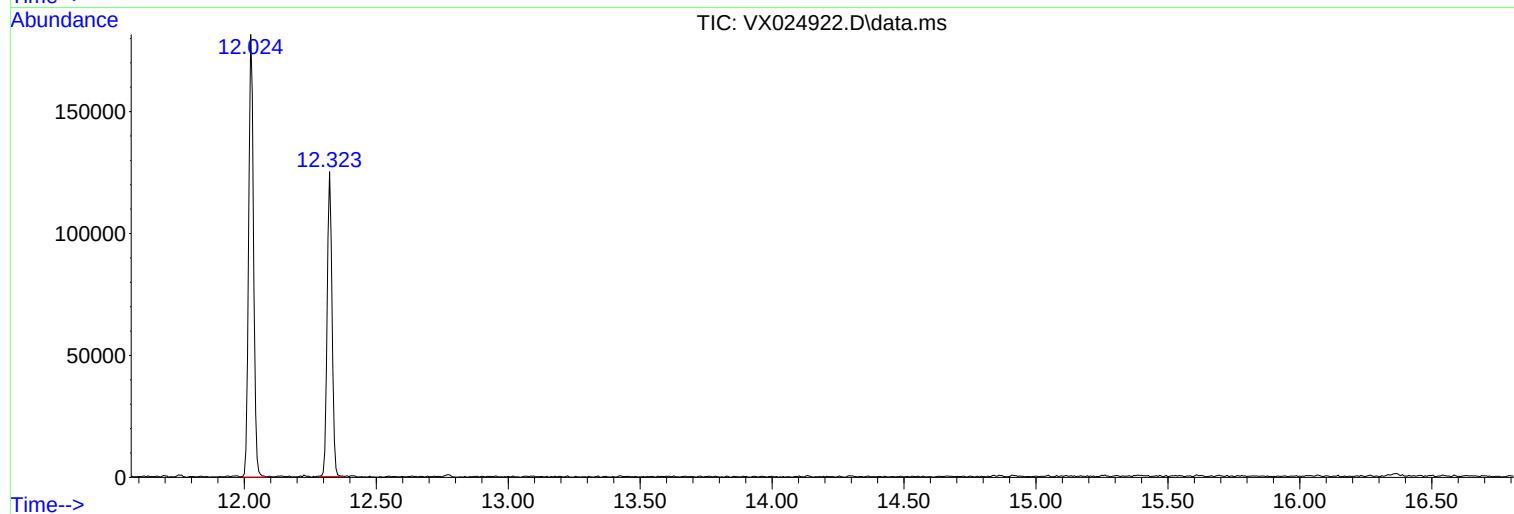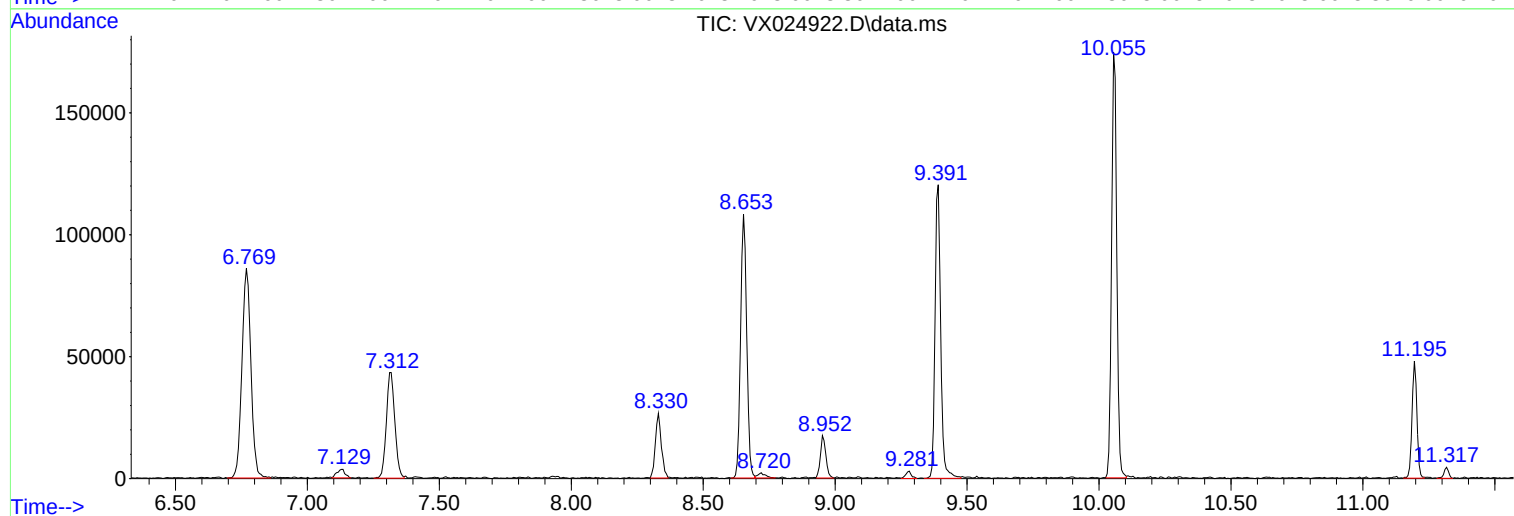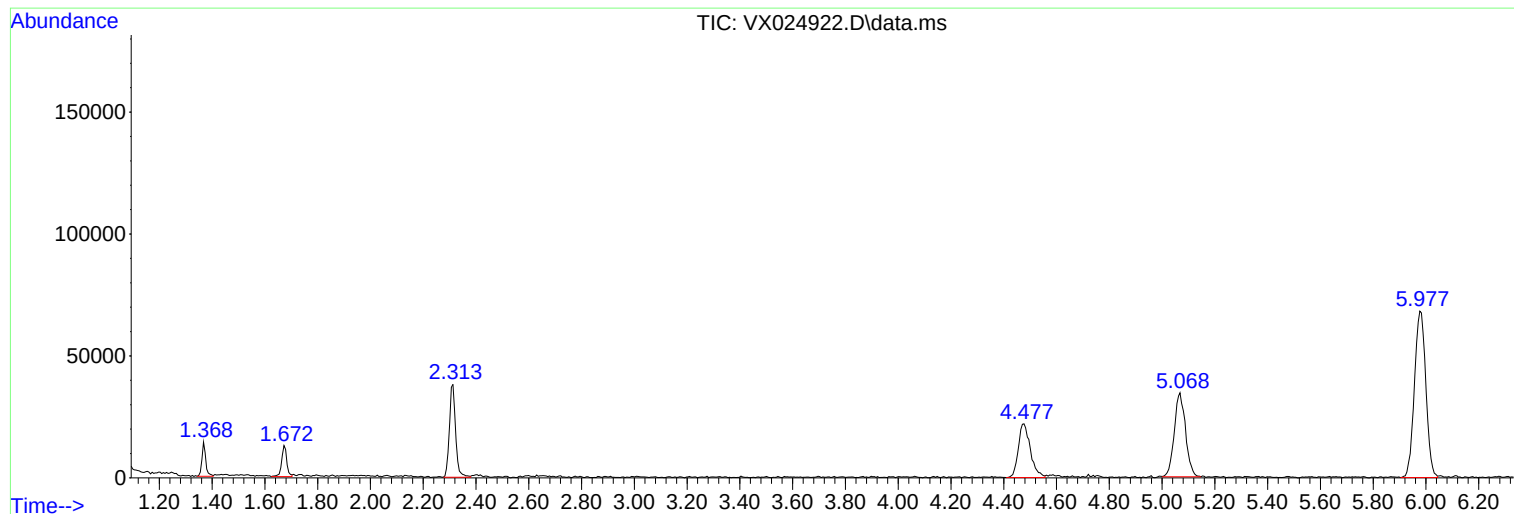

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024922.D
Acq On : 25 Oct 2021 20:11
Operator : JC/MD
Sample : M4303-20
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P042-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024922.D
Acq On : 25 Oct 2021 20:11
Operator : JC/MD
Sample : M4303-20
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P042-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc