

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
 Data File : VX024924.D
 Acq On : 25 Oct 2021 20:58
 Operator : JC/MD
 Sample : M4304-02
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P059-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.325	30	39	42	rBV3	2658	6612	2.82%	0.357%
2	1.368	43	46	53	rVB	12898	14398	6.15%	0.778%
3	1.673	92	96	100	rVB	12070	13949	5.96%	0.753%
4	2.307	193	200	210	rBV	35551	59499	25.42%	3.213%
5	4.483	549	557	574	rBV	17323	63578	27.16%	3.433%
6	5.068	641	653	663	rBV3	33054	99225	42.39%	5.358%
7	5.977	790	802	815	rBV3	67380	196194	83.81%	10.595%
8	6.769	924	932	944	rBV2	84991	201955	86.27%	10.906%
9	7.312	1014	1021	1031	rVB3	40360	91010	38.88%	4.915%
10	8.330	1182	1188	1197	rVB2	24608	42491	18.15%	2.295%
11	8.653	1234	1241	1248	rBV	106998	166841	71.27%	9.010%
12	8.726	1248	1253	1256	rVB3	2732	4084	1.74%	0.221%
13	8.958	1283	1291	1297	rBV	15972	25540	10.91%	1.379%
14	9.281	1339	1344	1350	rBV3	2655	4346	1.86%	0.235%
15	9.391	1354	1362	1369	rBV	116764	171012	73.05%	9.235%
16	10.055	1466	1471	1480	rBV	174693	233972	99.95%	12.635%
17	11.195	1652	1658	1665	rBV2	50336	62665	26.77%	3.384%
18	11.317	1671	1678	1685	rVB2	4972	7518	3.21%	0.406%
19	12.024	1789	1794	1807	rVB	181726	234087	100.00%	12.641%
20	12.323	1837	1843	1850	rBV	118784	152828	65.29%	8.253%




Sum of corrected areas: 1851804

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024924.D
Acq On : 25 Oct 2021 20:58
Operator : JC/MD
Sample : M4304-02
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P059-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

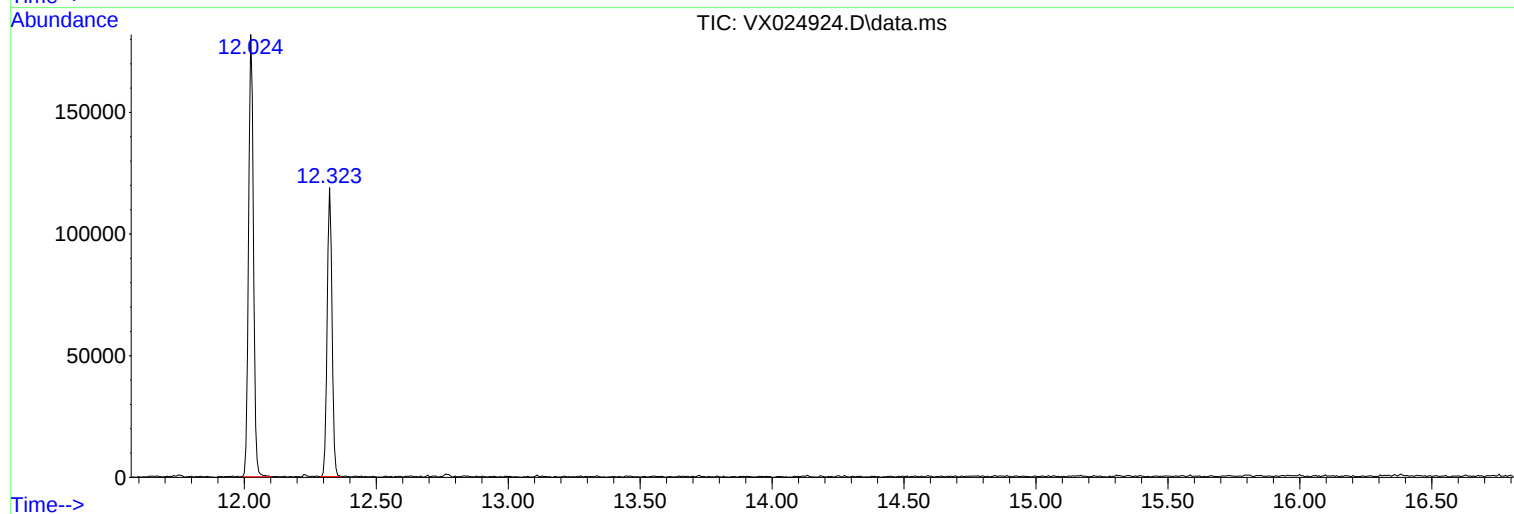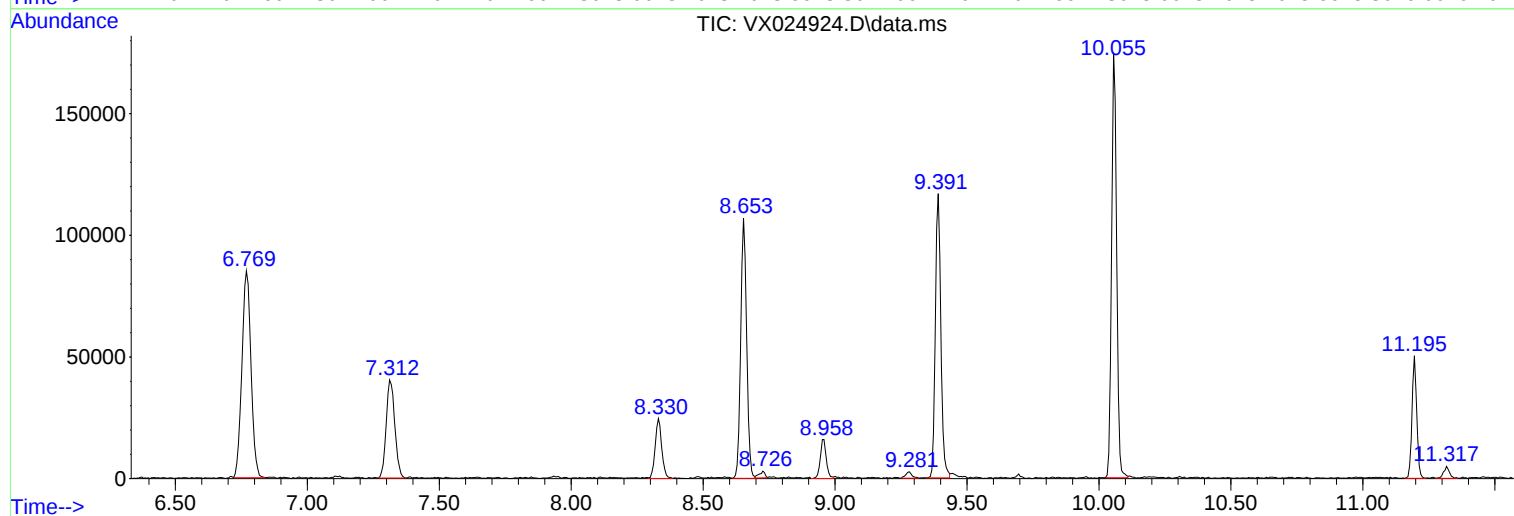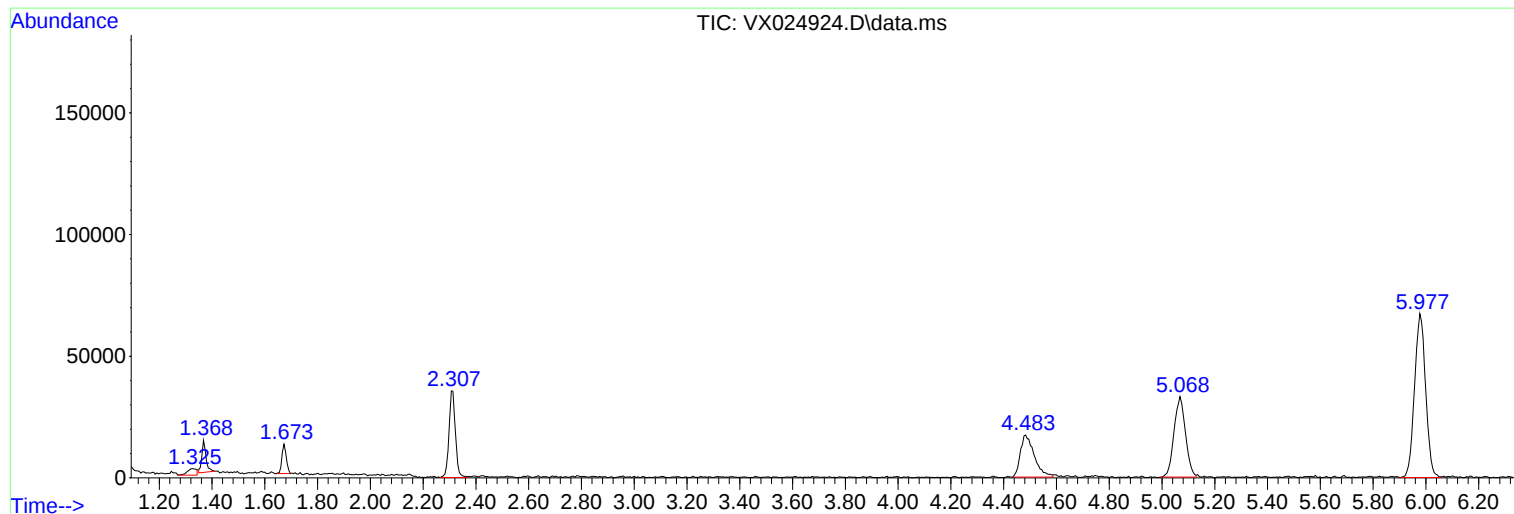

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024924.D
Acq On : 25 Oct 2021 20:58
Operator : JC/MD
Sample : M4304-02
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P059-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024924.D
Acq On : 25 Oct 2021 20:58
Operator : JC/MD
Sample : M4304-02
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P059-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc