

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
 Data File : VX024928.D
 Acq On : 25 Oct 2021 22:34
 Operator : JC/MD
 Sample : M4318-06
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P017-TW001-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rBV	14438	15735	7.29%	0.832%
2	1.672	93	96	105	rVB	14355	17969	8.32%	0.951%
3	2.313	192	201	209	rBV	40081	65166	30.17%	3.447%
4	2.867	287	292	299	rVB3	2431	5663	2.62%	0.300%
5	4.483	546	557	568	rBV2	20911	71432	33.07%	3.779%
6	5.068	640	653	668	rBV2	37069	112147	51.93%	5.933%
7	5.977	791	802	816	rBV2	74663	215975	100.00%	11.426%
8	6.769	922	932	947	rBV2	75024	180711	83.67%	9.560%
9	7.117	983	989	995	rBV5	1010	2420	1.12%	0.128%
10	7.318	1013	1022	1030	rBV	44970	99324	45.99%	5.254%
11	8.330	1181	1188	1194	rBV2	26118	45590	21.11%	2.412%
12	8.653	1233	1241	1249	rBV	115781	183150	84.80%	9.689%
13	8.726	1249	1253	1259	rVB2	2369	4282	1.98%	0.227%
14	8.958	1284	1291	1297	rBV	17780	26890	12.45%	1.423%
15	9.275	1336	1343	1350	rBV2	2403	4911	2.27%	0.260%
16	9.391	1353	1362	1372	rBV	129135	184765	85.55%	9.774%
17	10.055	1466	1471	1479	rBV	148867	209152	96.84%	11.065%
18	11.195	1653	1658	1669	rVB	50352	66356	30.72%	3.510%
19	11.317	1673	1678	1684	rVV3	4178	5920	2.74%	0.313%
20	12.024	1789	1794	1802	rBV	165591	207025	95.86%	10.952%
21	12.323	1837	1843	1849	rBV	129283	165702	76.72%	8.766%




Sum of corrected areas: 1890285

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024928.D
Acq On : 25 Oct 2021 22:34
Operator : JC/MD
Sample : M4318-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P017-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

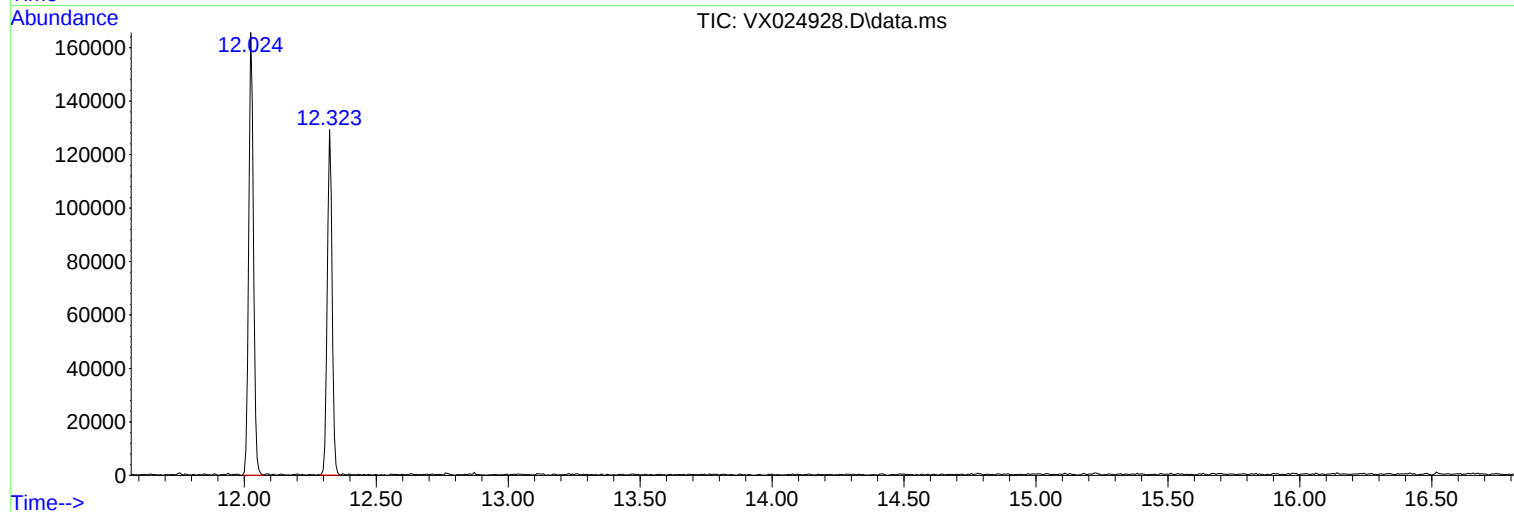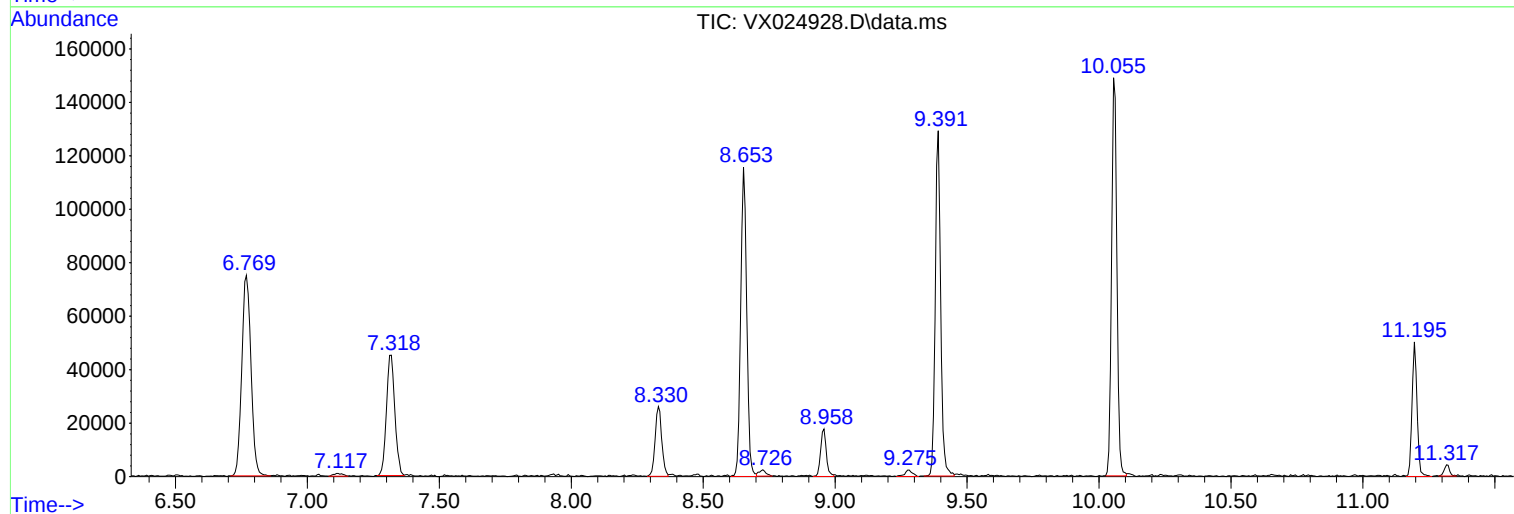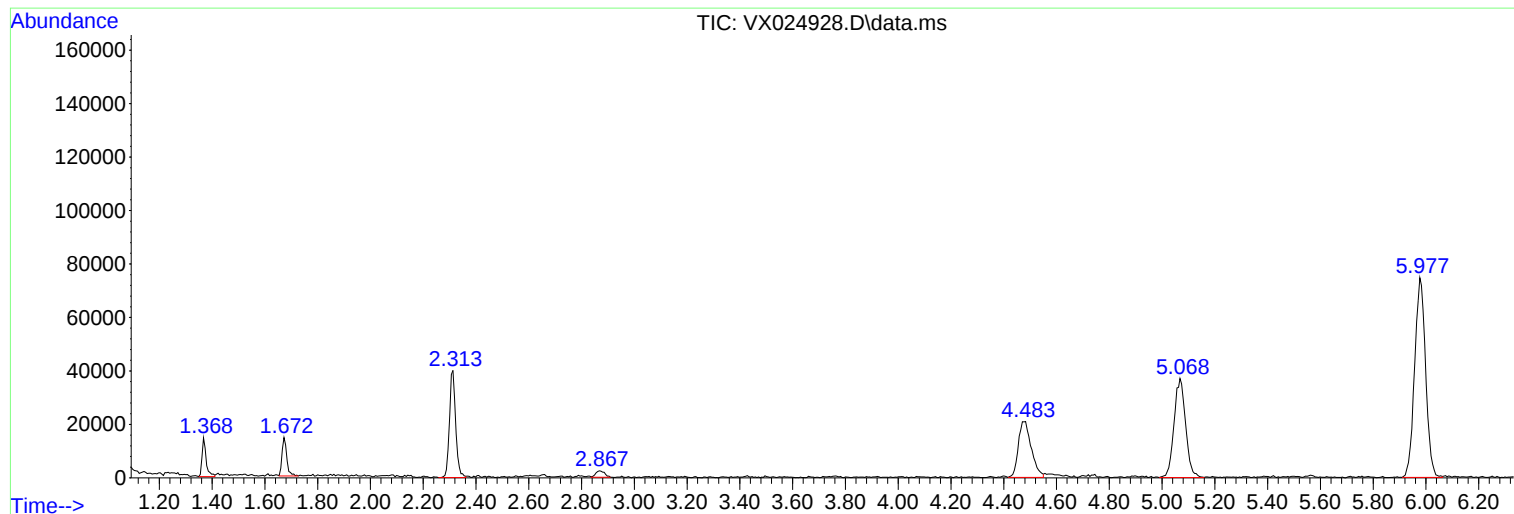

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024928.D
Acq On : 25 Oct 2021 22:34
Operator : JC/MD
Sample : M4318-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P017-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024928.D
Acq On : 25 Oct 2021 22:34
Operator : JC/MD
Sample : M4318-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P017-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc