

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
 Data File : VX024931.D
 Acq On : 25 Oct 2021 23:45
 Operator : JC/MD
 Sample : M4304-03
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P060-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	12929	12788	5.72%	0.683%
2	1.672	92	96	101	rVB	12365	15499	6.93%	0.828%
3	2.307	195	200	209	rBV	36791	60986	27.27%	3.258%
4	4.489	547	558	574	rBV2	18221	67179	30.04%	3.588%
5	4.733	592	598	602	rBV2	1995	4584	2.05%	0.245%
6	5.068	641	653	667	rBV2	34673	107591	48.12%	5.747%
7	5.977	789	802	812	rBV3	68998	206367	92.29%	11.023%
8	6.769	923	932	944	rBV2	78817	191072	85.45%	10.206%
9	7.111	982	988	993	rBV3	1714	2825	1.26%	0.151%
10	7.312	1011	1021	1031	rBV2	43433	95372	42.65%	5.094%
11	8.330	1182	1188	1196	rBV	25440	41620	18.61%	2.223%
12	8.653	1234	1241	1248	rBV	109489	173842	77.74%	9.286%
13	8.726	1248	1253	1257	rVB	3557	5827	2.61%	0.311%
14	8.958	1286	1291	1298	rBV	17555	26894	12.03%	1.437%
15	9.275	1339	1343	1350	rVB4	2094	3480	1.56%	0.186%
16	9.391	1356	1362	1378	rBV	122592	181499	81.17%	9.695%
17	10.055	1465	1471	1483	rBV	161451	223608	100.00%	11.944%
18	11.195	1653	1658	1663	rBV	49858	63187	28.26%	3.375%
19	11.317	1674	1678	1682	rVB3	2720	3553	1.59%	0.190%
20	12.024	1789	1794	1801	rBV	178937	221664	99.13%	11.840%
21	12.323	1837	1843	1849	rBV	133023	162671	72.75%	8.689%




Sum of corrected areas: 1872108

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024931.D
Acq On : 25 Oct 2021 23:45
Operator : JC/MD
Sample : M4304-03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P060-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

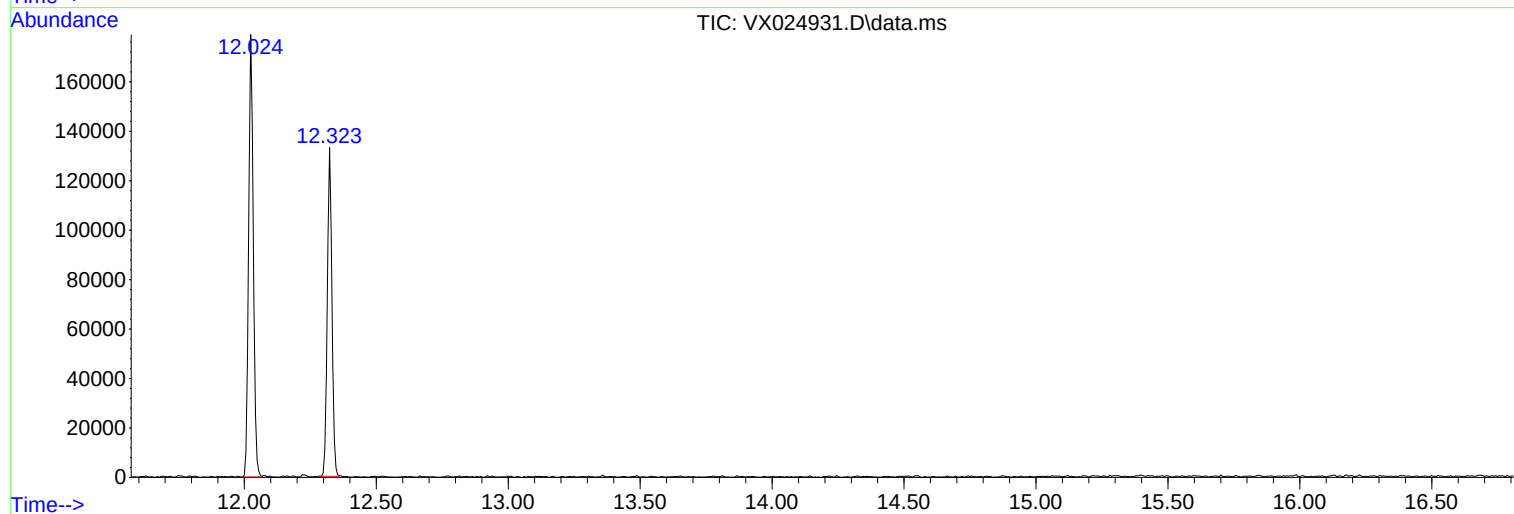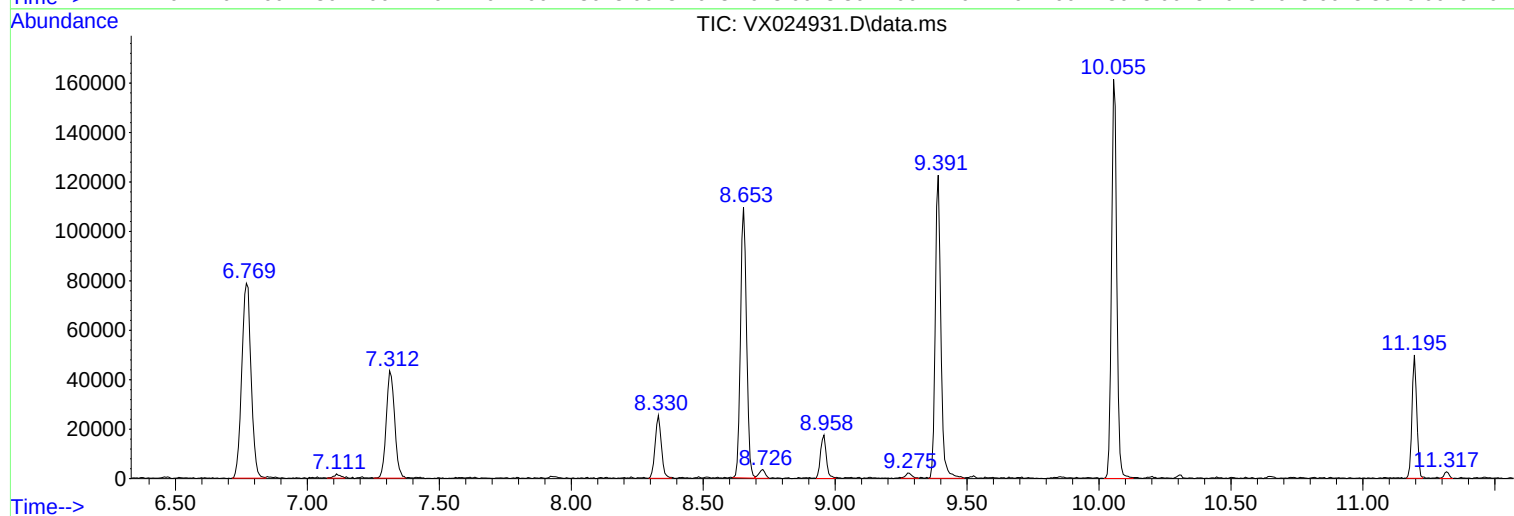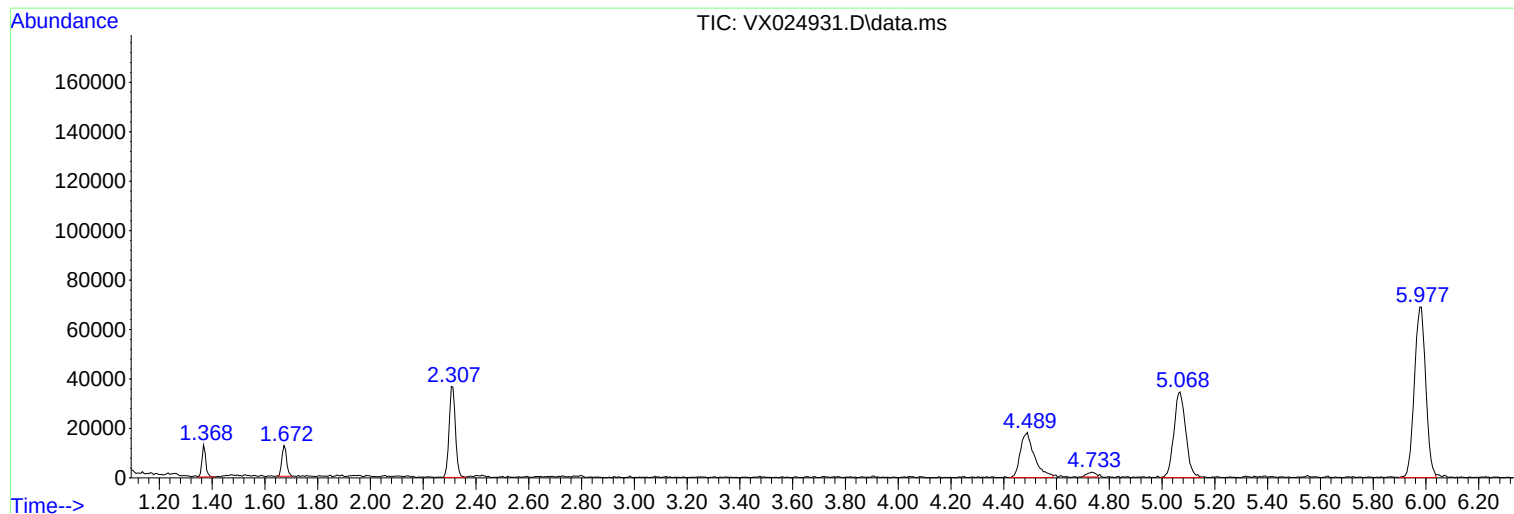

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024931.D
Acq On : 25 Oct 2021 23:45
Operator : JC/MD
Sample : M4304-03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P060-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102521\
Data File : VX024931.D
Acq On : 25 Oct 2021 23:45
Operator : JC/MD
Sample : M4304-03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P060-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc