

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
 Data File : VX032361.D
 Acq On : 25 Oct 2022 14:03
 Operator : JC/MD
 Sample : N5187-01ME 10X
 Misc : 1.06g/10mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BUR-1202ME

Quant Time: Oct 27 14:17:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
 Quant Title : SW846 8260
 QLast Update : Sat Oct 22 04:56:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	127870	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	200480	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	174726	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	84289	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	79400	47.732	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	95.460%		
35) Dibromofluoromethane	5.391	113	64243	46.050	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	92.100%		
50) Toluene-d8	8.653	98	236892	47.172	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	94.340%		
62) 4-Bromofluorobenzene	11.079	95	83255	45.274	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	90.540%		
Target Compounds						
					Qvalue	
3) Chloromethane	1.288	50	80	Below Cal	#	44
6) Chloroethane	1.709	64	63	2.001	ug/l #	41
11) Tert butyl alcohol	2.946	59	1509	Below Cal	#	74
16) Acetone	2.380	43	16322	30.236	ug/l	99
20) Methylene Chloride	2.788	84	931	0.672	ug/l #	95
25) 2-Butanone	4.574	43	221	0.262	ug/l #	48
31) Cyclohexane	5.550	56	3431	1.804	ug/l #	41
36) 1,1-Dichloropropene	5.556	75	9960	5.550	ug/l #	50
38) Carbon Tetrachloride	5.556	117	13482	7.117	ug/l #	17
39) Methylcyclohexane	7.379	83	547	0.255	ug/l #	61
52) Toluene	8.720	92	16683	4.951	ug/l	96
53) t-1,3-Dichloropropene	8.720	75	202	1.914	ug/l #	1
55) 1,1,2-Trichloroethane	9.098	97	418	0.305	ug/l #	15
59) 2-Hexanone	9.384	43	770	0.597	ug/l #	25
67) Ethyl Benzene	10.195	91	5097	0.804	ug/l	98
68) m/p-Xylenes	10.305	106	6332	2.528	ug/l	98
69) o-Xylene	10.646	106	3415	1.423	ug/l	94
73) Isopropylbenzene	10.963	105	3314	0.551	ug/l	99
74) N-amyl acetate	10.866	43	2198	0.989	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.219	83	901	0.466	ug/l #	25
76) 1,2,3-Trichloropropane	11.079	75	44978	26.931	ug/l #	45
78) n-propylbenzene	11.305	91	13408	1.947	ug/l	98
79) 2-Chlorotoluene	11.378	91	6662	1.605	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	15205	2.927	ug/l	96
81) trans-1,4-Dichloro-2-b...	11.079	75	44978	82.698	ug/l #	7
82) 4-Chlorotoluene	11.451	91	2247	0.465	ug/l #	45
83) tert-Butylbenzene	11.756	119	7495	1.442	ug/l #	46
84) 1,2,4-Trimethylbenzene	11.756	105	60103	11.900	ug/l	100
85) sec-Butylbenzene	11.890	105	10928	1.740	ug/l	91
86) p-Isopropyltoluene	12.012	119	6248	1.169	ug/l	92
89) n-Butylbenzene	12.329	91	24807	5.269	ug/l #	49
90) Hexachloroethane	12.555	117	2644	3.188	ug/l #	11
92) 1,2-Dibromo-3-Chloropr...	12.926	75	258	0.698	ug/l #	1
95) Naphthalene	13.780	128	14042	2.418	ug/l #	89
96) 1,2,3-Trichlorobenzene	13.975	180	795	0.436	ug/l #	1

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
Data File : VX032361.D
Acq On : 25 Oct 2022 14:03
Operator : JC/MD
Sample : N5187-01ME 10X
Misc : 1.06g/10mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME

Quant Time: Oct 27 14:17:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260
QLast Update : Sat Oct 22 04:56:40 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
Data File : VX032361.D
Acq On : 25 Oct 2022 14:03
Operator : JC/MD
Sample : N5187-01ME 10X
Misc : 1.06g/10mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME

Quant Time: Oct 27 14:17:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260
QLast Update : Sat Oct 22 04:56:40 2022
Response via : Initial Calibration




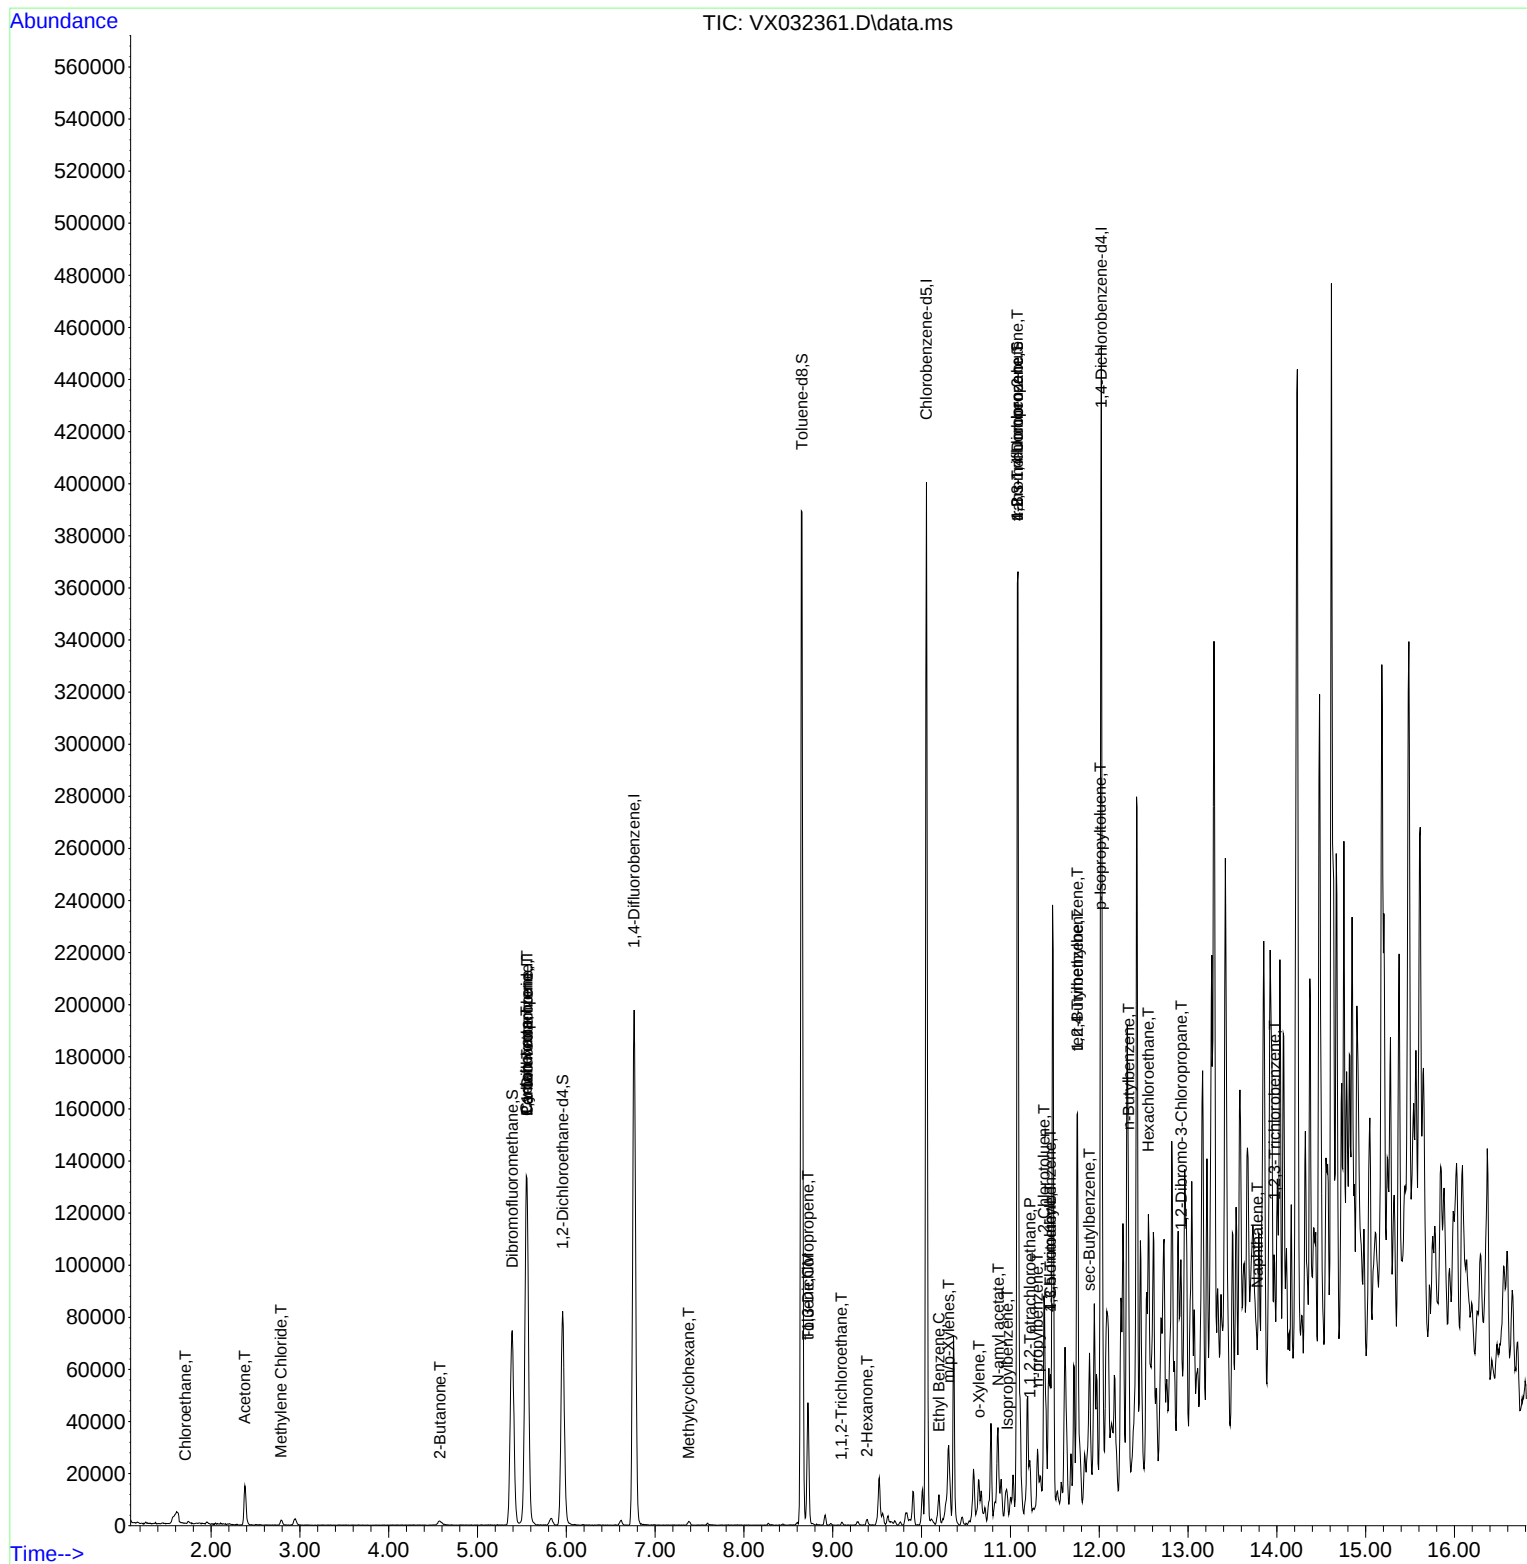




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME

Tgt Ion:168 Resp: 127870
Ion Ratio Lower Upper
168 100
99 57.2 44.8 67.2




#3
Chloromethane
Concen: Below Cal
RT: 1.288 min Scan# 33
Delta R.T. -0.007 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03

Tgt Ion: 50 Resp: 80
Ion Ratio Lower Upper
50 100
52 0.0 24.7 37.1#



Abundance Scan 98 (1.685 min): VX032201.D\data.ms (-89)

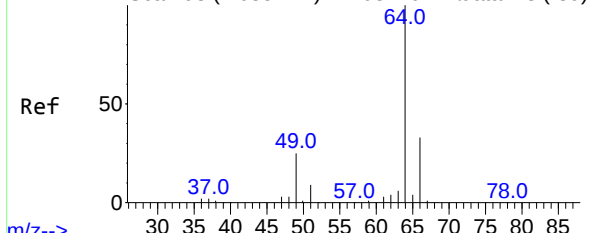

#6

Chloroethane

Concen: 2.001 ug/l

RT: 1.709 min Scan# 11

Delta R.T. 0.024 min

Lab File: VX032361.D

Acq: 25 Oct 2022 14:03

Instrument :

MSVOA_X

ClientSampleId :

BUR-1202ME


Tgt Ion: 64 Resp: 63

Ion Ratio Lower Upper


64 100

66 0.0 26.6 39.8#


Abundance Scan 102 (1.709 min): VX032361.D\data.ms

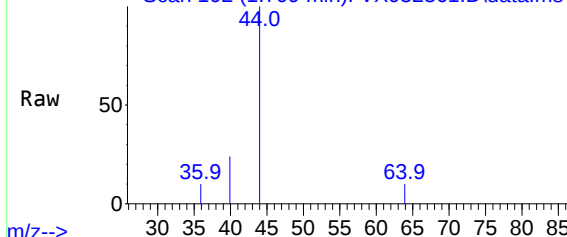


Abundance

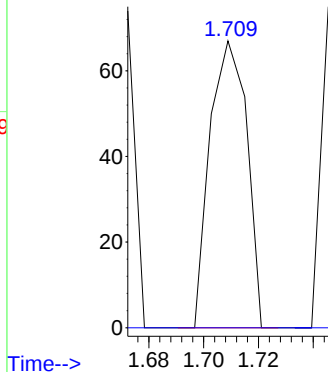

Abundance Scan 102 (1.709 min): VX032361.D\data.ms (-49)

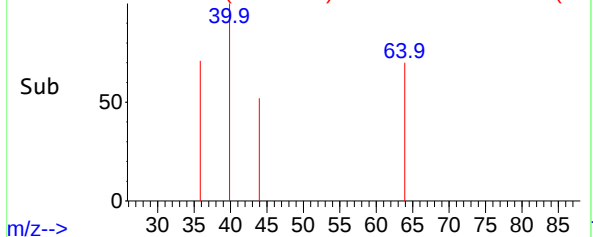

Abundance Scan 310 (2.977 min): VX032201.D\data.ms (-29)

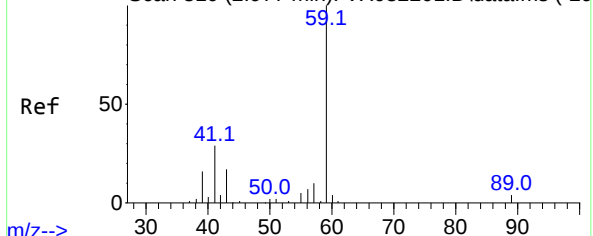

#11

Tert butyl alcohol

Concen: Below Cal

RT: 2.946 min Scan# 305

Delta R.T. -0.031 min

Lab File: VX032361.D

Acq: 25 Oct 2022 14:03


Tgt Ion: 59 Resp: 1509

Ion Ratio Lower Upper


59 100

57 0.0 7.5 11.3#


Abundance Scan 305 (2.946 min): VX032361.D\data.ms

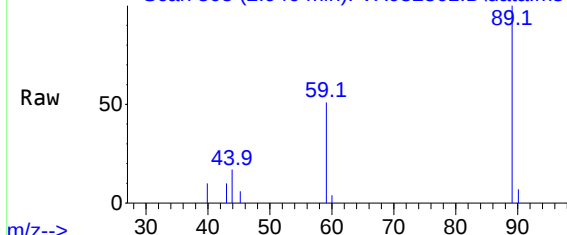


Abundance

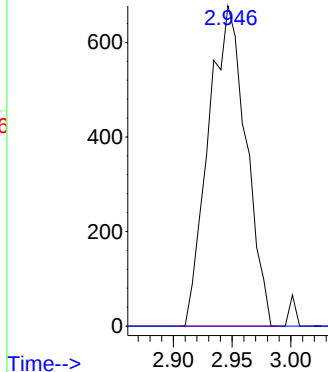

Abundance Scan 305 (2.946 min): VX032361.D\data.ms (-26)




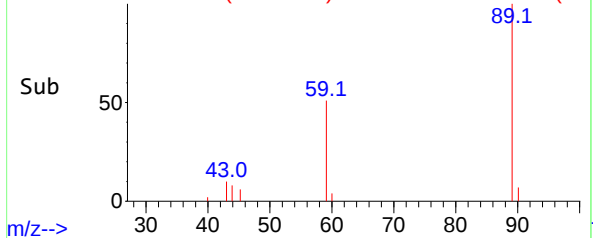




#16
Acetone
Concen: 30.236 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME


Tgt Ion: 43 Resp: 16322
Ion Ratio Lower Upper
43 100
58 29.8 24.2 36.2



#20
Methylene Chloride
Concen: 0.672 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03

Tgt Ion: 84 Resp: 931
Ion Ratio Lower Upper
84 100
49 113.3 92.6 139.0
51 44.2 29.2 43.8#
86 58.9 51.4 77.0

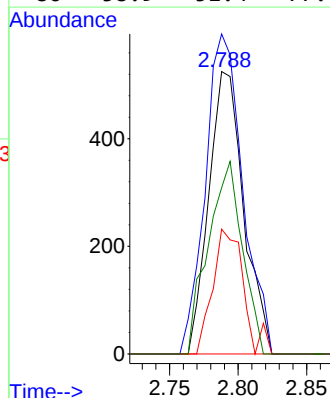



#25

2-Butanone

Concen: 0.262 ug/l

RT: 4.574 min Scan# 51

Delta R.T. 0.018 min

Lab File: VX032361.D

Acq: 25 Oct 2022 14:03

Instrument :

MSVOA_X

ClientSampleId :





BUR-1202ME

Tgt Ion: 43 Resp: 221

Ion Ratio Lower Upper

43 100

72 0.0 21.7 32.5#



#31

Cyclohexane

Concen: 1.804 ug/l

RT: 5.550 min Scan# 732

Delta R.T. 0.073 min

Lab File: VX032361.D

Acq: 25 Oct 2022 14:03




Tgt Ion: 56 Resp: 3431


Ion Ratio Lower Upper

56 100

69 140.3 25.4 38.0#

84 99.2 71.2 106.8

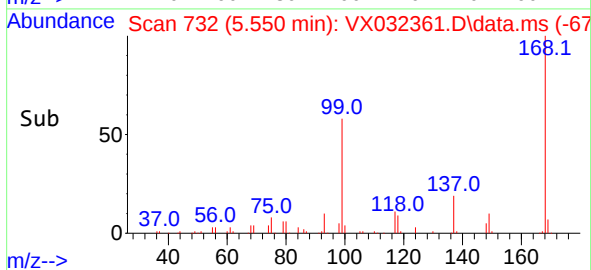



#33

1,2-Dichloroethane-d4

Concen: 47.732 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX032361.D

Acq: 25 Oct 2022 14:03

Instrument :

MSVOA_X

ClientSampleId :





BUR-1202ME

Tgt Ion: 65 Resp: 79400

Ion Ratio Lower Upper

65 100

67 51.5 0.0 103.6

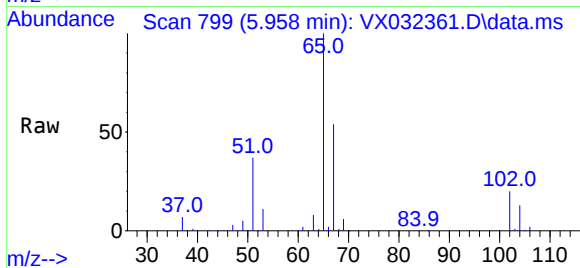

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX032361.D

Acq: 25 Oct 2022 14:03




Tgt Ion: 114 Resp: 200480


Ion Ratio Lower Upper

114 100

63 20.2 0.0 38.6

88 15.9 0.0 32.6



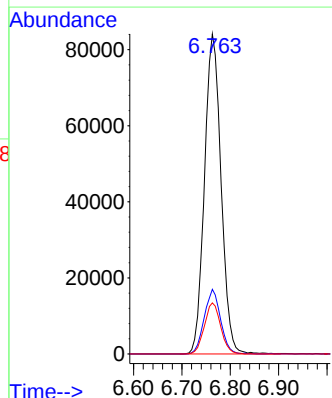
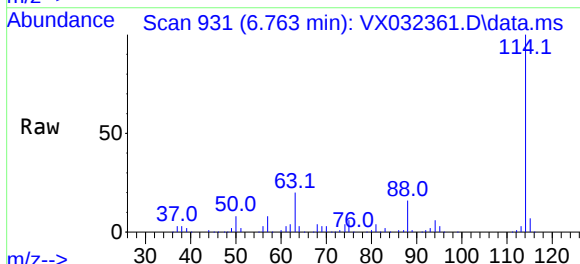


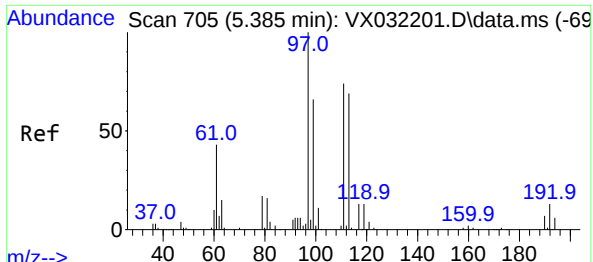

#35
Dibromofluoromethane
Concen: 46.050 ug/l
RT: 5.391 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME


Tgt Ion:113 Resp: 64243
Ion Ratio Lower Upper
113 100
111 102.3 82.8 124.2
192 19.6 15.5 23.3

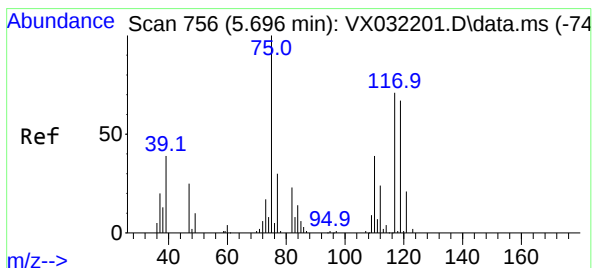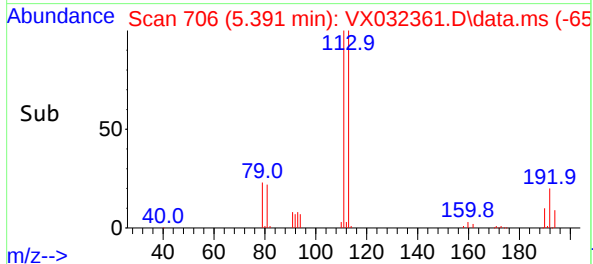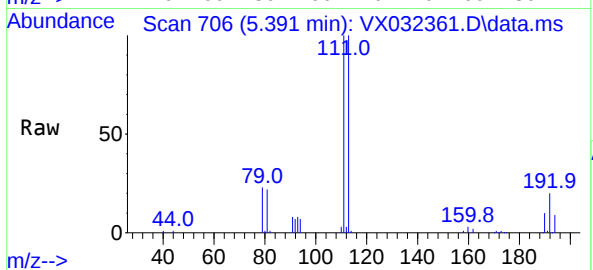

#36
1,1-Dichloropropene
Concen: 5.550 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03


Tgt Ion: 75 Resp: 9960
Ion Ratio Lower Upper
75 100
110 10.2 18.4 55.0#
77 0.0 24.7 37.1#

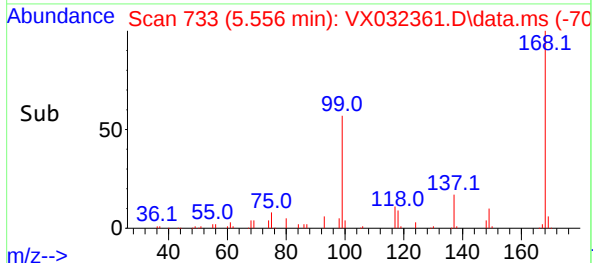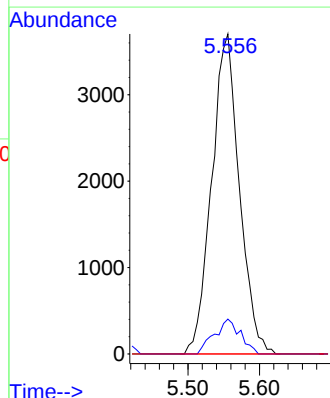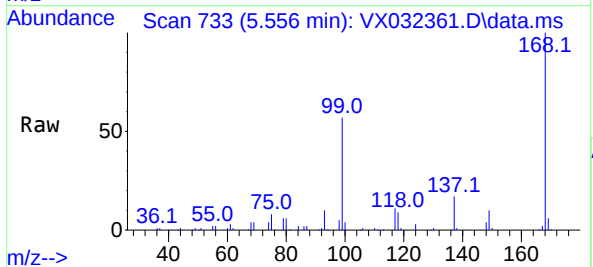



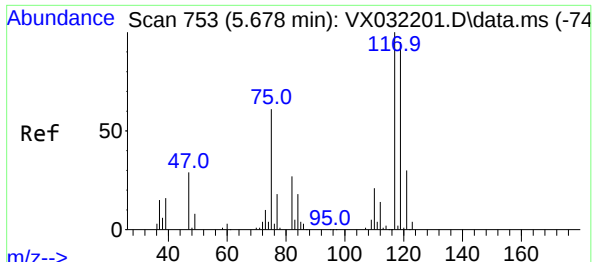


#38
Carbon Tetrachloride
Concen: 7.117 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03


Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME

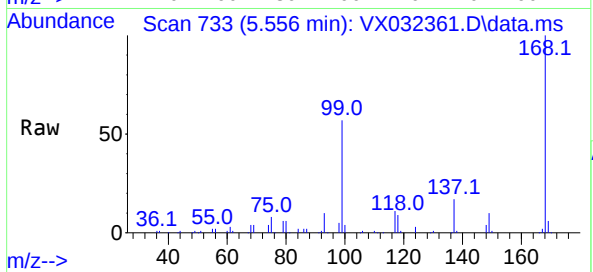



Tgt Ion:117 Resp: 13482
Ion Ratio Lower Upper
117 100
119 5.2 75.4 113.0#
121 0.0 23.9 35.9#

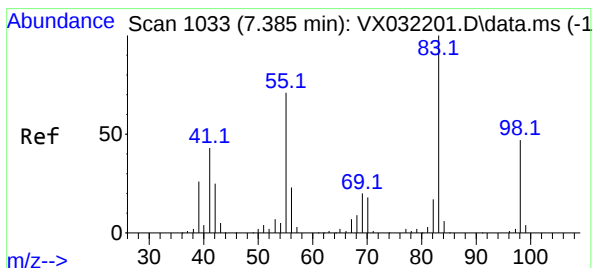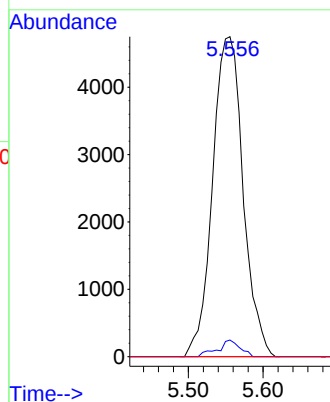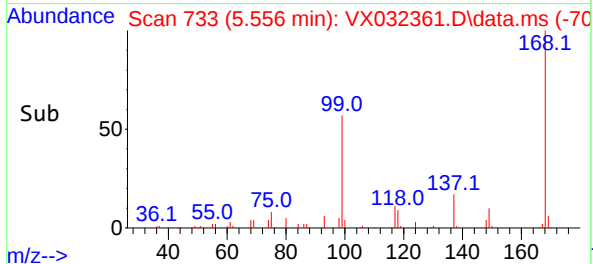


#39
Methylcyclohexane
Concen: 0.255 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03

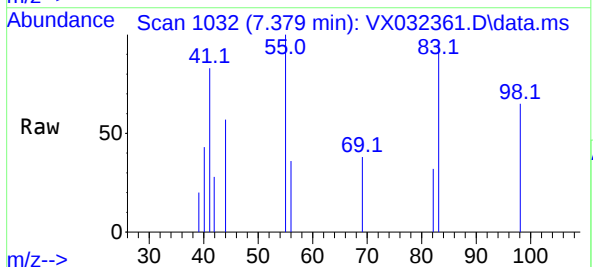

Tgt Ion: 83 Resp: 547
Ion Ratio Lower Upper
83 100
55 105.7 56.6 85.0#
98 69.2 37.4 56.0#

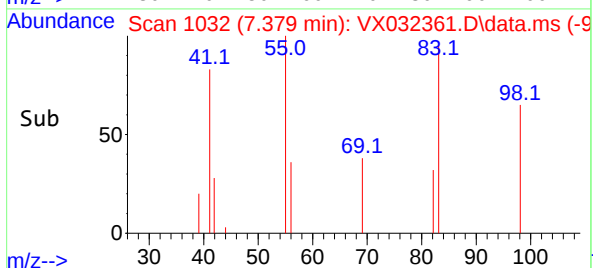

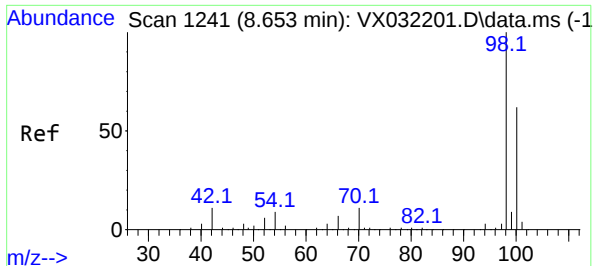

#50

Toluene-d8

Concen: 47.172 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX032361.D

Acq: 25 Oct 2022 14:03

Instrument :

MSVOA_X

ClientSampleId :





BUR-1202ME

Tgt Ion: 98 Resp: 236892

Ion Ratio Lower Upper

98 100

100 63.9 50.7 76.1

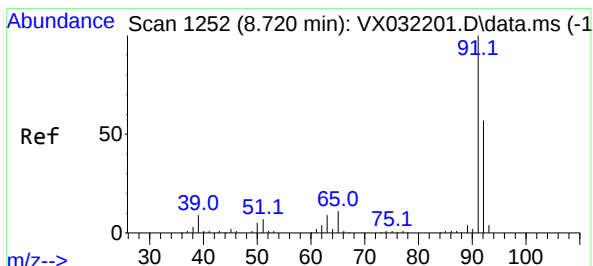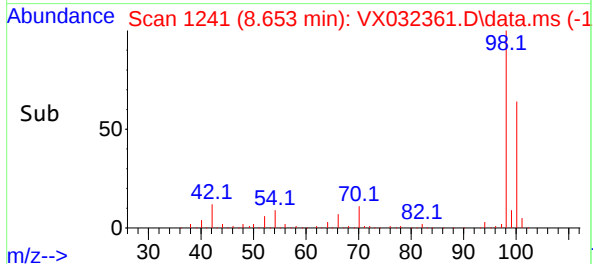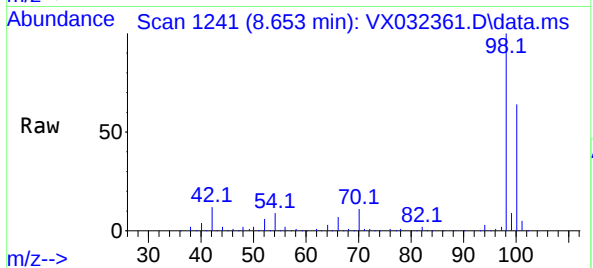

#52

Toluene

Concen: 4.951 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX032361.D




Acq: 25 Oct 2022 14:03


Tgt Ion: 92 Resp: 16683

Ion Ratio Lower Upper

92 100

91 181.1 140.3 210.5

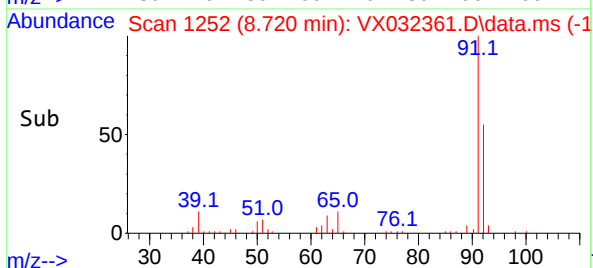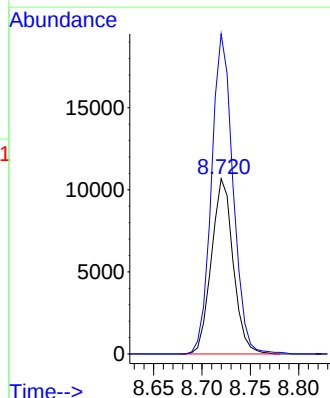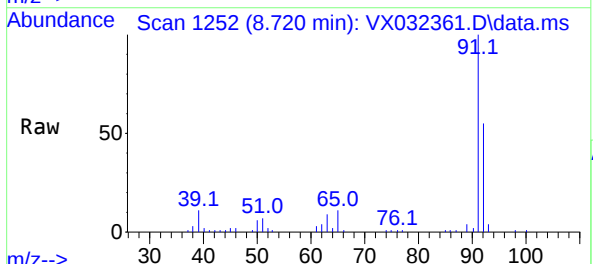

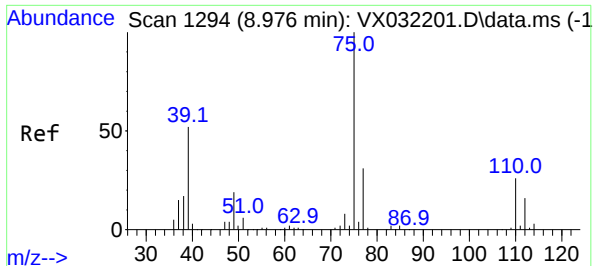

#53

t-1,3-Dichloropropene

Concen: 1.914 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.256 min

Lab File: VX032361.D

Acq: 25 Oct 2022 14:03

Instrument :

MSVOA_X

ClientSampleId :


BUR-1202ME

Tgt Ion: 75 Resp: 202




Ion Ratio Lower Upper

75 100

77 150.6 25.2 37.8#

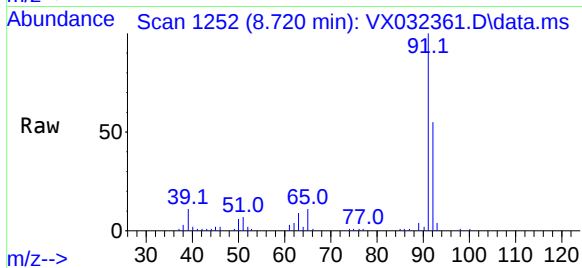

Abundance

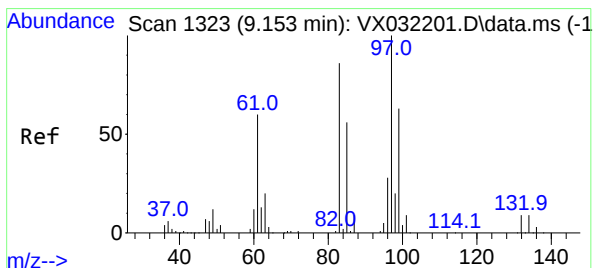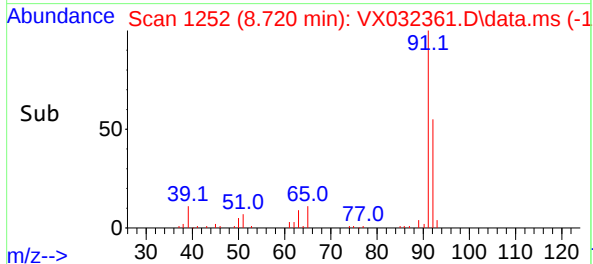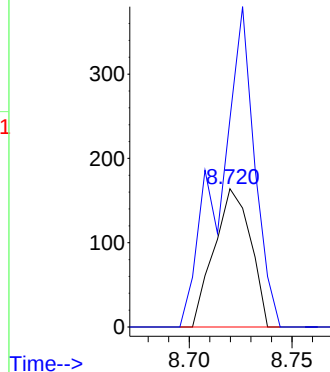

#55

1,1,2-Trichloroethane

Concen: 0.305 ug/l

RT: 9.098 min Scan# 1314

Delta R.T. -0.055 min

Lab File: VX032361.D

Acq: 25 Oct 2022 14:03

Tgt Ion: 97 Resp: 418


Ion Ratio Lower Upper

97 100



83 0.0 68.8 103.2#


85 0.0 44.7 67.1#

99 0.0 50.6 76.0#

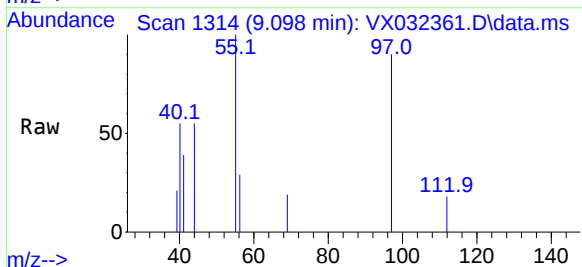

Abundance

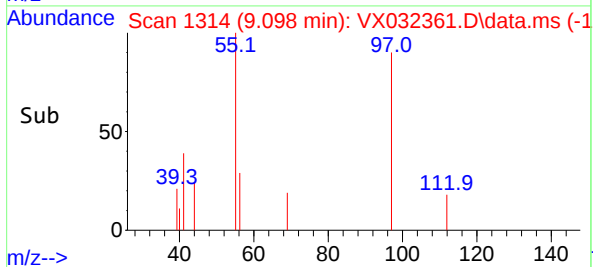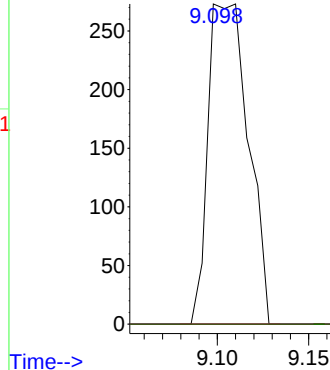

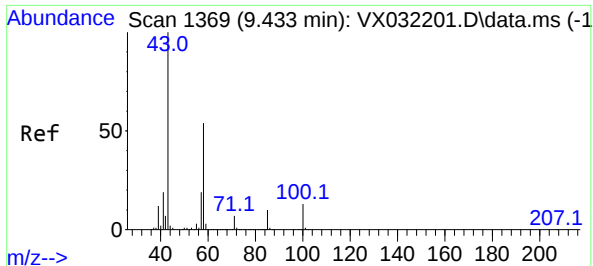

#59

2-Hexanone

Concen: 0.597 ug/l

RT: 9.384 min Scan# 11

Delta R.T. -0.049 min

Lab File: VX032361.D

Acq: 25 Oct 2022 14:03

Instrument :

MSVOA_X

ClientSampleId :





BUR-1202ME

Tgt Ion: 43 Resp: 770

Ion Ratio Lower Upper

43 100

58 0.0 26.7 80.1#

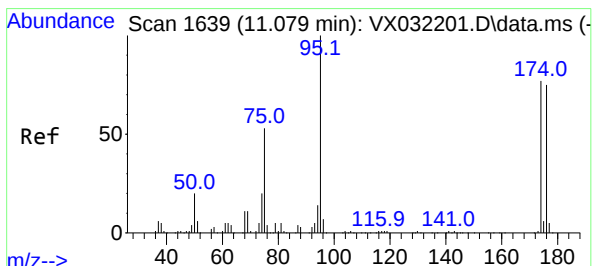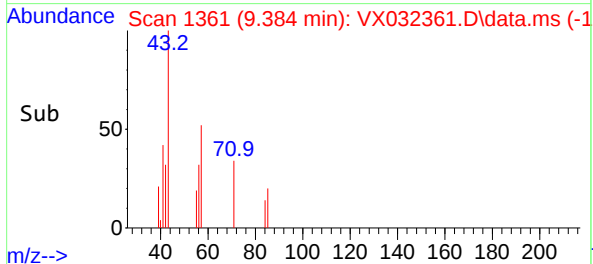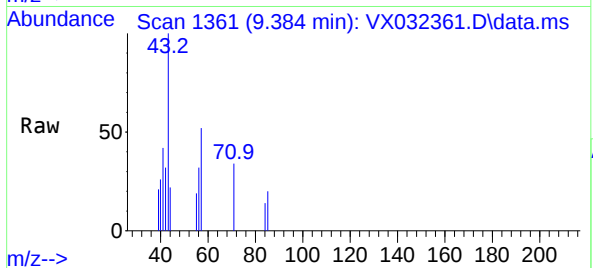

#62

4-Bromofluorobenzene

Concen: 45.274 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX032361.D

Acq: 25 Oct 2022 14:03




Tgt Ion: 95 Resp: 83255


Ion Ratio Lower Upper

95 100

174 81.7 0.0 166.8

176 79.2 0.0 161.4


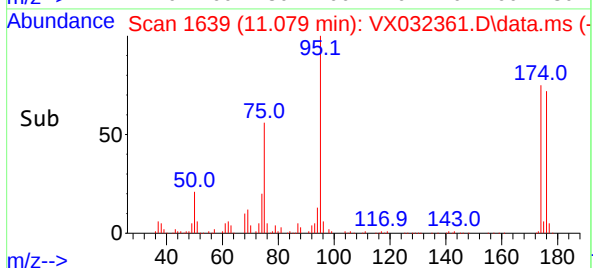
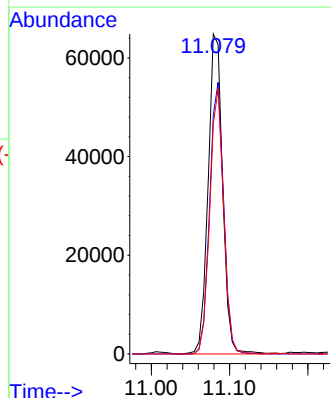
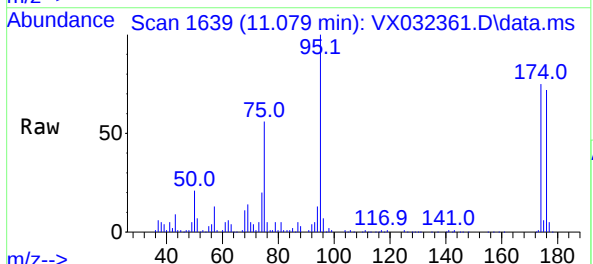




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME


Tgt Ion:117 Resp: 174726
Ion Ratio Lower Upper
117 100
82 54.8 44.2 66.4
119 32.0 25.8 38.8

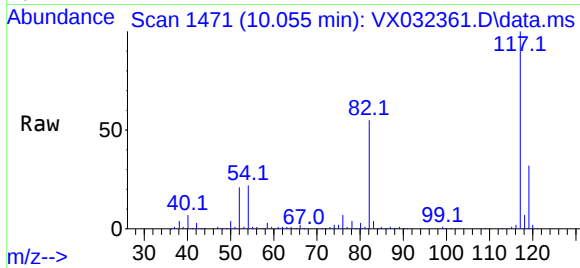

#67
Ethyl Benzene
Concen: 0.804 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03

Tgt Ion: 91 Resp: 5097
Ion Ratio Lower Upper
91 100
106 30.0 25.0 37.4



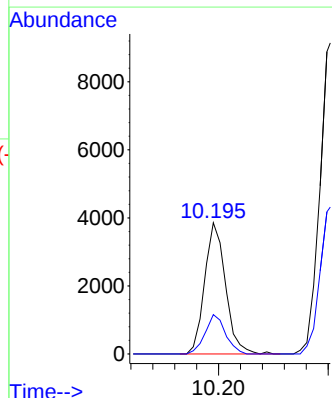
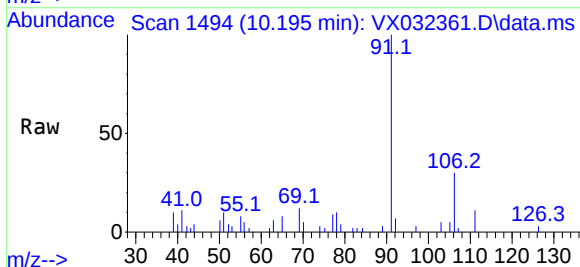




#68
m/p-Xylenes
Concen: 2.528 ug/l
RT: 10.305 min Scan# 1511
Delta R.T. 0.006 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME


Tgt Ion:106 Resp: 6332
Ion Ratio Lower Upper
106 100
91 206.6 162.6 244.0

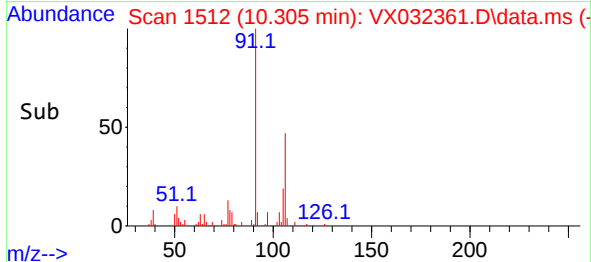

#69
o-Xylene
Concen: 1.423 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03

Tgt Ion:106 Resp: 3415
Ion Ratio Lower Upper
106 100
91 226.5 108.3 324.9


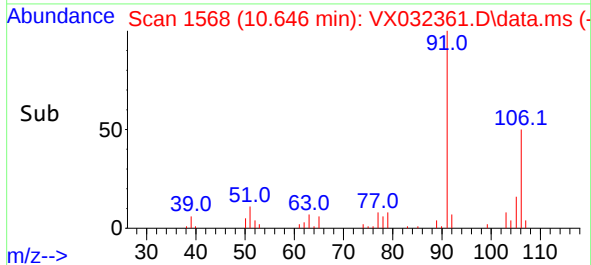

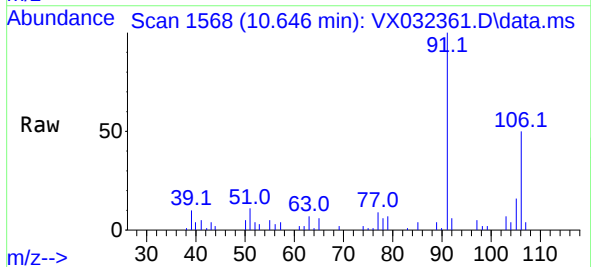




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME


Tgt Ion:152 Resp: 84289
Ion Ratio Lower Upper
152 100
115 59.4 43.1 129.4
150 158.5 0.0 348.6

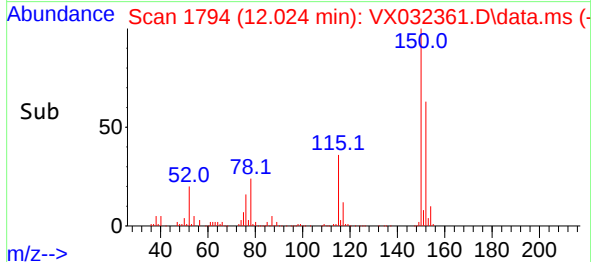

#73
Isopropylbenzene
Concen: 0.551 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.001 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03

Tgt Ion:105 Resp: 3314
Ion Ratio Lower Upper
105 100
120 25.8 13.2 39.6


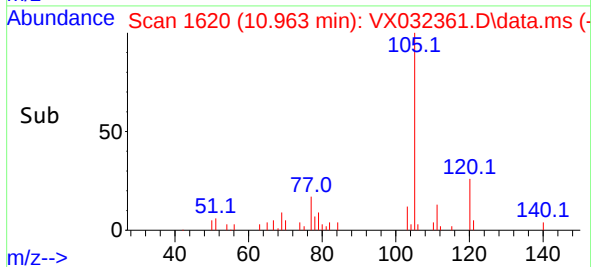

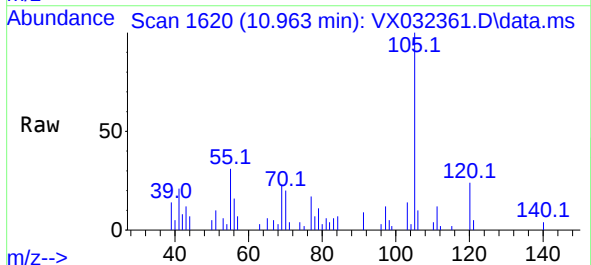




#74
N-amy1 acetate
Concen: 0.989 ug/l
RT: 10.866 min Scan# 1604
Delta R.T. 0.024 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME


Tgt Ion: 43 Resp: 2198
Ion Ratio Lower Upper
43 100
70 113.1 33.9 50.9#
55 392.6 19.1 28.7#
61 0.0 19.0 28.4#

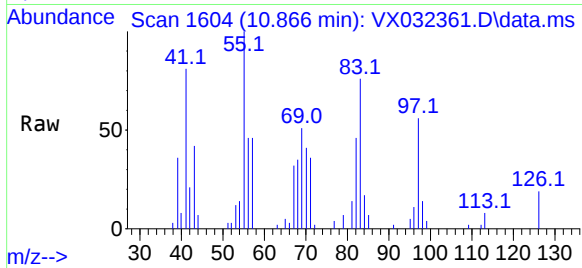

#75
1,1,2,2-Tetrachloroethane
Concen: 0.466 ug/l
RT: 11.219 min Scan# 1662
Delta R.T. 0.005 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03

Tgt Ion: 83 Resp: 901
Ion Ratio Lower Upper
83 100
131 0.0 5.2 15.6#
85 0.0 32.3 96.9#




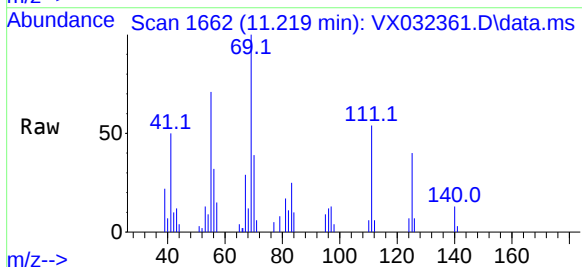




#76
1,2,3-Trichloropropane
Concen: 26.931 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME


Tgt Ion: 75 Resp: 44978
Ion Ratio Lower Upper
75 100
77 1.3 16.0 47.9#

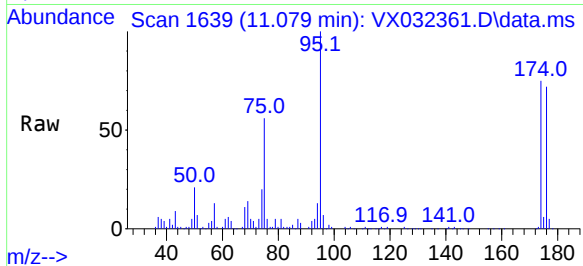

#78
n-propylbenzene
Concen: 1.947 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03

Tgt Ion: 91 Resp: 13408
Ion Ratio Lower Upper
91 100
120 22.2 11.6 34.8


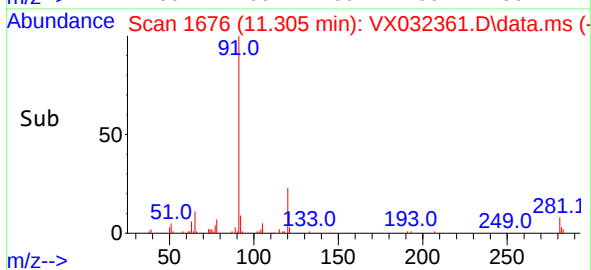

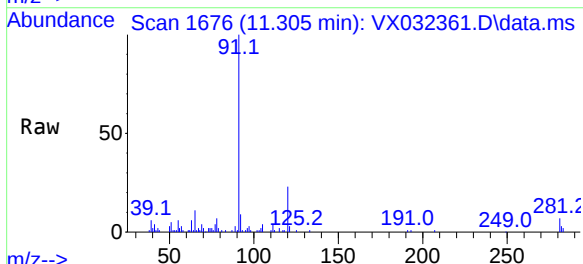




#79
2-Chlorotoluene
Concen: 1.605 ug/l
RT: 11.378 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME


Tgt Ion: 91 Resp: 6662
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#

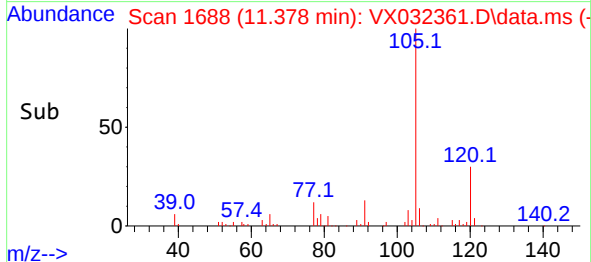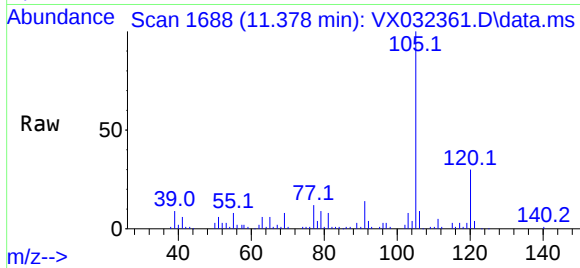

#80
1,3,5-Trimethylbenzene
Concen: 2.927 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03

Tgt Ion: 105 Resp: 15205
Ion Ratio Lower Upper
105 100
120 49.5 23.5 70.6


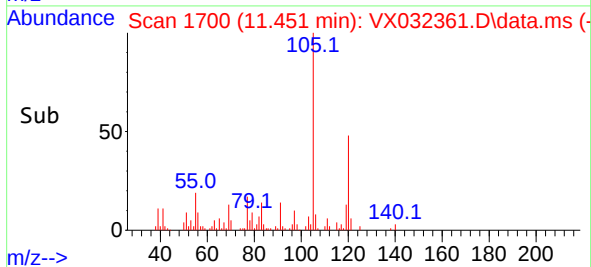

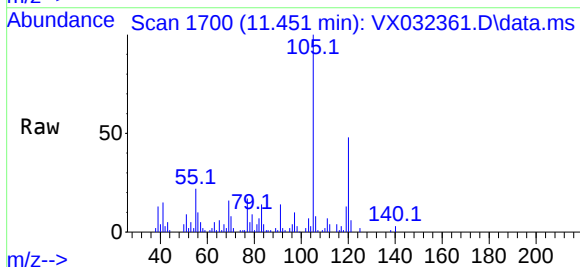




#81
trans-1,4-Dichloro-2-butene
Concen: 82.698 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME


Tgt Ion: 75 Resp: 44978
Ion Ratio Lower Upper
75 100
53 1.5 87.8 131.8#
89 0.0 37.8 56.8#

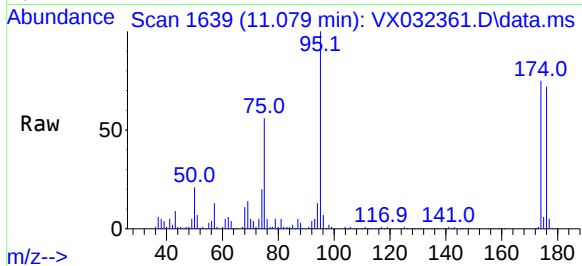

#82
4-Chlorotoluene
Concen: 0.465 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03

Tgt Ion: 91 Resp: 2247
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#


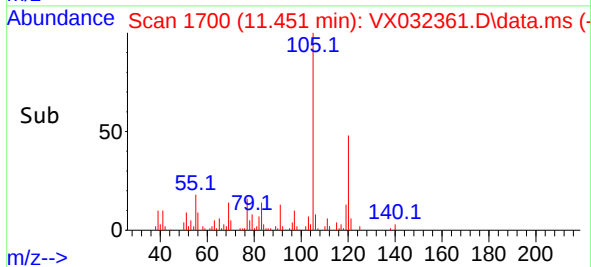

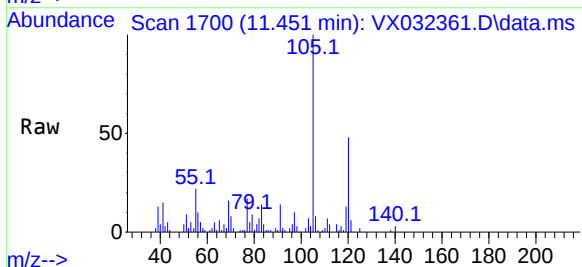




#83
tert-Butylbenzene
Concen: 1.442 ug/l
RT: 11.756 min Scan# 1743
Delta R.T. 0.043 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME


Tgt Ion:119 Resp: 7495
Ion Ratio Lower Upper
119 100
91 100.8 29.1 87.3#
134 0.0 11.3 33.8#

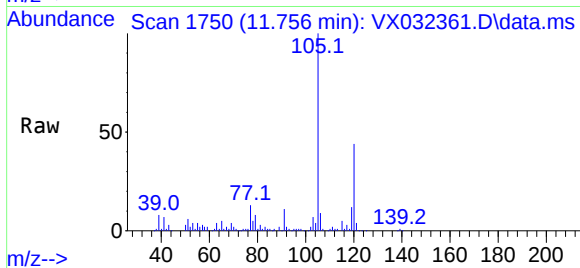

#84
1,2,4-Trimethylbenzene
Concen: 11.900 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03

Tgt Ion:105 Resp: 60103
Ion Ratio Lower Upper
105 100
120 44.0 22.1 66.1


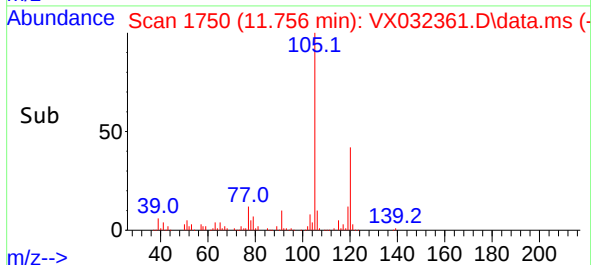
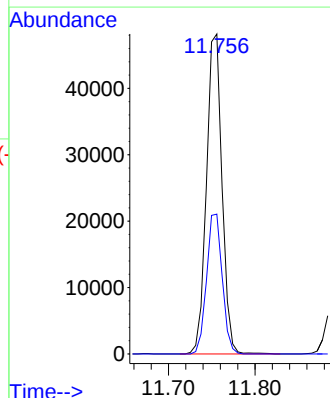
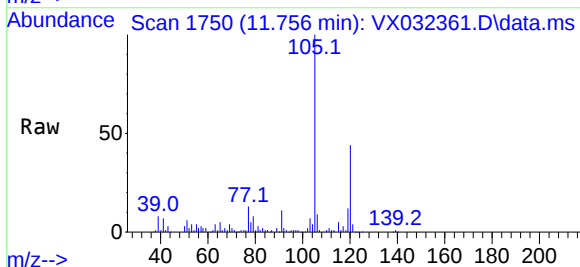




#85
sec-Butylbenzene
Concen: 1.740 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. -0.000 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME


Tgt Ion:105 Resp: 10928
Ion Ratio Lower Upper
105 100
134 24.2 10.1 30.3

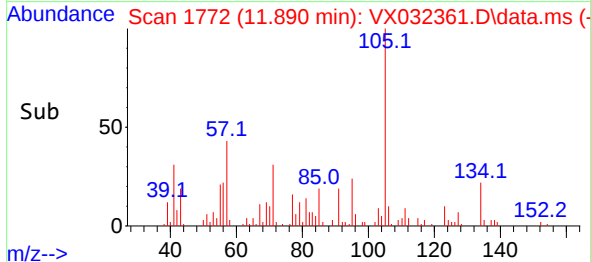

#86
p-Isopropyltoluene
Concen: 1.169 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. -0.000 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03

Tgt Ion:119 Resp: 6248
Ion Ratio Lower Upper
119 100
134 29.1 13.2 39.5
91 30.3 12.4 37.2

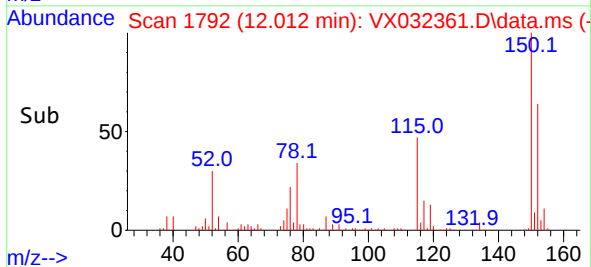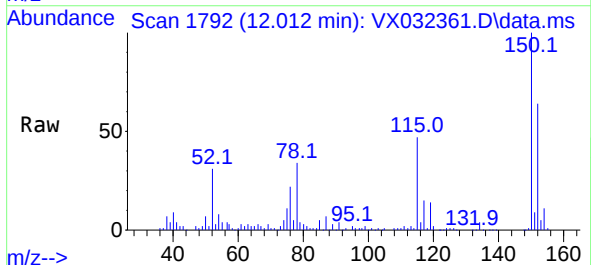



#89

n-Butylbenzene

Concen: 5.269 ug/l

RT: 12.329 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX032361.D

Acq: 25 Oct 2022 14:03

Instrument :

MSVOA_X

ClientSampleId :

BUR-1202ME





Tgt Ion: 91 Resp: 24807

Ion Ratio Lower Upper

91 100

92 36.4 26.3 78.9

134 80.8 13.0 39.0#

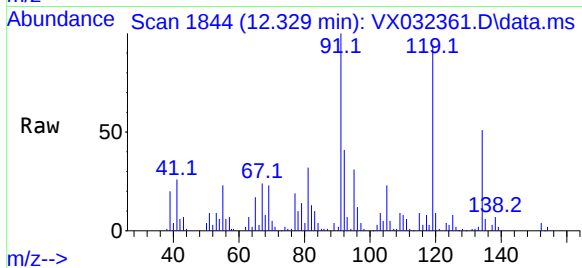

#90

Hexachloroethane

Concen: 3.188 ug/l

RT: 12.555 min Scan# 1881

Delta R.T. 0.012 min

Lab File: VX032361.D




Acq: 25 Oct 2022 14:03


Tgt Ion:117 Resp: 2644

Ion Ratio Lower Upper

117 100

201 0.0 38.5 115.3#


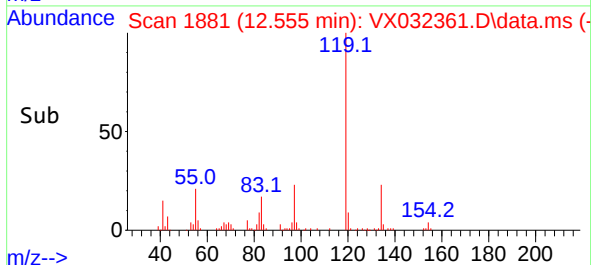
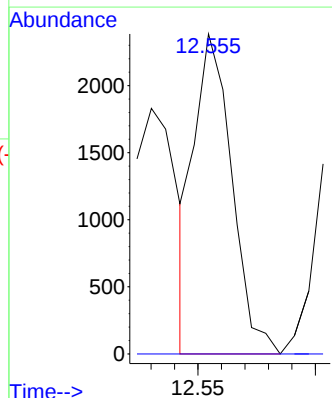
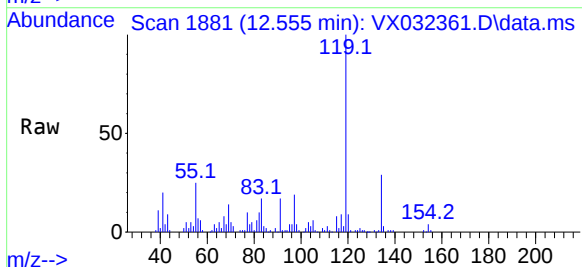


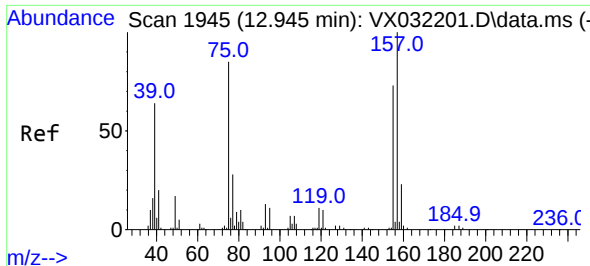

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.698 ug/l
RT: 12.926 min Scan# 1945
Delta R.T. -0.019 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03




Instrument :
MSVOA_X
ClientSampleId :
BUR-1202ME


Tgt Ion: 75 Resp: 258
Ion Ratio Lower Upper
75 100
155 0.0 43.1 129.3#
157 0.0 57.1 171.5#

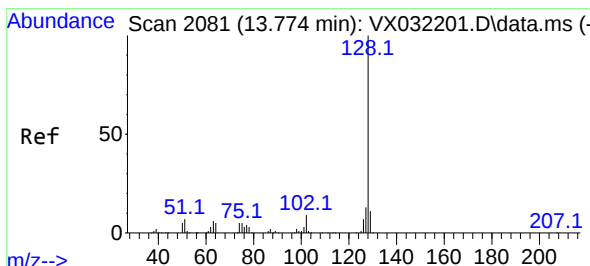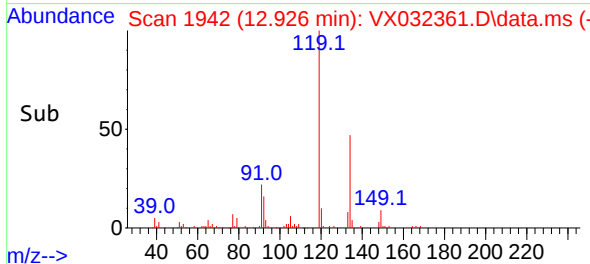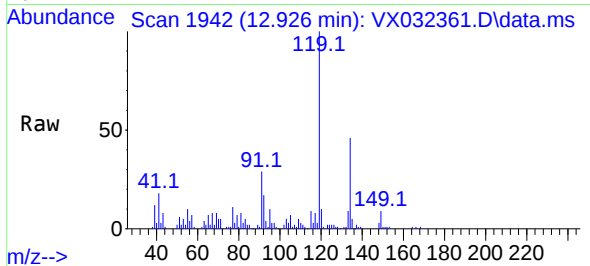

#95
Naphthalene
Concen: 2.418 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX032361.D
Acq: 25 Oct 2022 14:03


Tgt Ion: 128 Resp: 14042
Ion Ratio Lower Upper
128 100
127 15.5 10.3 15.5#
129 17.3 8.7 13.1#

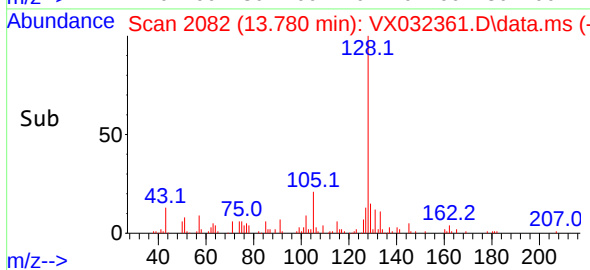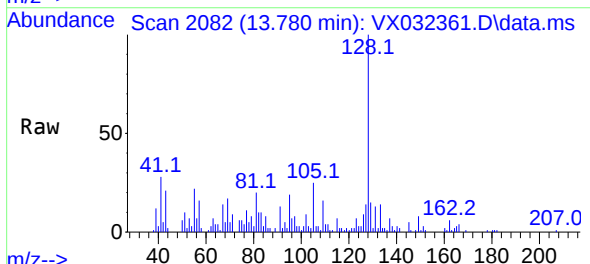



#96
 1,2,3-Trichlorobenzene
 Concen: 0.436 ug/l
 RT: 13.975 min Scan# 2114
 Delta R.T. 0.012 min
 Lab File: VX032361.D
 Acq: 25 Oct 2022 14:03

Instrument :
 MSVOA_X
 ClientSampleId :
 BUR-1202ME



Tgt Ion:180 Resp: 795
 Ion Ratio Lower Upper
 180 100
 182 40.1 47.4 142.2#
 145 883.1 16.5 49.5#

