

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
 Data File : VX032390.D
 Acq On : 26 Oct 2022 01:42
 Operator : JC/MD
 Sample : N5267-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP3-1024

Quant Time: Oct 27 14:21:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
 Quant Title : SW846 8260
 QLast Update : Sat Oct 22 04:56:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	129742	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	206573	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	184947	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	85548	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	82911	49.123	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	98.240%		
35) Dibromofluoromethane	5.385	113	66406	46.196	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	92.400%		
50) Toluene-d8	8.653	98	248851	48.092	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	96.180%		
62) 4-Bromofluorobenzene	11.079	95	84854	44.782	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	89.560%		
Target Compounds						
					Qvalue	
3) Chloromethane	1.288	50	458	Below Cal	#	44
6) Chloroethane	1.660	64	20	1.968	ug/l #	41
11) Tert butyl alcohol	2.953	59	1006	Below Cal	#	74
13) Acrolein	2.239	56	146	0.711	ug/l	97
16) Acetone	2.380	43	15514	28.324	ug/l	94
18) Methyl Acetate	2.703	43	1245	0.670	ug/l #	83
20) Methylene Chloride	2.794	84	6907	4.911	ug/l	97
25) 2-Butanone	4.568	43	2501	2.925	ug/l #	87
29) Tetrahydrofuran	5.032	42	195	0.353	ug/l #	48
31) Cyclohexane	5.550	56	2853	1.479	ug/l #	17
36) 1,1-Dichloropropene	5.556	75	10050	5.435	ug/l #	50
37) Ethyl Acetate	4.721	43	16357	9.035	ug/l	98
38) Carbon Tetrachloride	5.550	117	13131	6.727	ug/l #	18
41) Methacrylonitrile	5.019	41	198	0.207	ug/l #	26
43) Isopropyl Acetate	6.342	43	68257	24.021	ug/l	99
48) Methyl methacrylate	7.799	41	63158	44.567	ug/l #	43
49) 1,4-Dioxane	7.805	88	25	0.879	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	55756	31.302	ug/l #	49
53) t-1,3-Dichloropropene	8.952	75	364	1.986	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	24393	11.752	ug/l #	67
56) Ethyl methacrylate	9.244	69	494	0.243	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	3000	1.313	ug/l #	42
59) 2-Hexanone	9.482	43	44241	33.287	ug/l #	51
73) Isopropylbenzene	10.963	105	1232	0.202	ug/l	90
74) N-amyl acetate	10.640	43	14786	6.557	ug/l #	52
76) 1,2,3-Trichloropropane	11.079	75	46098	27.195	ug/l #	45
81) trans-1,4-Dichloro-2-b...	11.079	75	46098	83.482	ug/l #	6
85) sec-Butylbenzene	11.890	105	2125	0.333	ug/l	96
86) p-Isopropyltoluene	12.183	119	2473	0.456	ug/l	94
89) n-Butylbenzene	12.335	91	1009	0.211	ug/l #	48
90) Hexachloroethane	12.616	117	1673	1.987	ug/l #	11
92) 1,2-Dibromo-3-Chloropr...	12.920	75	110	0.293	ug/l #	1
95) Naphthalene	13.780	128	9215	1.563	ug/l #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
TP3-1024

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
Data File : VX032390.D
Acq On : 26 Oct 2022 01:42
Operator : JC/MD
Sample : N5267-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP3-1024

Quant Time: Oct 27 14:21:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260
QLast Update : Sat Oct 22 04:56:40 2022
Response via : Initial Calibration




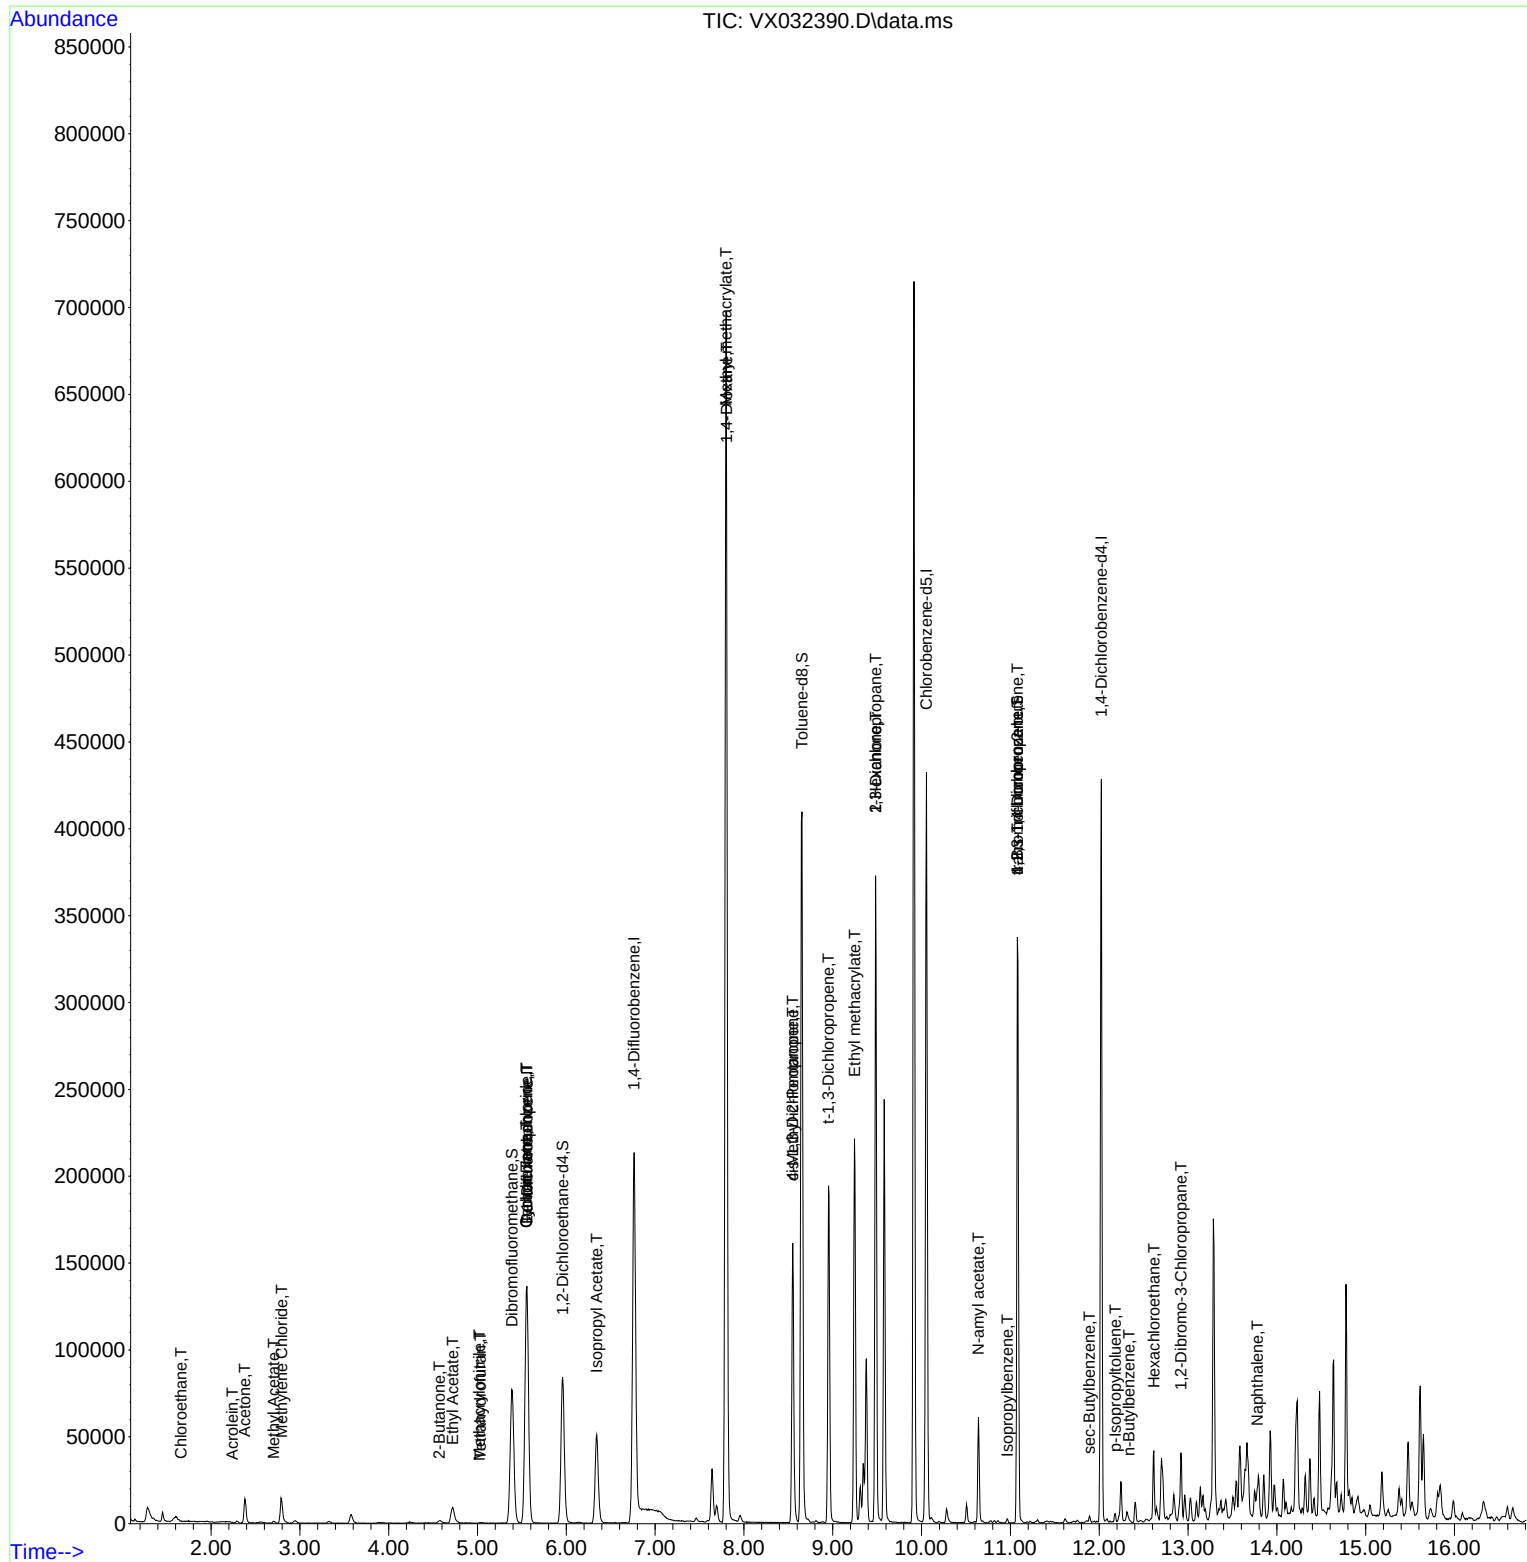




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion:168 Resp: 129742
Ion Ratio Lower Upper
168 100
99 57.2 44.8 67.2



#3
Chloromethane
Concen: Below Cal
RT: 1.288 min Scan# 33
Delta R.T. -0.007 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion: 50 Resp: 458
Ion Ratio Lower Upper
50 100
52 0.0 24.7 37.1#


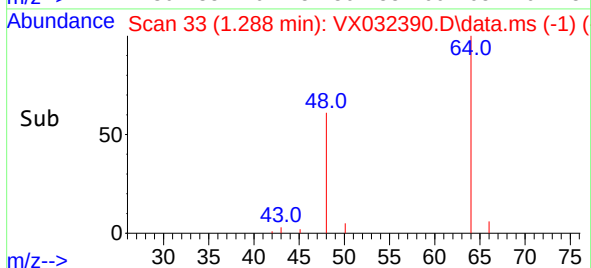




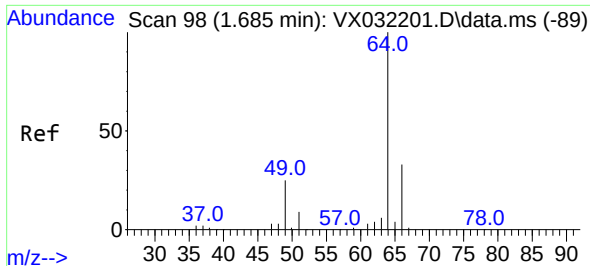

#6
Chloroethane
Concen: 1.968 ug/l
RT: 1.660 min Scan# 94
Delta R.T. -0.025 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024

Tgt Ion: 64 Resp: 20
Ion Ratio Lower Upper
64 100
66 0.0 26.6 39.8#

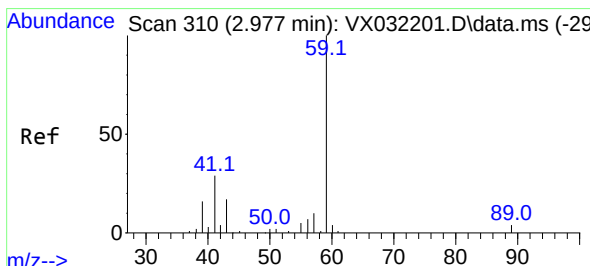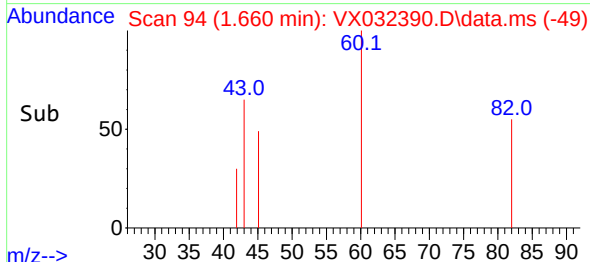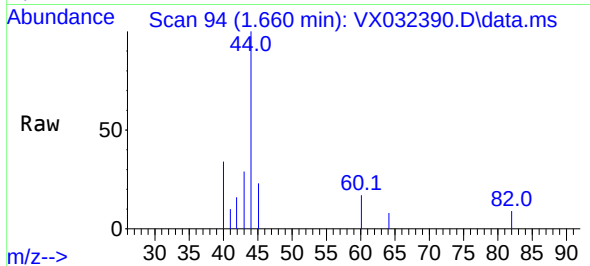


#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.953 min Scan# 306
Delta R.T. -0.024 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion: 59 Resp: 1006
Ion Ratio Lower Upper
59 100
57 0.0 7.5 11.3#

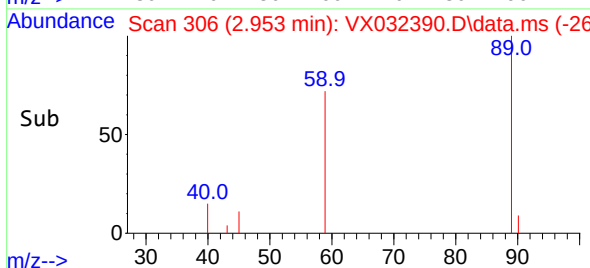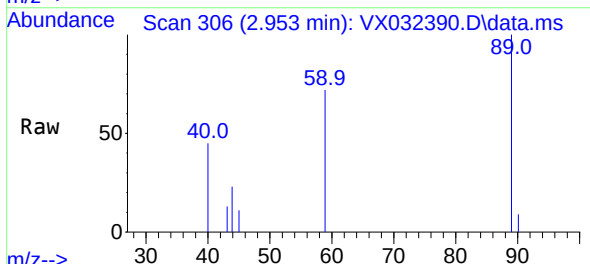

Abundance Scan 188 (2.233 min): VX032201.D\data.ms (-18

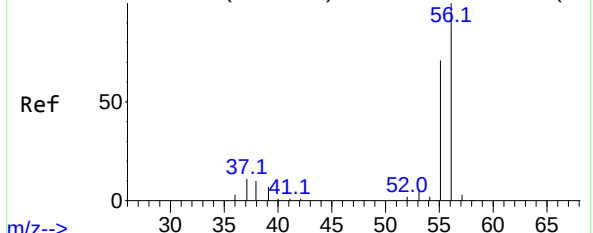

#13

Acrolein

Concen: 0.711 ug/l

RT: 2.239 min Scan# 189

Delta R.T. 0.006 min

Lab File: VX032390.D

Acq: 26 Oct 2022 01:42

Instrument :

MSVOA_X

ClientSampleId :

TP3-1024


Tgt Ion: 56 Resp: 146

Ion Ratio Lower Upper


56 100

55 67.8 56.4 84.6


Abundance Scan 189 (2.239 min): VX032390.D\data.ms

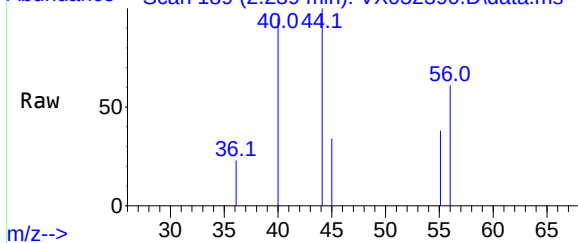


Abundance

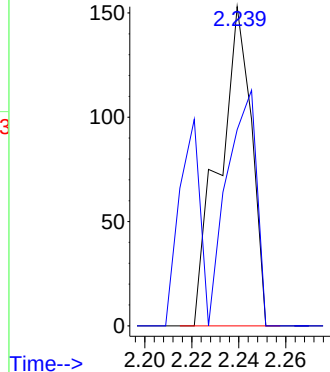

Abundance Scan 189 (2.239 min): VX032390.D\data.ms (-13

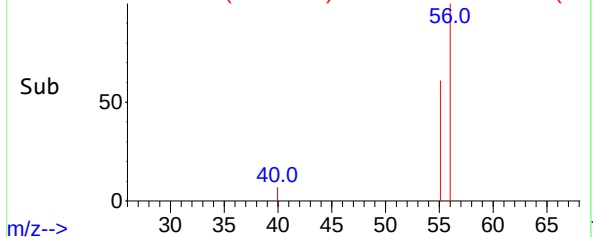

Abundance Scan 212 (2.380 min): VX032201.D\data.ms (-20

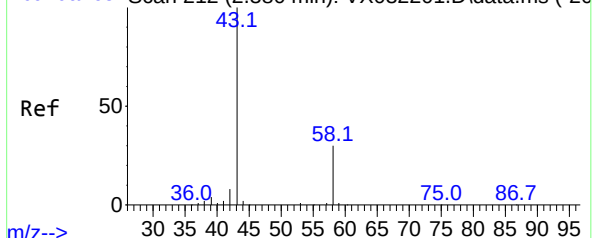

#16

Acetone

Concen: 28.324 ug/l

RT: 2.380 min Scan# 212

Delta R.T. -0.000 min

Lab File: VX032390.D

Acq: 26 Oct 2022 01:42


Tgt Ion: 43 Resp: 15514

Ion Ratio Lower Upper


43 100

58 27.0 24.2 36.2


Abundance Scan 212 (2.380 min): VX032390.D\data.ms

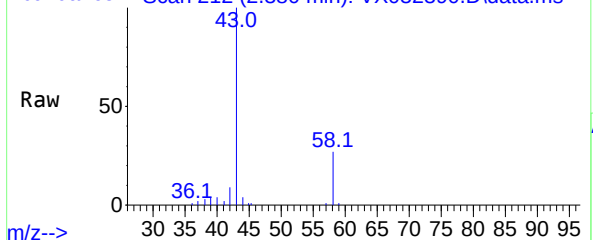


Abundance

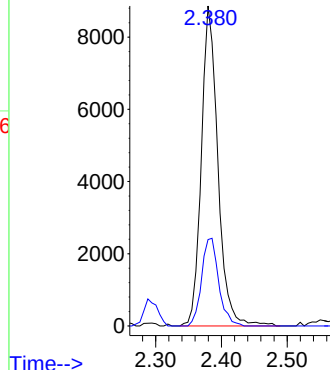

Abundance Scan 212 (2.380 min): VX032390.D\data.ms (-16




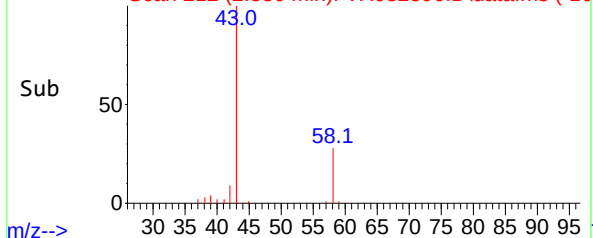




#18
Methyl Acetate
Concen: 0.670 ug/l
RT: 2.703 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion: 43 Resp: 1245
Ion Ratio Lower Upper
43 100
74 16.3 19.8 29.8#

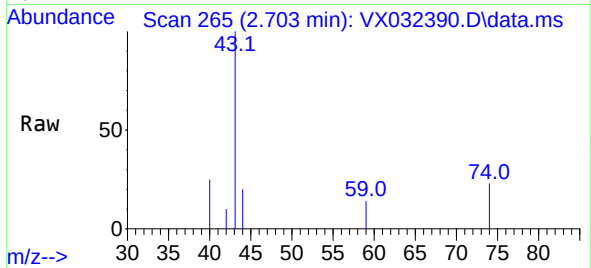

#20
Methylene Chloride
Concen: 4.911 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.006 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion: 84 Resp: 6907
Ion Ratio Lower Upper
84 100
49 112.1 92.6 139.0
51 33.8 29.2 43.8
86 61.9 51.4 77.0

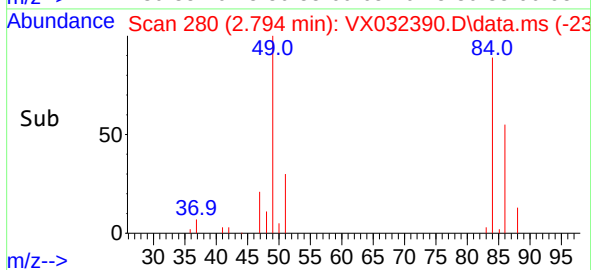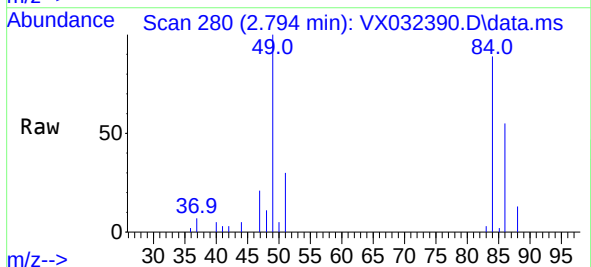



#25

2-Butanone

Concen: 2.925 ug/l

RT: 4.568 min Scan# 51

Delta R.T. 0.012 min

Lab File: VX032390.D

Acq: 26 Oct 2022 01:42

Instrument :

MSVOA_X

ClientSampleId :





TP3-1024

Tgt Ion: 43 Resp: 2501

Ion Ratio Lower Upper

43 100

72 20.2 21.7 32.5#

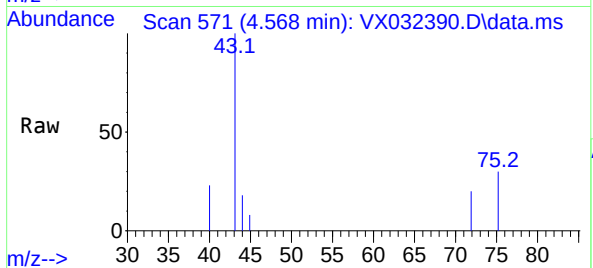

#29

Tetrahydrofuran

Concen: 0.353 ug/l

RT: 5.032 min Scan# 647

Delta R.T. 0.025 min

Lab File: VX032390.D

Acq: 26 Oct 2022 01:42




Tgt Ion: 42 Resp: 195


Ion Ratio Lower Upper

42 100

72 0.0 37.5 56.3#


71 23.1 34.7 52.1#

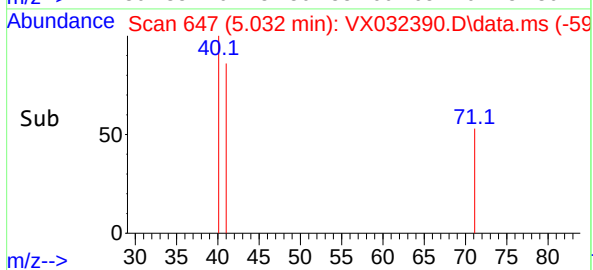






#31
Cyclohexane
Concen: 1.479 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.073 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Instrument :
MSVOA_X
ClientSampleId :
TP3-1024



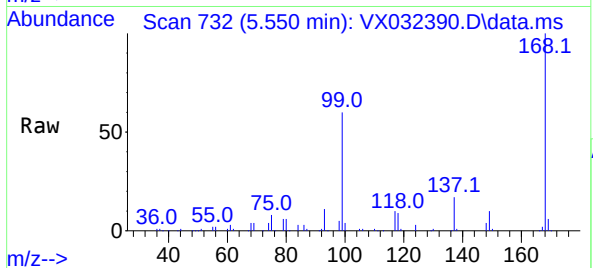



Tgt Ion: 56 Resp: 2853
Ion Ratio Lower Upper
56 100
69 164.6 25.4 38.0#
84 114.8 71.2 106.8#



#33
1,2-Dichloroethane-d4
Concen: 49.123 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion: 65 Resp: 82911
Ion Ratio Lower Upper
65 100
67 50.3 0.0 103.6


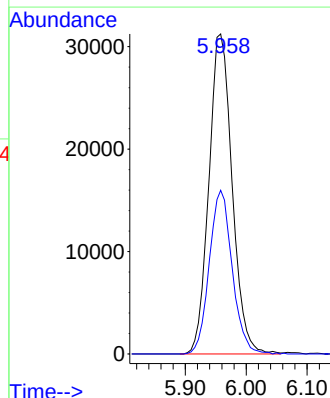
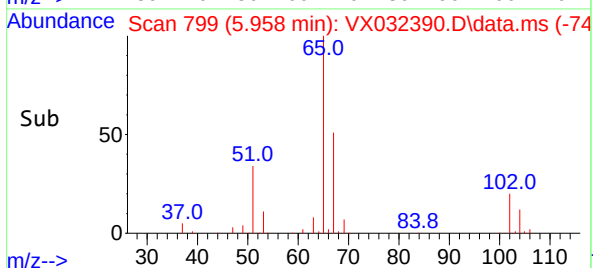





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion:114 Resp: 206573
Ion Ratio Lower Upper
114 100
63 19.2 0.0 38.6
88 15.1 0.0 32.6

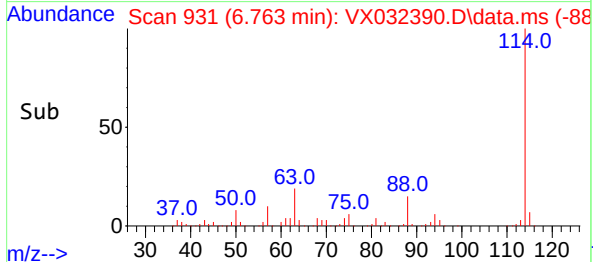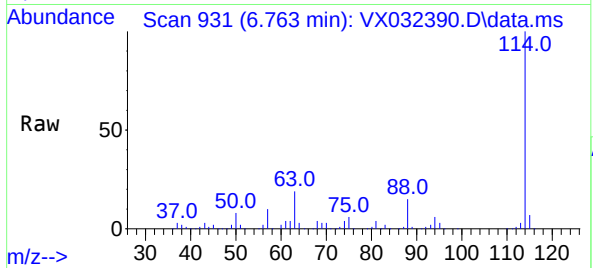

#35
Dibromofluoromethane
Concen: 46.196 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion:113 Resp: 66406
Ion Ratio Lower Upper
113 100
111 102.1 82.8 124.2
192 19.4 15.5 23.3


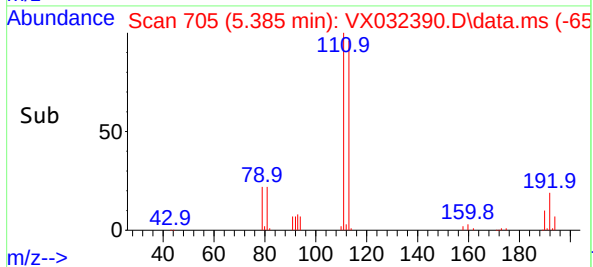

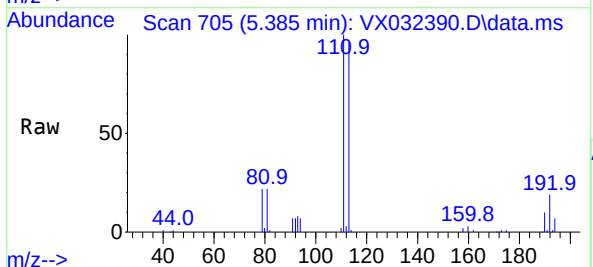


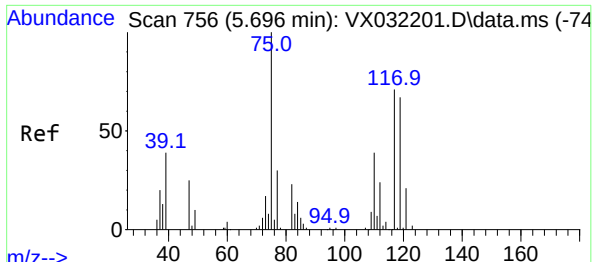

#36
1,1-Dichloropropene
Concen: 5.435 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion: 75 Resp: 10050
Ion Ratio Lower Upper
75 100
110 10.2 18.4 55.0#
77 0.0 24.7 37.1#

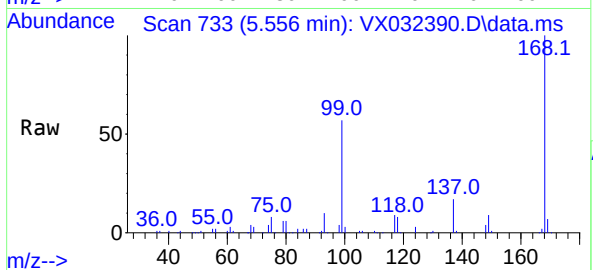

#37
Ethyl Acetate
Concen: 9.035 ug/l
RT: 4.721 min Scan# 596
Delta R.T. 0.006 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42


Tgt Ion: 43 Resp: 16357
Ion Ratio Lower Upper
43 100
61 13.6 11.4 17.2
70 10.4 8.8 13.2

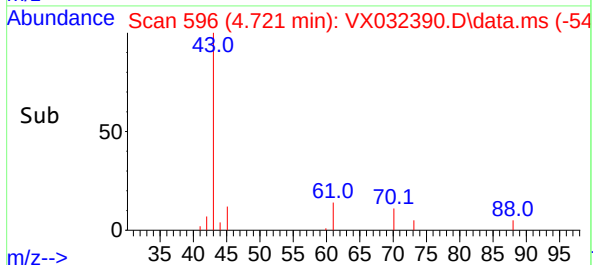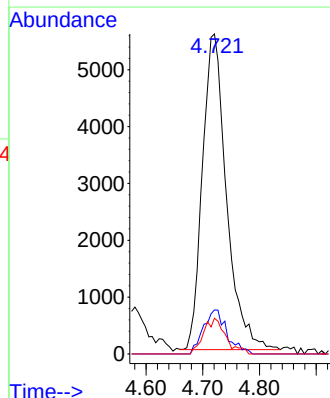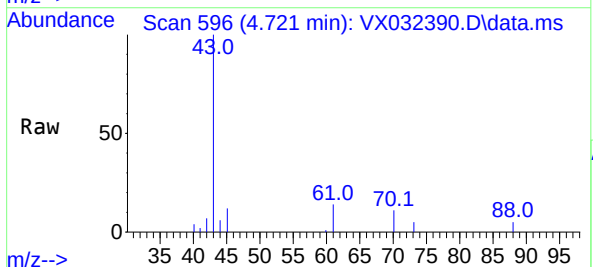



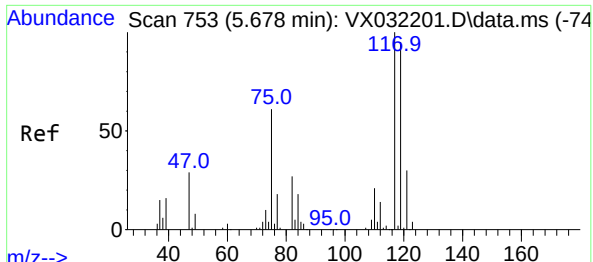


#38
Carbon Tetrachloride
Concen: 6.727 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Instrument :
MSVOA_X
ClientSampleId :
TP3-1024



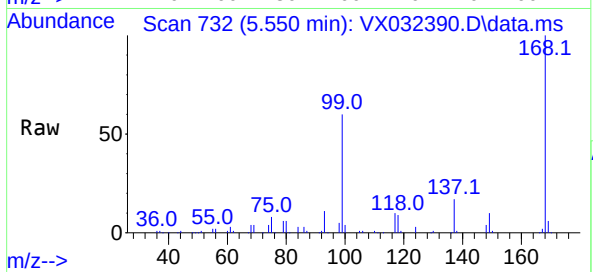



Tgt Ion:117 Resp: 13131
Ion Ratio Lower Upper
117 100
119 7.1 75.4 113.0#
121 0.0 23.9 35.9#

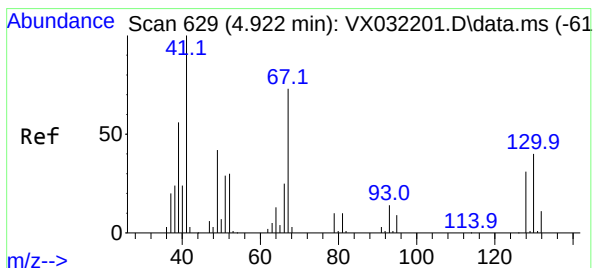

#41
Methacrylonitrile
Concen: 0.207 ug/l
RT: 5.019 min Scan# 645
Delta R.T. 0.097 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion: 41 Resp: 198
Ion Ratio Lower Upper
41 100
39 9.6 45.5 68.3#
67 0.0 59.4 89.2#
52 0.0 25.3 37.9#


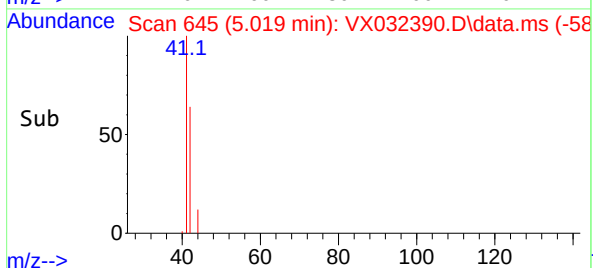
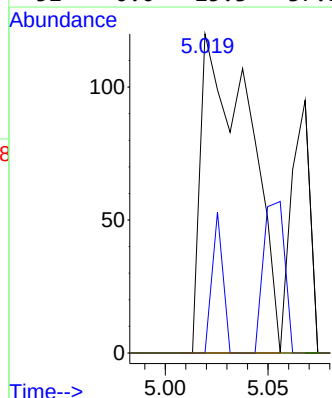
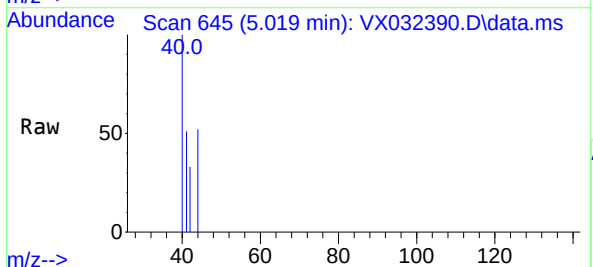




#43
Isopropyl Acetate
Concen: 24.021 ug/l
RT: 6.342 min Scan# 81
Delta R.T. 0.000 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion: 43 Resp: 68257
Ion Ratio Lower Upper
43 100
61 19.1 15.5 23.3
87 13.6 11.0 16.6

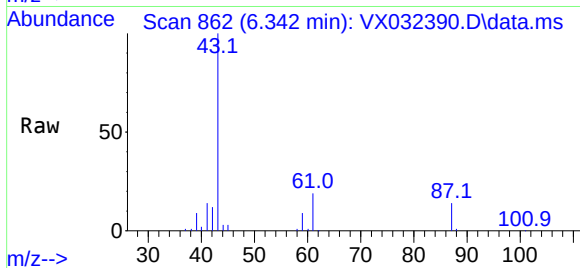

#48
Methyl methacrylate
Concen: 44.567 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.109 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion: 41 Resp: 63158
Ion Ratio Lower Upper
41 100
69 0.1 67.3 100.9#
39 56.9 53.8 80.8

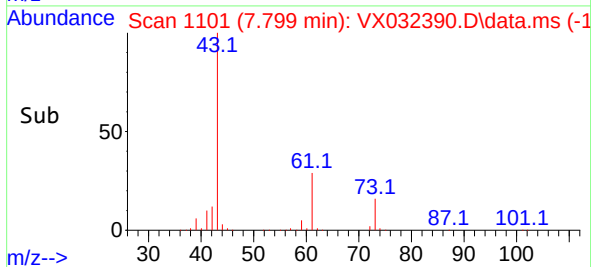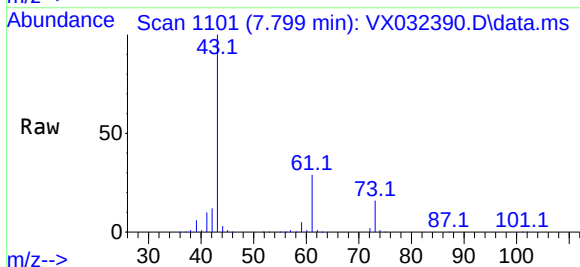



#49

1,4-Dioxane

Concen: 0.879 ug/l

RT: 7.805 min Scan# 1102

Delta R.T. 0.115 min

Lab File: VX032390.D

Acq: 26 Oct 2022 01:42

Instrument :

MSVOA_X

ClientSampleId :

TP3-1024





Tgt Ion: 88 Resp: 25

Ion Ratio Lower Upper

88 100

43 2470856.0 26.9 40.3#

58 11104.0 50.7 76.1#

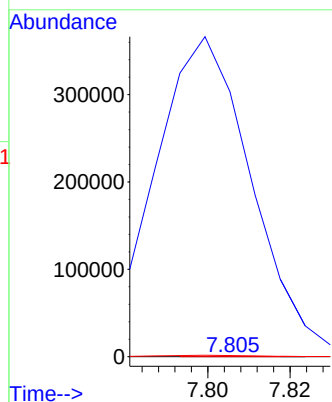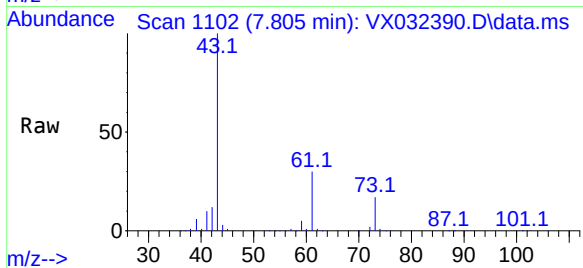

#50

Toluene-d8

Concen: 48.092 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX032390.D




Acq: 26 Oct 2022 01:42


Tgt Ion: 98 Resp: 248851

Ion Ratio Lower Upper

98 100

100 63.4 50.7 76.1


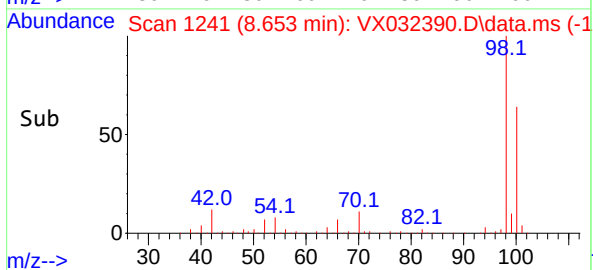

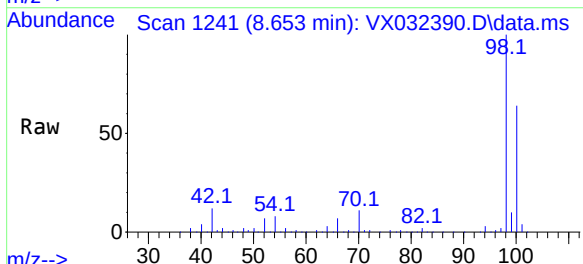




#51
4-Methyl-2-Pentanone
Concen: 31.302 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.025 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion: 43 Resp: 55756
Ion Ratio Lower Upper
43 100
58 7.4 31.0 46.4#

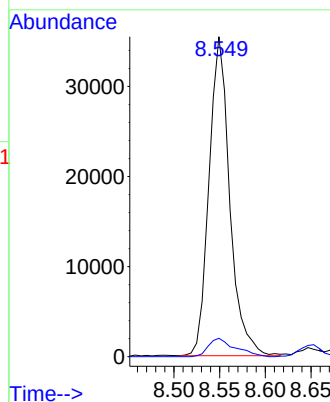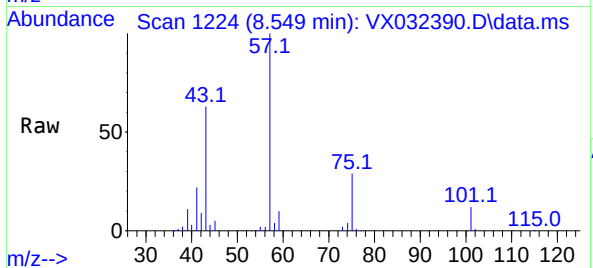

#53
t-1,3-Dichloropropene
Concen: 1.986 ug/l
RT: 8.952 min Scan# 1290
Delta R.T. -0.024 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion: 75 Resp: 364
Ion Ratio Lower Upper
75 100
77 0.0 25.2 37.8#

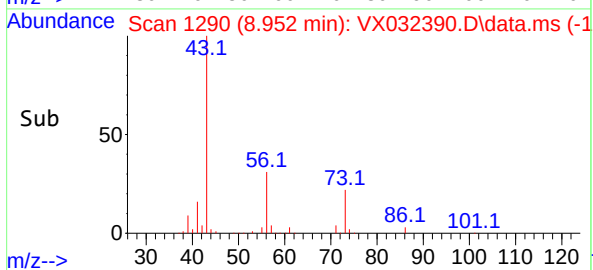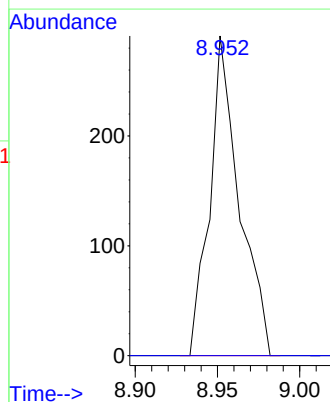



#54

cis-1,3-Dichloropropene

Concen: 11.752 ug/l

RT: 8.549 min Scan# 11

Delta R.T. 0.183 min

Lab File: VX032390.D

Acq: 26 Oct 2022 01:42

Instrument :

MSVOA_X

ClientSampleId :

TP3-1024





Tgt Ion: 75 Resp: 24393

Ion Ratio Lower Upper

75 100

77 0.4 25.3 37.9#

39 39.2 42.4 63.6#

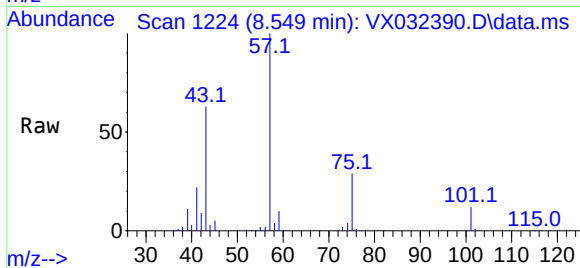

#56

Ethyl methacrylate

Concen: 0.243 ug/l

RT: 9.244 min Scan# 1338

Delta R.T. 0.128 min

Lab File: VX032390.D

Acq: 26 Oct 2022 01:42




Tgt Ion: 69 Resp: 494


Ion Ratio Lower Upper

69 100

41 7531.8 54.5 81.7#

39 3395.7 35.7 53.5#


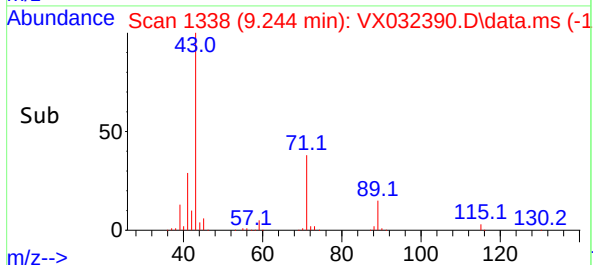
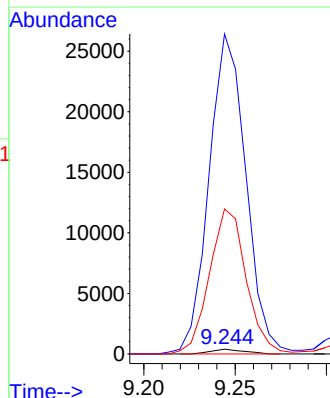
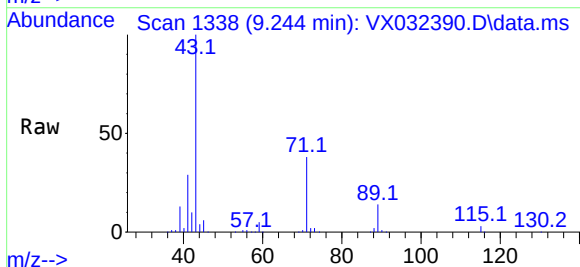




#57
1,3-Dichloropropane
Concen: 1.313 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.177 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion: 76 Resp: 3000
Ion Ratio Lower Upper
76 100
78 0.0 26.0 39.0#

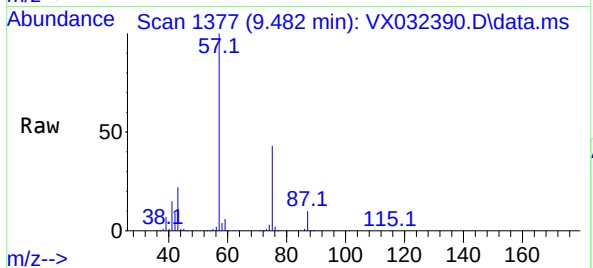

#59
2-Hexanone
Concen: 33.287 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.049 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion: 43 Resp: 44241
Ion Ratio Lower Upper
43 100
58 18.7 26.7 80.1#


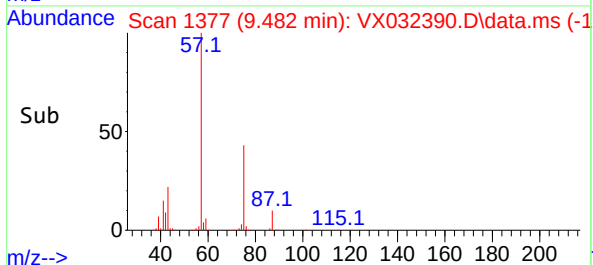

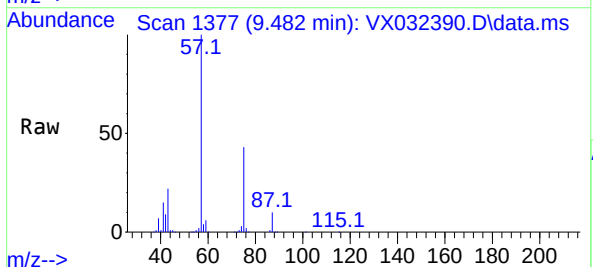




#62
4-Bromofluorobenzene
Concen: 44.782 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion: 95 Resp: 84854
Ion Ratio Lower Upper
95 100
174 82.4 0.0 166.8
176 80.9 0.0 161.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion: 117 Resp: 184947
Ion Ratio Lower Upper
117 100
82 54.8 44.2 66.4
119 31.9 25.8 38.8


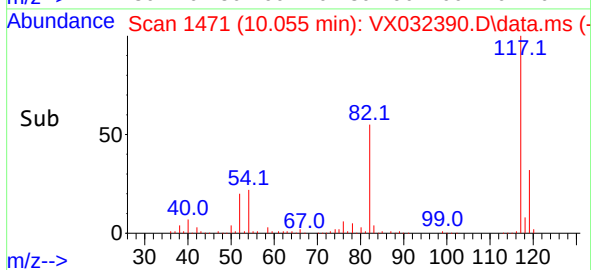






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion:152 Resp: 85548
Ion Ratio Lower Upper
152 100
115 60.3 43.1 129.4
150 157.3 0.0 348.6

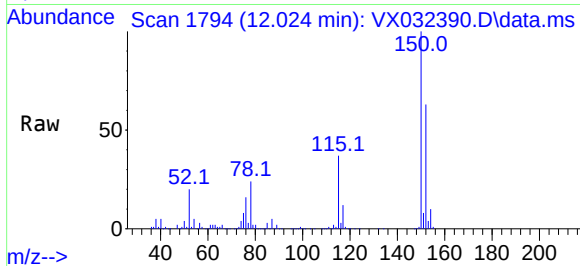

#73
Isopropylbenzene
Concen: 0.202 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.001 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion:105 Resp: 1232
Ion Ratio Lower Upper
105 100
120 31.6 13.2 39.6


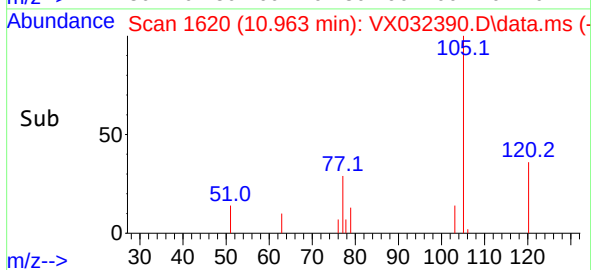

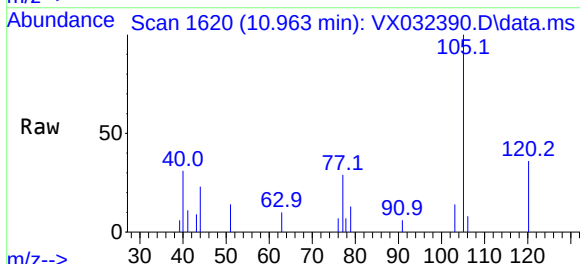




#74
N-amy1 acetate
Concen: 6.557 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.202 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion:	43	Resp:	14786
Ion	Ratio	Lower	Upper
43	100		
70	2.1	33.9	50.9#
55	4.4	19.1	28.7#
61	9.7	19.0	28.4#

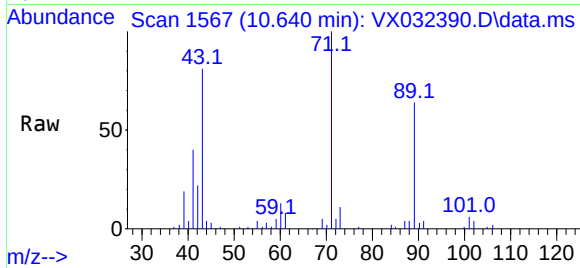

#76
1,2,3-Trichloropropane
Concen: 27.195 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion:	75	Resp:	46098
Ion	Ratio	Lower	Upper
75	100		
77	1.2	16.0	47.9#


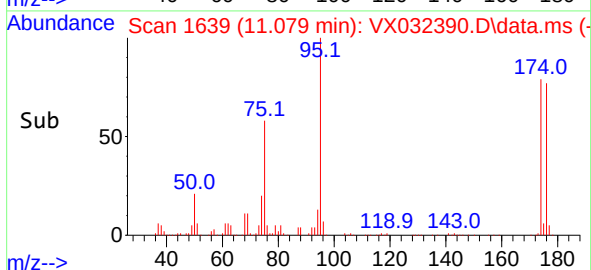

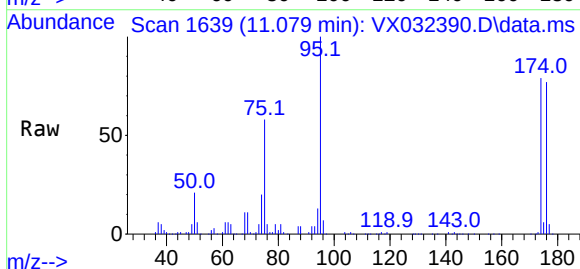




#81
trans-1,4-Dichloro-2-butene
Concen: 83.482 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion: 75 Resp: 46098
Ion Ratio Lower Upper
75 100
53 0.0 87.8 131.8#
89 0.0 37.8 56.8#

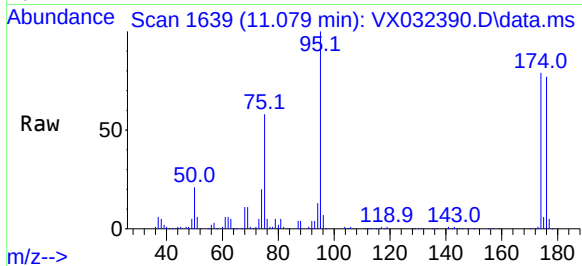

#85
sec-Butylbenzene
Concen: 0.333 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion: 105 Resp: 2125
Ion Ratio Lower Upper
105 100
134 22.1 10.1 30.3


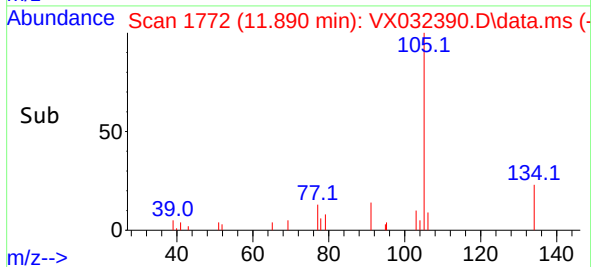

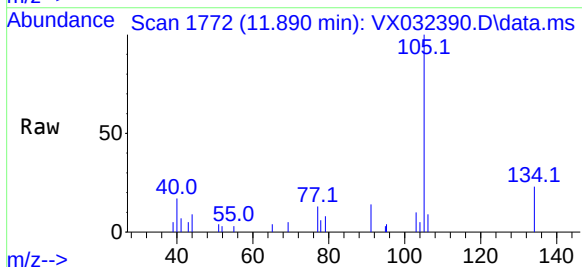




#86
p-Isopropyltoluene
Concen: 0.456 ug/l
RT: 12.183 min Scan# 119
Delta R.T. 0.171 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion:119 Resp: 2473
Ion Ratio Lower Upper
119 100
134 27.5 13.2 39.5
91 29.3 12.4 37.2

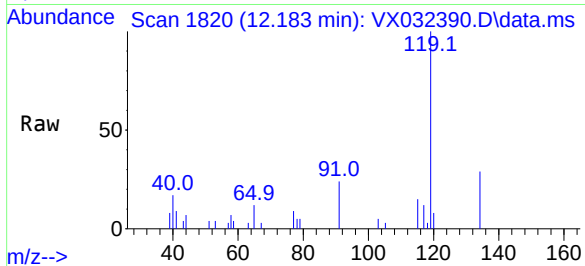

#89
n-Butylbenzene
Concen: 0.211 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Tgt Ion: 91 Resp: 1009
Ion Ratio Lower Upper
91 100
92 28.7 26.3 78.9
134 71.4 13.0 39.0#


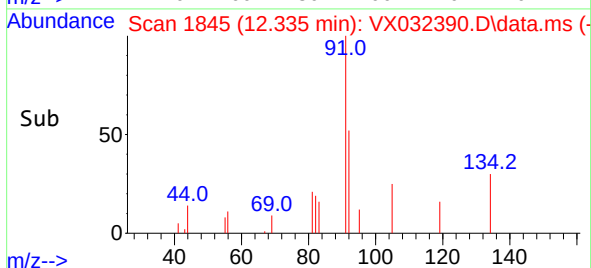
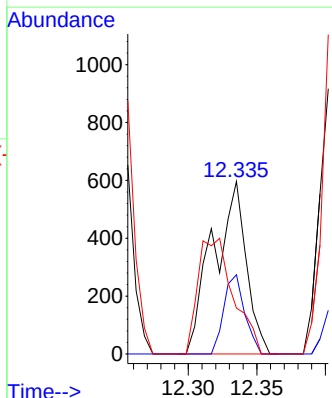
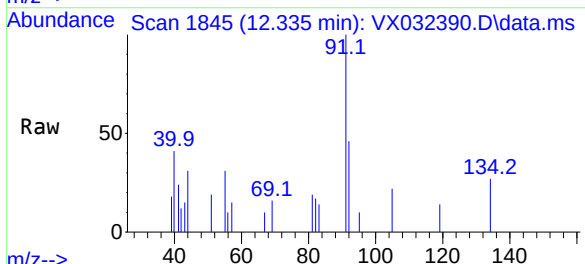




#90
Hexachloroethane
Concen: 1.987 ug/l
RT: 12.616 min Scan# 117
Delta R.T. 0.073 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42




Instrument :
MSVOA_X
ClientSampleId :
TP3-1024


Tgt Ion:117 Resp: 1673
Ion Ratio Lower Upper
117 100
201 0.0 38.5 115.3#

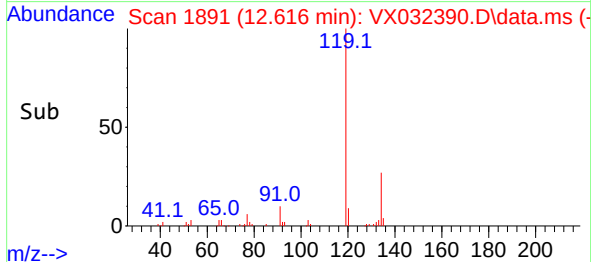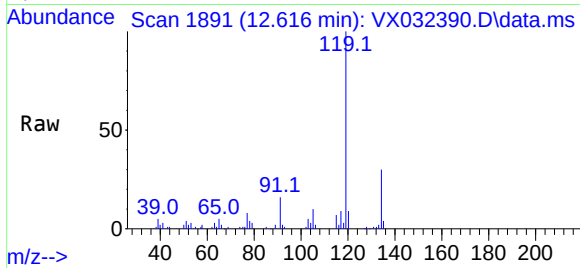

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.293 ug/l
RT: 12.920 min Scan# 1941
Delta R.T. -0.025 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42


Tgt Ion: 75 Resp: 110
Ion Ratio Lower Upper
75 100
155 0.0 43.1 129.3#
157 0.0 57.1 171.5#

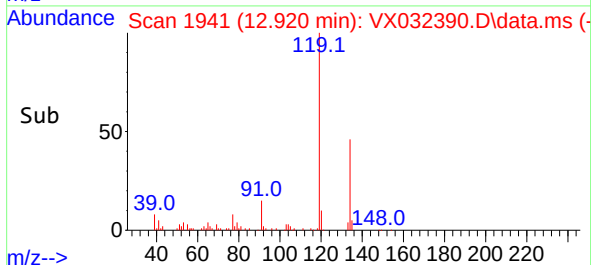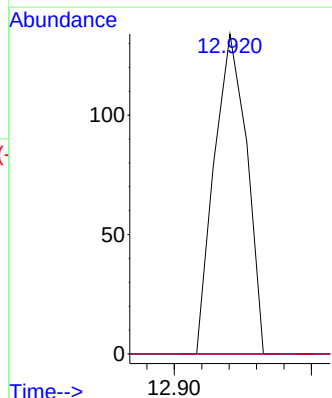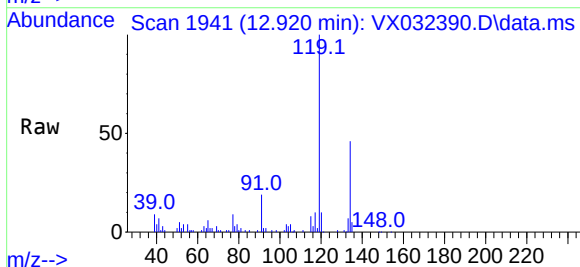

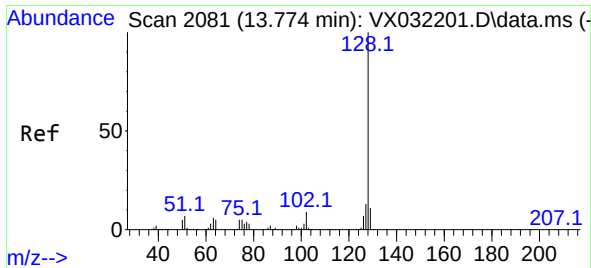

#95
Naphthalene
Concen: 1.563 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX032390.D
Acq: 26 Oct 2022 01:42

Instrument :
MSVOA_X
ClientSampleId :
TP3-1024

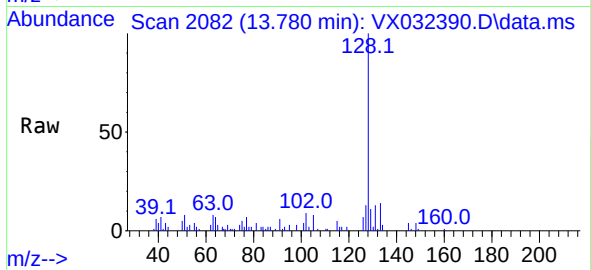

Tgt Ion:128 Resp: 9215
Ion Ratio Lower Upper
128 100
127 17.9 10.3 15.5#
129 15.4 8.7 13.1#

