

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
 Data File : VX032364.D
 Acq On : 25 Oct 2022 15:13
 Operator : JC/MD
 Sample : N5249-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-MW-32-20221019

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M

Title : SW846 8260

Signal : TIC: VX032364.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	20	rVB	30854	31895	3.36%	0.698%
2	1.368	36	46	52	rBV2	34619	47936	5.06%	1.049%
3	4.495	551	559	567	rBV3	3739	10250	1.08%	0.224%
4	5.385	694	705	722	rBV2	78402	230068	24.27%	5.035%
5	5.556	722	733	748	rVB	141686	397219	41.90%	8.693%
6	5.958	789	799	812	rBV	86754	224536	23.68%	4.914%
7	6.763	922	931	943	rBV	205804	489028	51.58%	10.702%
8	7.129	981	991	1011	rBV	439760	948046	100.00%	20.748%
9	8.653	1234	1241	1248	rBV	414829	652911	68.87%	14.289%
10	8.720	1248	1252	1259	rVB2	6741	11665	1.23%	0.255%
11	10.055	1465	1471	1481	rBV	419151	558521	58.91%	12.223%
12	11.079	1634	1639	1652	rBV	333986	437956	46.20%	9.585%
13	12.024	1788	1794	1803	rBV	419644	529355	55.84%	11.585%




Sum of corrected areas: 4569386

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
Data File : VX032364.D
Acq On : 25 Oct 2022 15:13
Operator : JC/MD
Sample : N5249-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-32-20221019

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

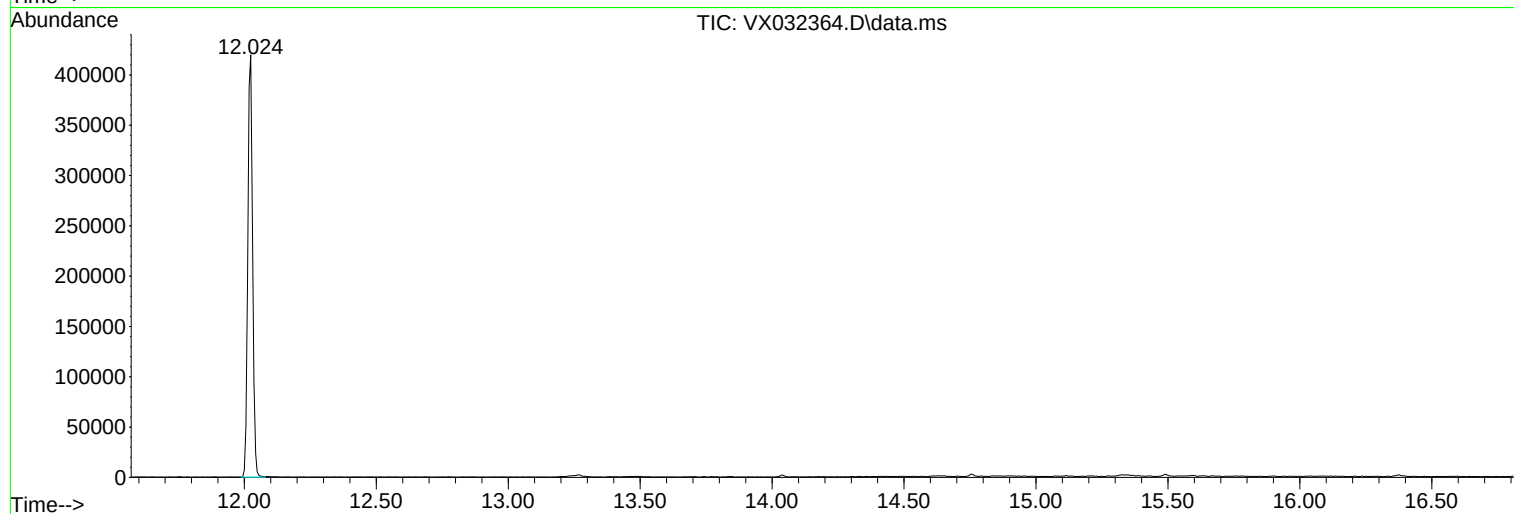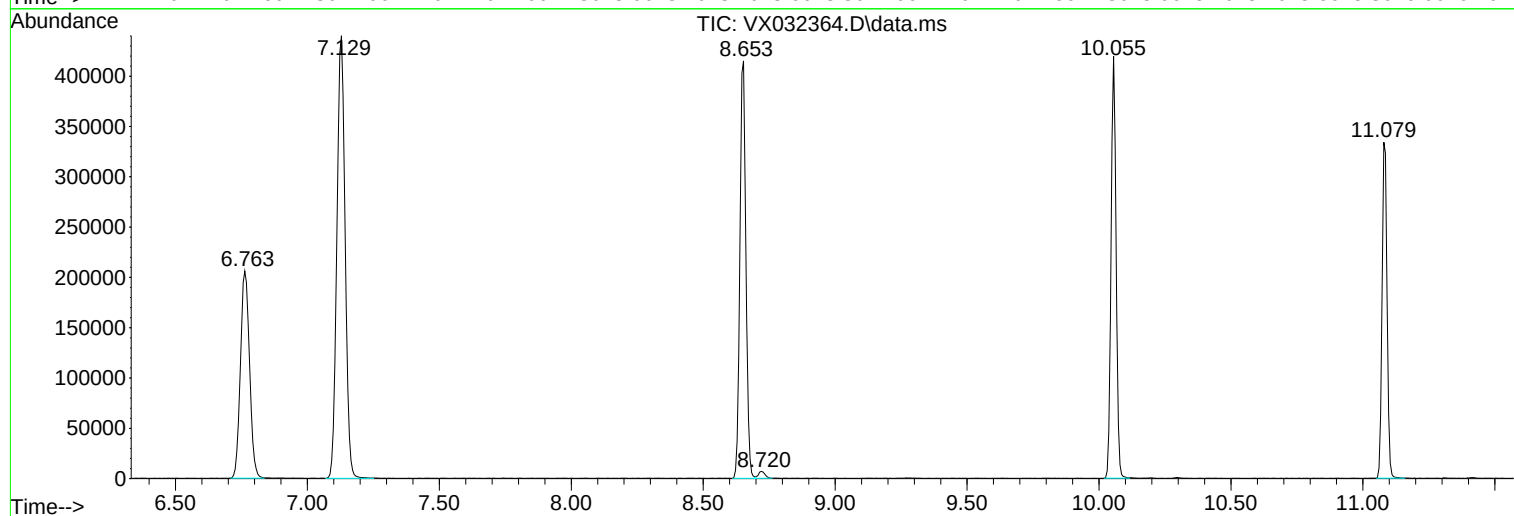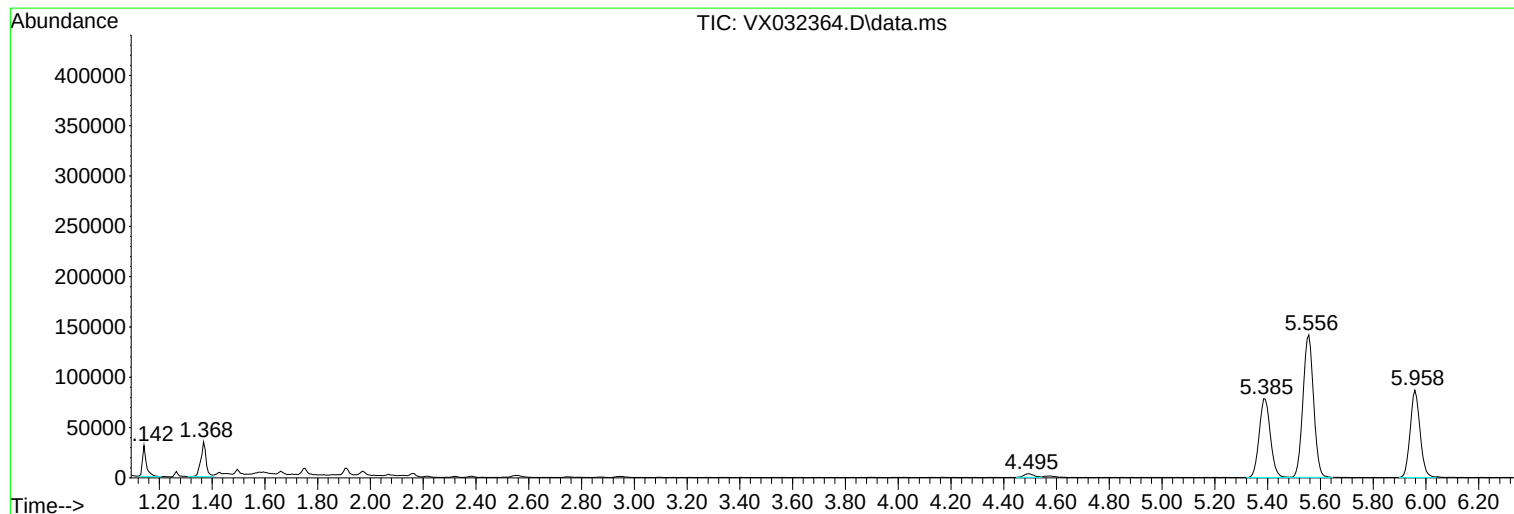

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
Data File : VX032364.D
Acq On : 25 Oct 2022 15:13
Operator : JC/MD
Sample : N5249-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-32-20221019










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.368	6.03 ug/l	47936	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane	58	C4H10	000106-97-8	59
2			Isopropylsulfonyl chloride	142	C3H7ClO2S	010147-37-2	17
3			Formic acid, chloro-, (3,4,4-tri...	194	C7H11ClO4	107323-92-2	9
4			Propane, 2-nitro-	89	C3H7NO2	000079-46-9	9
5			Propane, 1-nitro-	89	C3H7NO2	000108-03-2	9

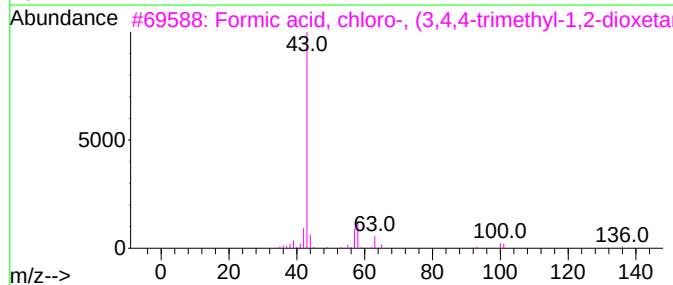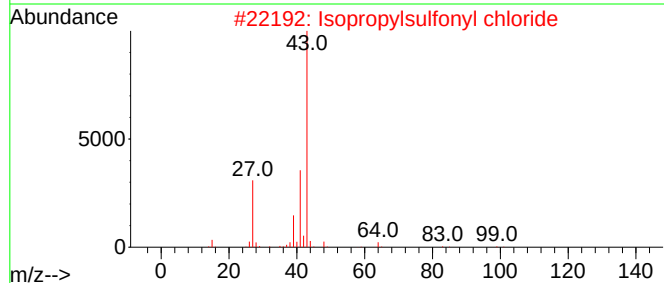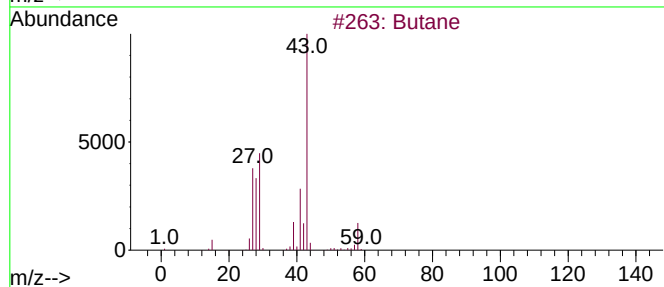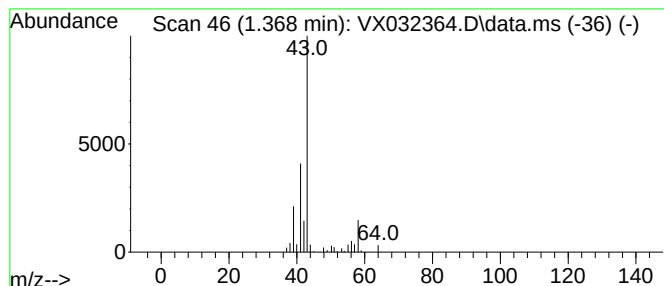

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
Data File : VX032364.D
Acq On : 25 Oct 2022 15:13
Operator : JC/MD
Sample : N5249-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-32-20221019

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane	1.368	6.0	ug/l	47936	1	5.556	397219	50.0