

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
 Data File : VX032394.D
 Acq On : 26 Oct 2022 03:16
 Operator : JC/MD
 Sample : N5267-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP7-1024

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
 Title : SW846 8260

Signal : TIC: VX032394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	24	32	43	rBV2	7032	22244	1.86%	0.264%
2	2.380	206	212	219	rBV	14035	23408	1.96%	0.277%
3	2.788	274	279	293	rVB	13642	27768	2.32%	0.329%
4	3.574	401	408	416	rBV4	5040	12126	1.01%	0.144%
5	4.721	585	596	607	rBV2	8053	24326	2.03%	0.288%
6	5.391	695	706	719	rBV2	82140	239161	19.98%	2.835%
7	5.556	722	733	750	rVB	143523	409880	34.24%	4.859%
8	5.958	788	799	816	rBV	91366	238484	19.92%	2.827%
9	6.342	852	862	878	rBV	51574	131501	10.98%	1.559%
10	6.763	917	931	946	rBV	229580	622208	51.97%	7.376%
11	7.641	1068	1075	1080	rBV	28051	51082	4.27%	0.606%
12	7.696	1080	1084	1090	rVB2	9404	16626	1.39%	0.197%
13	7.799	1093	1101	1114	rBV	711155	1197224	100.00%	14.192%
14	8.549	1218	1224	1234	rBV	164370	255086	21.31%	3.024%
15	8.647	1234	1240	1257	rVB	432987	707380	59.09%	8.385%
16	8.952	1284	1290	1303	rBV	209111	305283	25.50%	3.619%
17	9.244	1332	1338	1345	rBV	247415	338833	28.30%	4.017%
18	9.305	1345	1348	1351	rVV	19626	28074	2.34%	0.333%
19	9.342	1351	1354	1356	rVV	33322	44434	3.71%	0.527%
20	9.378	1356	1360	1369	rVV	96388	140213	11.71%	1.662%
21	9.482	1372	1377	1388	rVV	389621	494129	41.27%	5.858%
22	9.580	1388	1393	1405	rVB	248864	326257	27.25%	3.868%
23	9.915	1442	1448	1462	rBV	786464	966523	80.73%	11.457%
24	10.055	1462	1471	1478	rBV	462489	631112	52.71%	7.481%
25	10.281	1504	1508	1515	rVB	9241	12848	1.07%	0.152%
26	10.506	1539	1545	1554	rVB	11009	14198	1.19%	0.168%
27	10.640	1559	1567	1577	rBV	66264	81030	6.77%	0.961%
28	11.079	1634	1639	1650	rBV	375099	478043	39.93%	5.667%
29	12.024	1788	1794	1802	rBV	472442	581781	48.59%	6.897%
30	13.140	1966	1977	1980	rBV6	5273	14544	1.21%	0.172%




Sum of corrected areas: 8435806

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
Data File : VX032394.D
Acq On : 26 Oct 2022 03:16
Operator : JC/MD
Sample : N5267-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP7-1024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

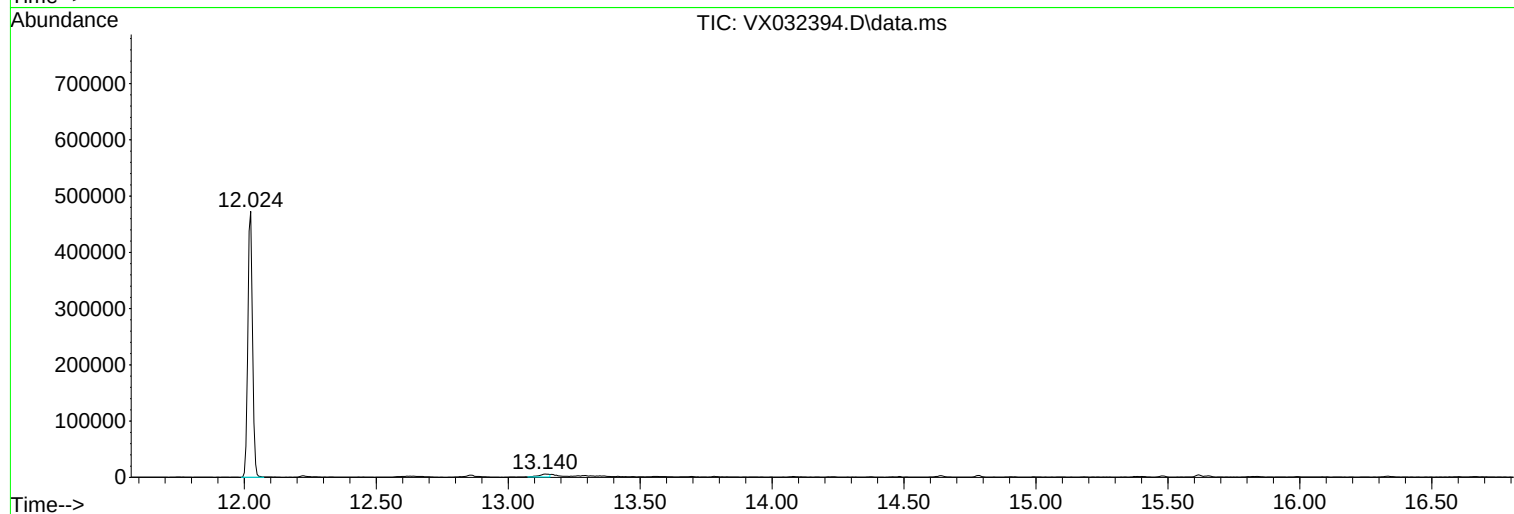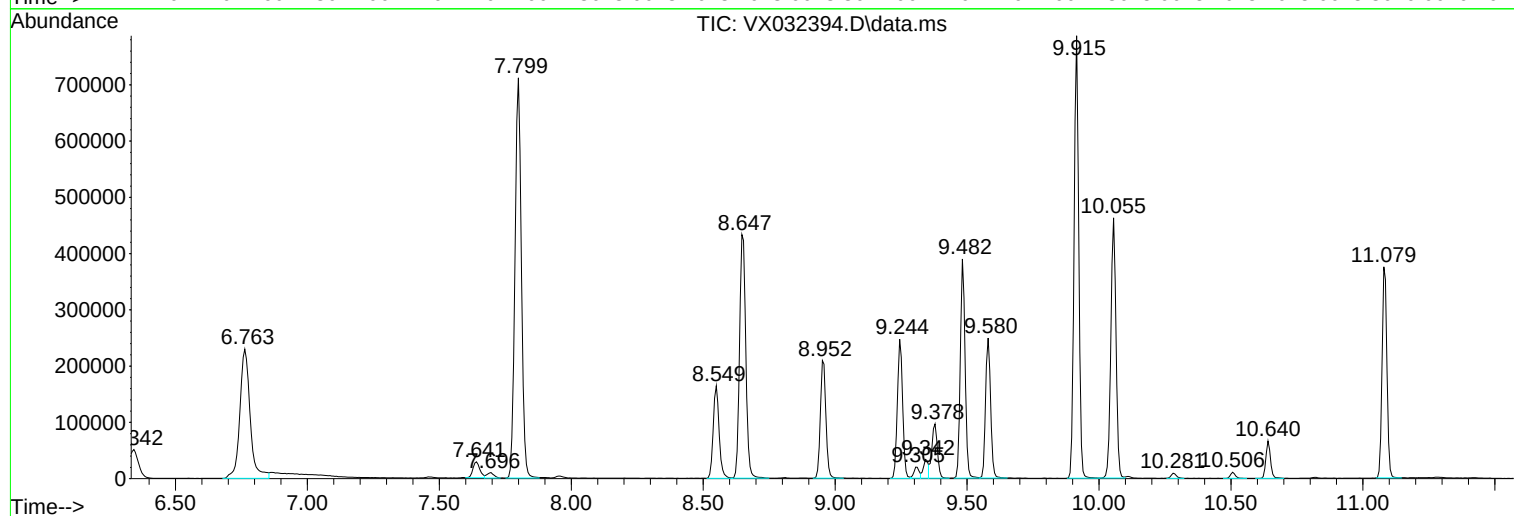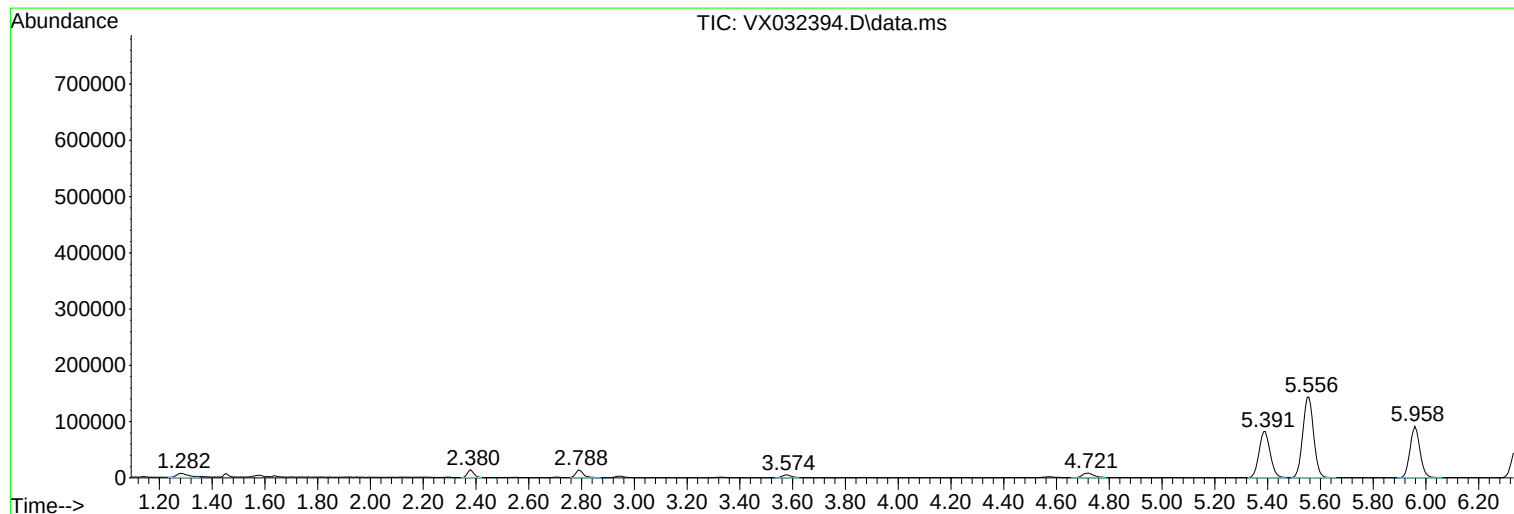

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
Data File : VX032394.D
Acq On : 26 Oct 2022 03:16
Operator : JC/MD
Sample : N5267-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP7-1024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102522\
Data File : VX032394.D
Acq On : 26 Oct 2022 03:16
Operator : JC/MD
Sample : N5267-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP7-1024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------