

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
 Data File : VX038475.D
 Acq On : 25 Oct 2023 13:24
 Operator : JC/MD
 Sample : 05007-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.093	647	657	668	rBV3	10674	33823	3.49%	0.650%
2	5.385	693	705	722	rBV	109416	319649	33.02%	6.141%
3	5.550	722	732	750	rVB	166975	475825	49.16%	9.142%
4	5.958	788	799	820	rBV	109199	295469	30.52%	5.677%
5	6.763	921	931	943	rBV	268711	641182	66.24%	12.318%
6	8.647	1233	1240	1258	rBV	556919	884427	91.37%	16.992%
7	10.055	1465	1471	1485	rBV	620424	860610	88.91%	16.534%
8	11.079	1634	1639	1651	rBV	539189	703800	72.71%	13.521%
9	12.024	1788	1794	1807	rVB	741619	967980	100.00%	18.597%
10	12.226	1821	1827	1834	rBV2	5583	10679	1.10%	0.205%
11	13.591	2046	2051	2060	rBV2	8748	11608	1.20%	0.223%




Sum of corrected areas: 5205052

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038475.D
Acq On : 25 Oct 2023 13:24
Operator : JC/MD
Sample : 05007-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

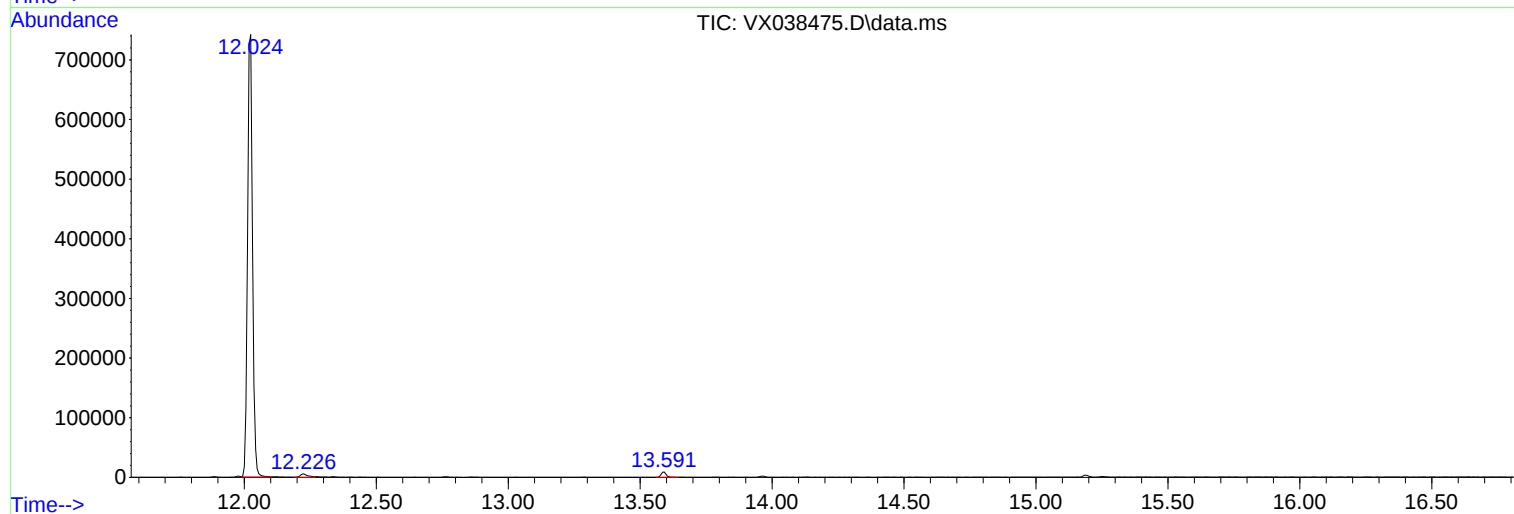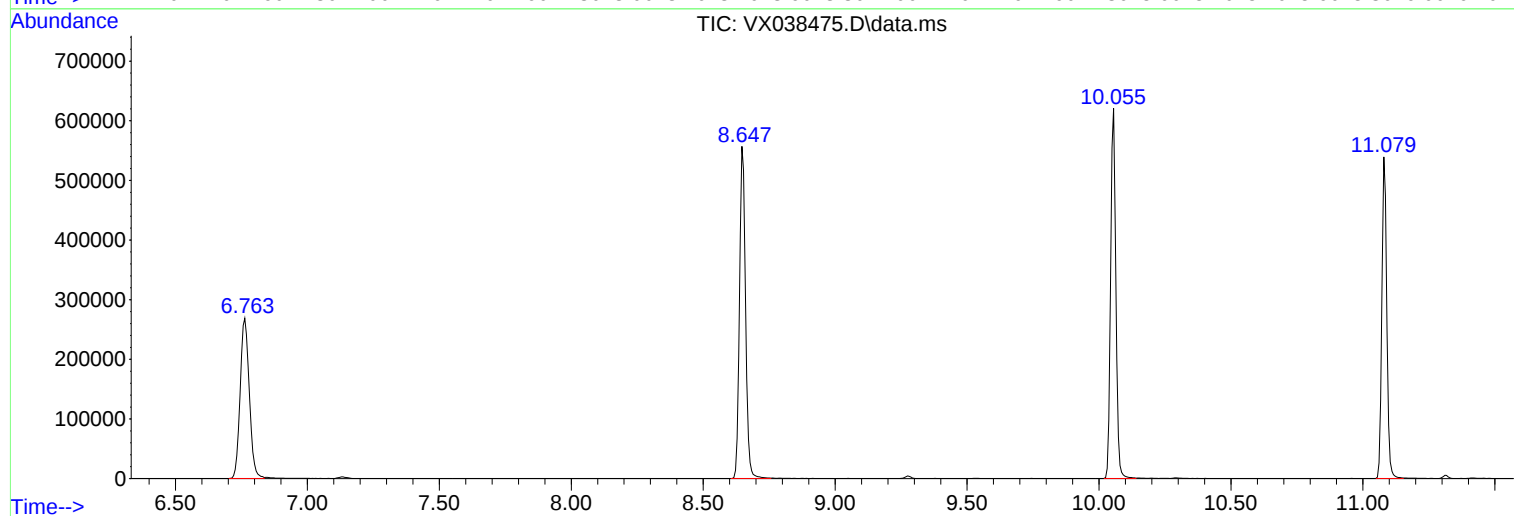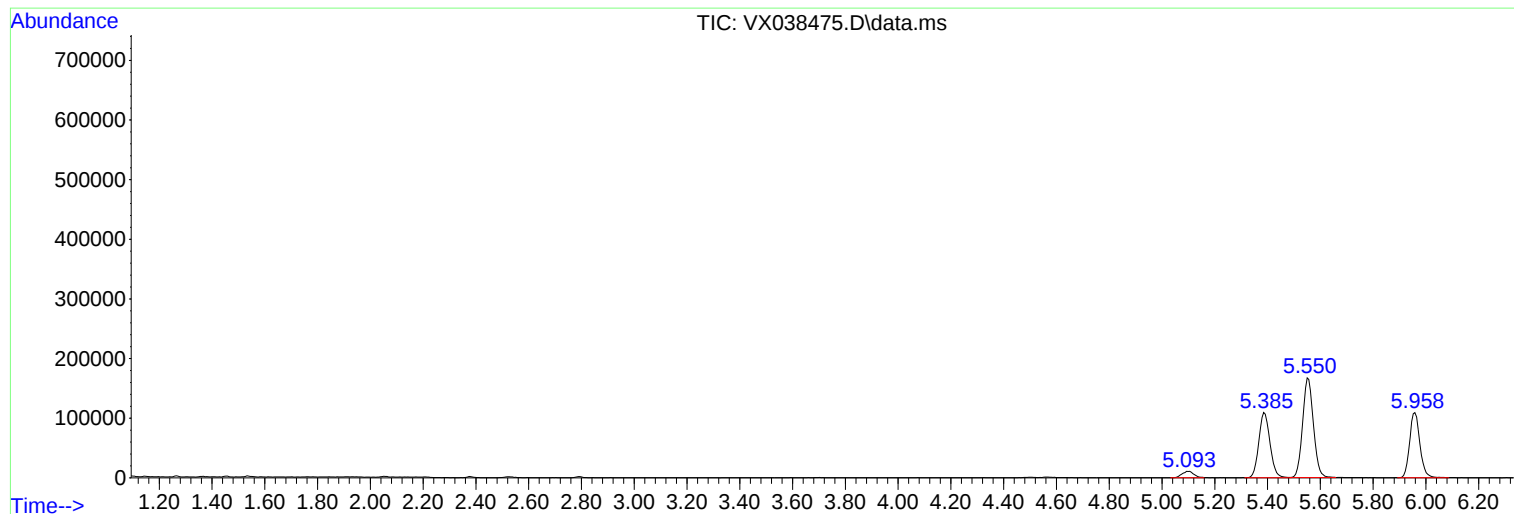

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038475.D
Acq On : 25 Oct 2023 13:24
Operator : JC/MD
Sample : 05007-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038475.D
Acq On : 25 Oct 2023 13:24
Operator : JC/MD
Sample : 05007-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------