

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038481.D
Acq On : 25 Oct 2023 15:43
Operator : JC/MD
Sample : 04980-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MAIN-BAILER-SUMP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038481.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.489	550	558	572	rBV	24218	64595	7.00%	1.219%
2	5.385	694	705	722	rBV	104586	310051	33.61%	5.852%
3	5.550	722	732	752	rVB	163170	468649	50.80%	8.845%
4	5.958	788	799	818	rBV	105590	289084	31.34%	5.456%
5	6.763	918	931	953	rBV	261836	636608	69.01%	12.016%
6	7.135	984	992	1005	rVB2	7737	18645	2.02%	0.352%
7	8.647	1233	1240	1260	rBV	543520	881173	95.52%	16.632%
8	9.275	1337	1343	1354	rVB	131417	194729	21.11%	3.675%
9	10.055	1465	1471	1483	rBV	620369	838178	90.86%	15.820%
10	11.079	1634	1639	1654	rBV	507631	673933	73.05%	12.720%
11	12.018	1788	1793	1806	rBV	704960	922527	100.00%	17.412%




Sum of corrected areas: 5298172

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038481.D
Acq On : 25 Oct 2023 15:43
Operator : JC/MD
Sample : 04980-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MAIN-BAILER-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

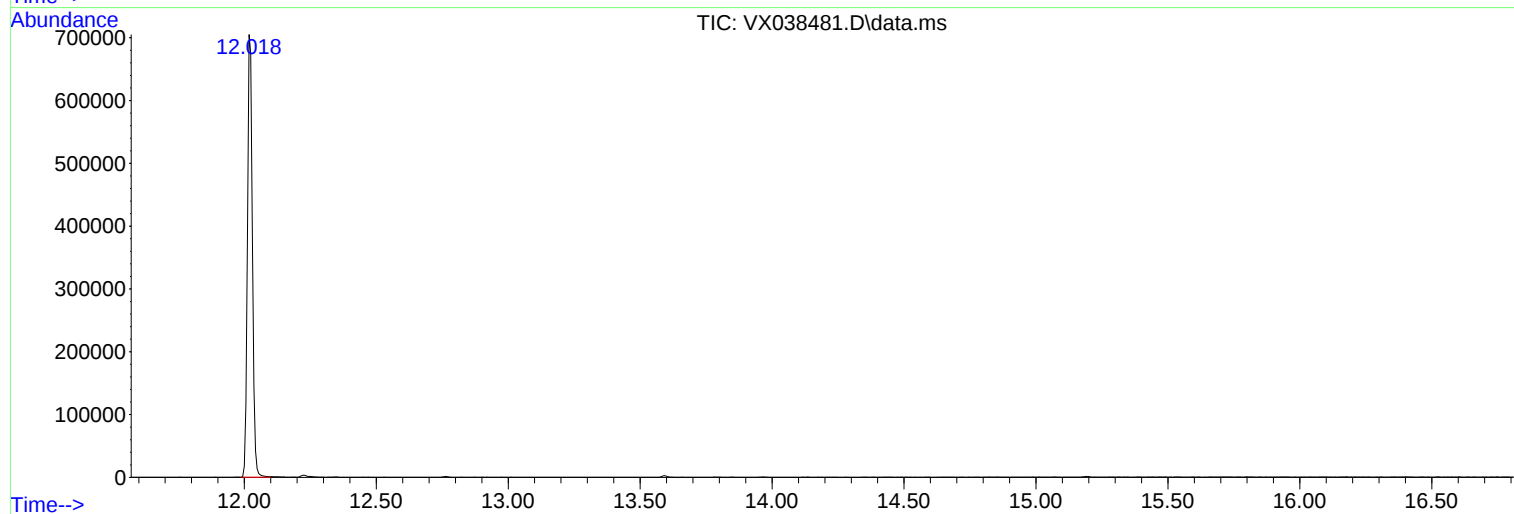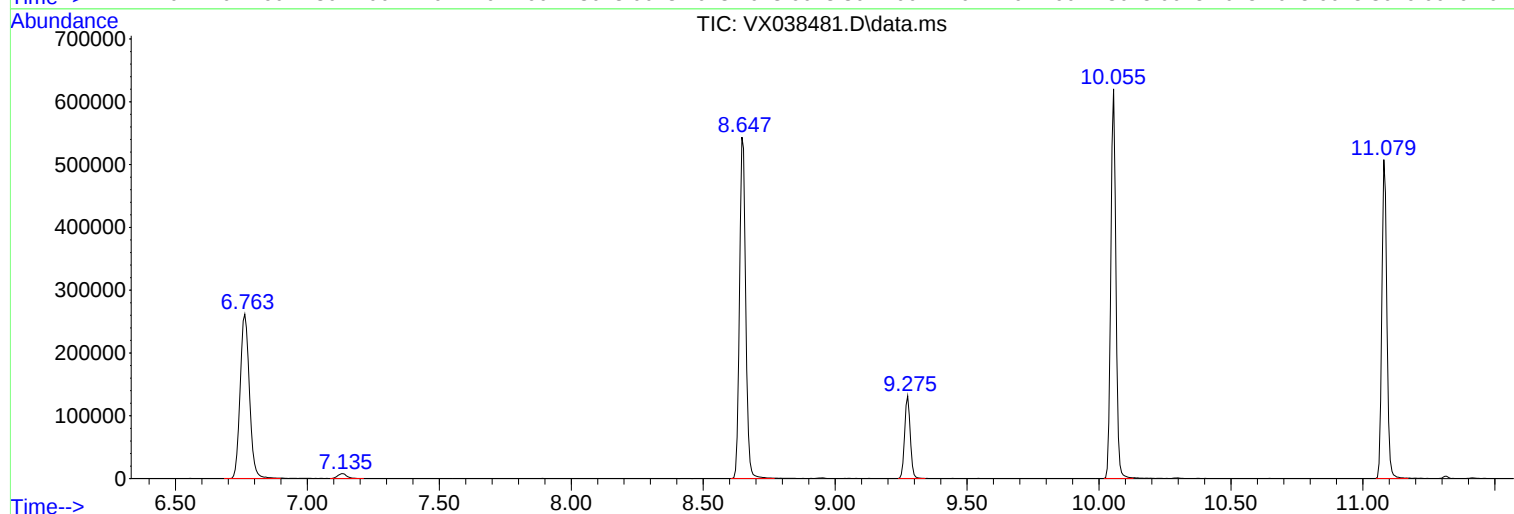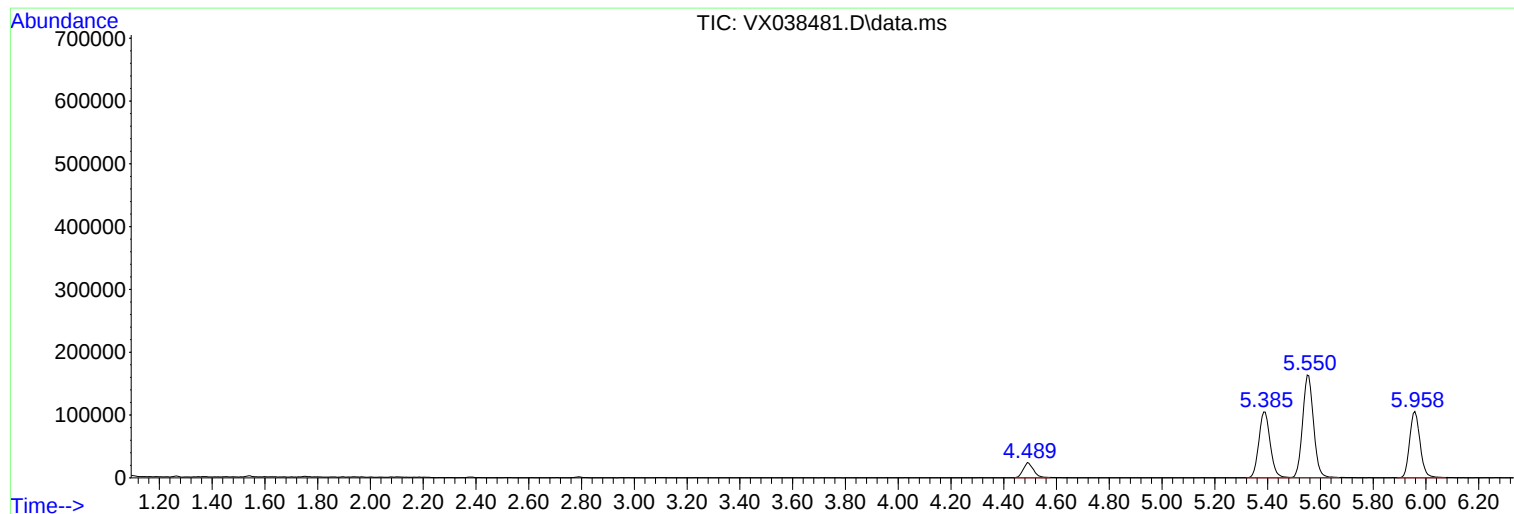

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038481.D
Acq On : 25 Oct 2023 15:43
Operator : JC/MD
Sample : 04980-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MAIN-BAILER-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038481.D
Acq On : 25 Oct 2023 15:43
Operator : JC/MD
Sample : 04980-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MAIN-BAILER-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------