

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
 Data File : VX038485.D
 Acq On : 25 Oct 2023 17:16
 Operator : JC/MD
 Sample : 05038-07 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-1069

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Title : SW846 8260

Signal : TIC: VX038485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	56	60	71	rBV	674104	772172	83.22%	11.877%
2	2.050	152	158	172	rBV	230033	377678	40.70%	5.809%
3	2.380	206	212	222	rVB	8229	14244	1.54%	0.219%
4	4.233	507	516	529	rBV3	16095	44610	4.81%	0.686%
5	5.391	693	706	720	rBV	104991	310287	33.44%	4.773%
6	5.550	721	732	748	rVB	163106	468743	50.52%	7.210%
7	5.958	789	799	812	rBV	106083	282985	30.50%	4.353%
8	6.763	921	931	947	rBV	263889	628460	67.73%	9.667%
9	7.214	999	1005	1021	rBV2	14496	43021	4.64%	0.662%
10	8.647	1234	1240	1250	rBV	557574	880440	94.89%	13.542%
11	9.518	1379	1383	1392	rBV	27462	42293	4.56%	0.651%
12	10.055	1465	1471	1488	rBV	613582	840157	90.55%	12.923%
13	10.585	1553	1558	1574	rBV	31105	65928	7.11%	1.014%
14	11.079	1634	1639	1651	rBV	525689	683702	73.69%	10.516%
15	11.756	1746	1750	1759	rVB	33784	48875	5.27%	0.752%
16	12.024	1788	1794	1804	rBV	726942	927843	100.00%	14.272%
17	12.219	1821	1826	1836	rBV2	10522	22075	2.38%	0.340%
18	12.951	1941	1946	1958	rBV	24037	36726	3.96%	0.565%
19	15.188	2308	2313	2319	rBV2	7049	11119	1.20%	0.171%




Sum of corrected areas: 6501358

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038485.D
Acq On : 25 Oct 2023 17:16
Operator : JC/MD
Sample : 05038-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1069

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

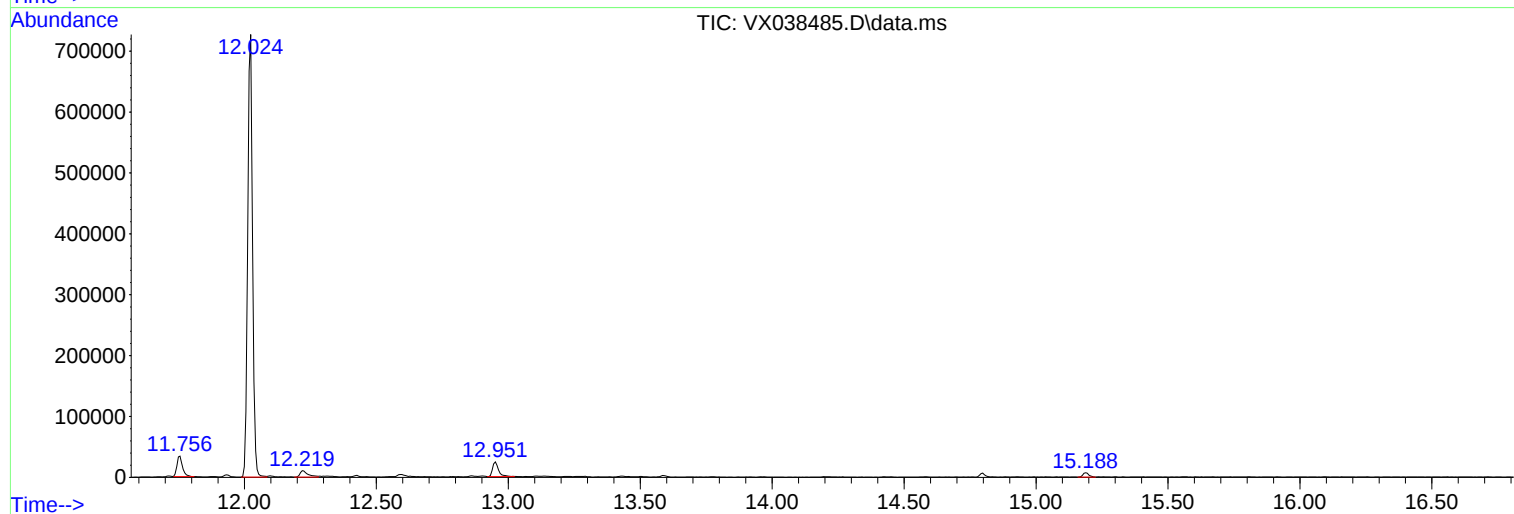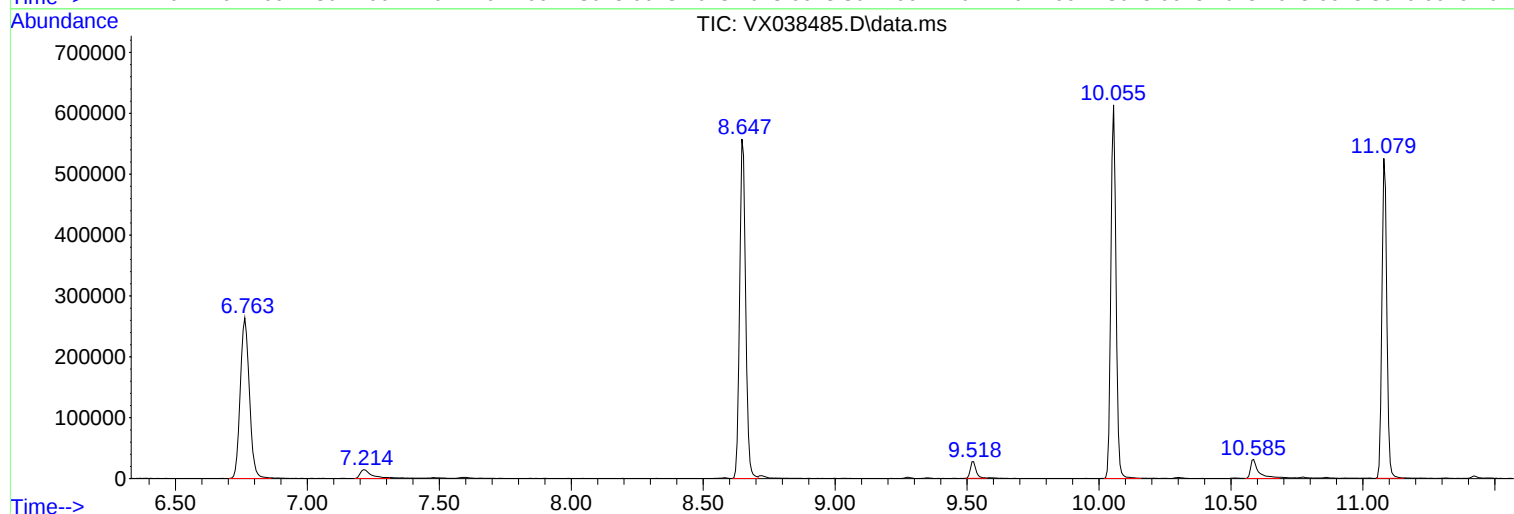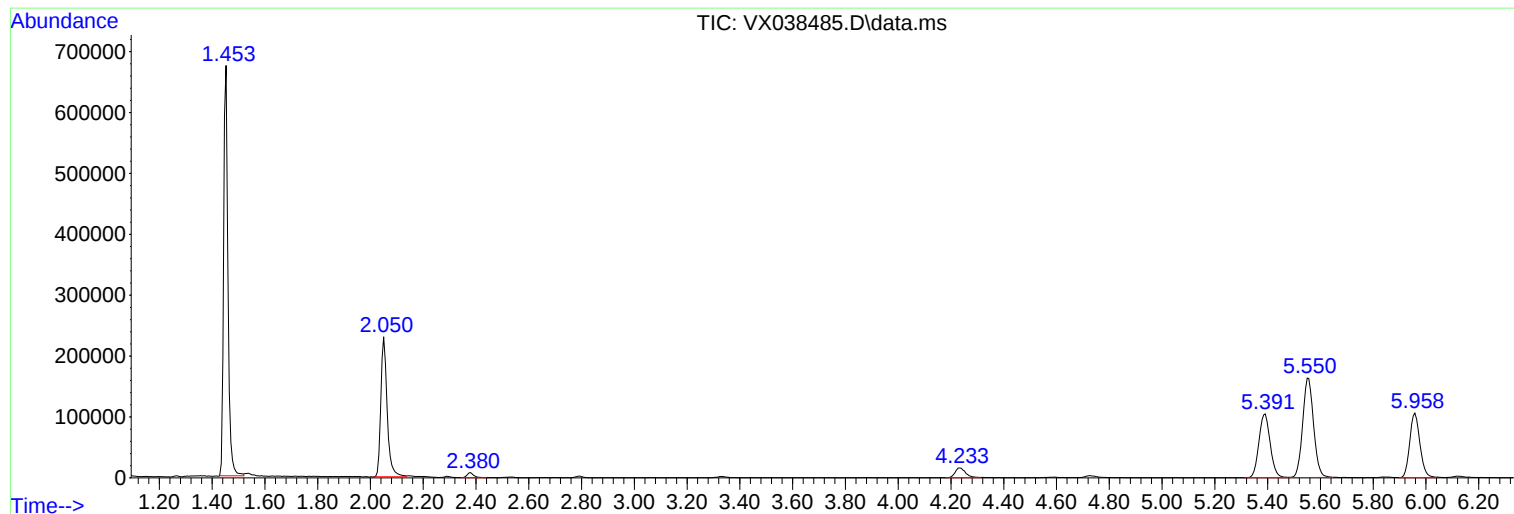

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038485.D
Acq On : 25 Oct 2023 17:16
Operator : JC/MD
Sample : 05038-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1069










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Ethanol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.050	40.29 ug/l	377678	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol	46	C2H6O	000064-17-5	64
2			Dimethyl ether	46	C2H6O	000115-10-6	9
3			Methane, nitroso-	45	CH3NO	000865-40-7	4
4			Formic acid	46	CH2O2	000064-18-6	4
5			Oxalic acid	90	C2H2O4	000144-62-7	4

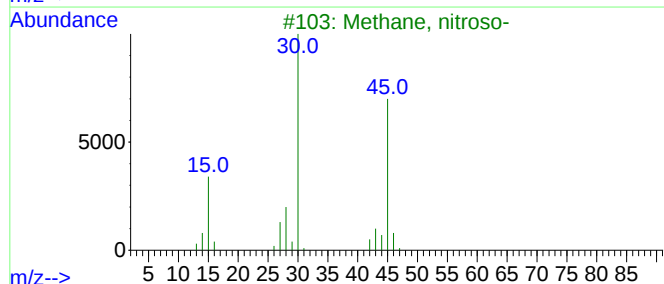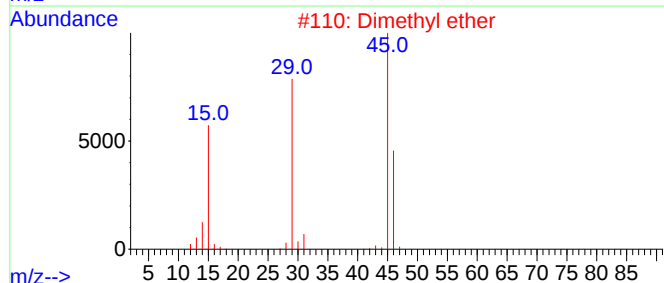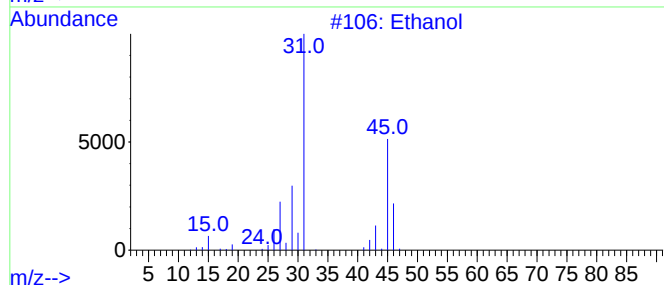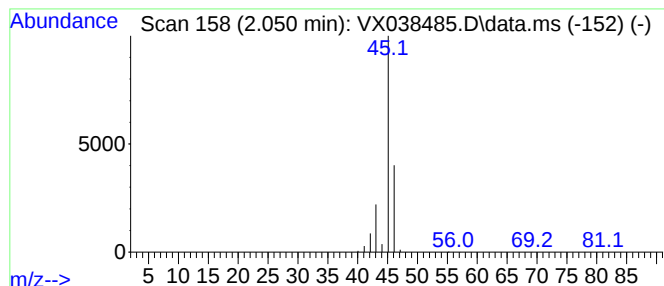

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038485.D
Acq On : 25 Oct 2023 17:16
Operator : JC/MD
Sample : 05038-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1069

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol	2.050	40.3	ug/l	377678	1	5.556	468743	50.0