

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
 Data File : VX038498.D
 Acq On : 26 Oct 2023 05:11
 Operator : JC/MD
 Sample : 05030-01 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRE-1723

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Title : SW846 8260

Signal : TIC: VX038498.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.373	205	211	222	rBV	302754	481221	45.56%	7.300%
2	3.849	446	453	469	rBV3	4149	13553	1.28%	0.206%
3	5.385	693	705	720	rBV	118187	352197	33.34%	5.343%
4	5.550	720	732	748	rVV	189279	539820	51.10%	8.189%
5	5.952	788	798	823	rVB	124390	324172	30.69%	4.917%
6	6.757	921	930	946	rBV	295639	713395	67.54%	10.822%
7	8.647	1233	1240	1248	rBV	637665	994298	94.13%	15.083%
8	8.720	1248	1252	1263	rVB	28790	49625	4.70%	0.753%
9	9.525	1376	1384	1395	rBV	8860	14621	1.38%	0.222%
10	10.055	1465	1471	1484	rBV	703651	951219	90.05%	14.429%
11	11.079	1634	1639	1654	rBV	597991	771768	73.06%	11.707%
12	11.750	1746	1749	1758	rVB	11096	14316	1.36%	0.217%
13	12.024	1788	1794	1801	rBV	809384	1056321	100.00%	16.023%
14	12.085	1801	1804	1814	rVB	7215	10855	1.03%	0.165%
15	12.219	1821	1826	1828	rBV2	9352	13009	1.23%	0.197%
16	12.317	1838	1842	1849	rVB4	7430	15738	1.49%	0.239%
17	12.963	1944	1948	1955	rVB	7863	11253	1.07%	0.171%
18	13.164	1978	1981	1986	rVB2	10989	14781	1.40%	0.224%
19	13.292	1992	2002	2007	rBV2	28233	44890	4.25%	0.681%
20	13.420	2019	2023	2031	rVB2	25237	33650	3.19%	0.510%
21	13.585	2046	2050	2054	rBV4	10246	15342	1.45%	0.233%
22	13.774	2077	2081	2087	rVB	10274	15474	1.46%	0.235%
23	13.853	2087	2094	2100	rVB3	10311	15814	1.50%	0.240%
24	13.926	2100	2106	2109	rBV3	8644	14296	1.35%	0.217%
25	14.225	2148	2155	2164	rVB2	24344	42166	3.99%	0.640%
26	14.481	2193	2197	2206	rVB3	16773	25593	2.42%	0.388%
27	14.615	2214	2219	2220	rBV2	11750	13842	1.31%	0.210%
28	14.633	2220	2222	2226	rVB	14190	17710	1.68%	0.269%
29	15.481	2356	2361	2366	rBV5	6901	11397	1.08%	0.173%




Sum of corrected areas: 6592336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038498.D
Acq On : 26 Oct 2023 05:11
Operator : JC/MD
Sample : 05030-01 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1723

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

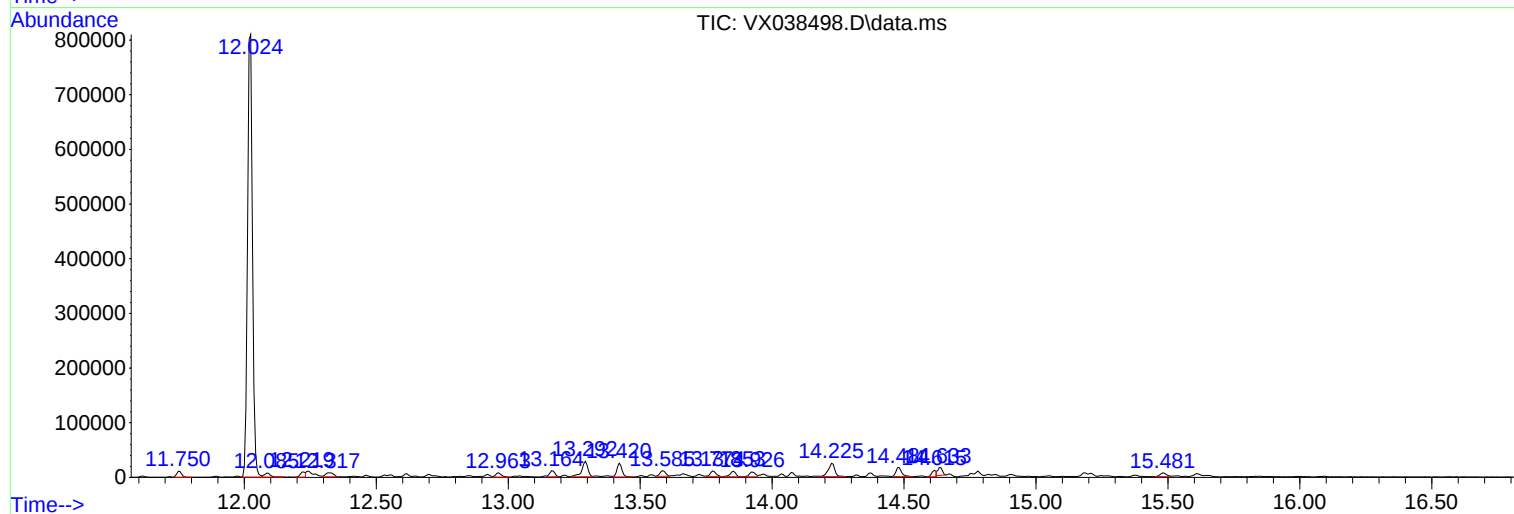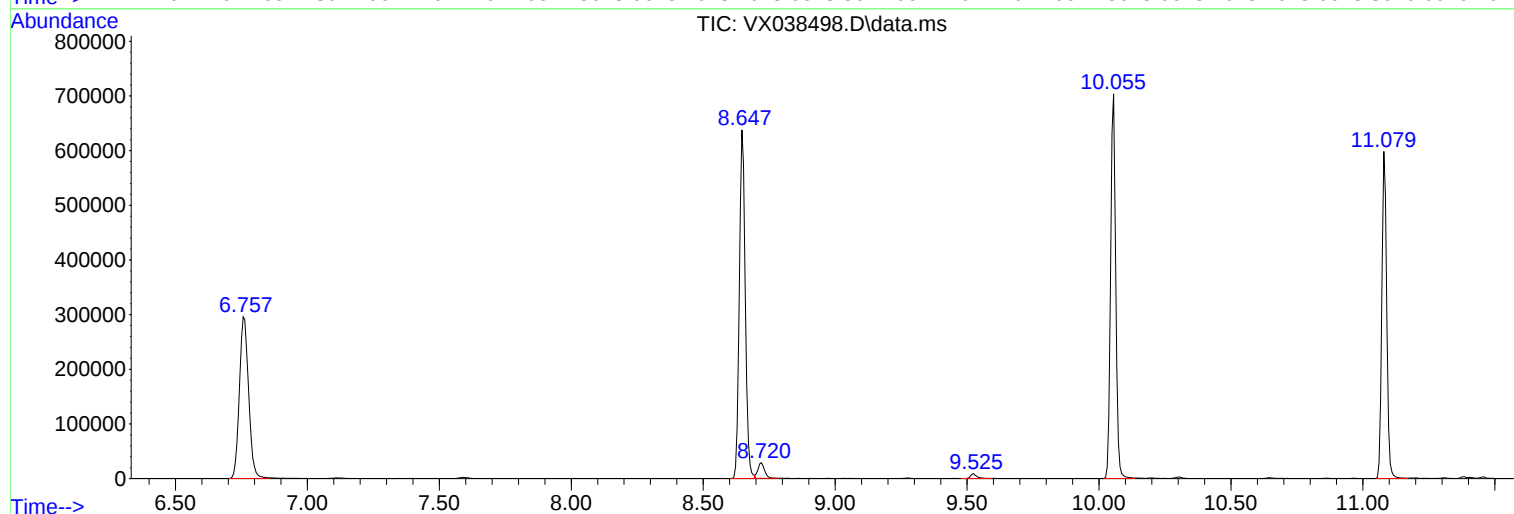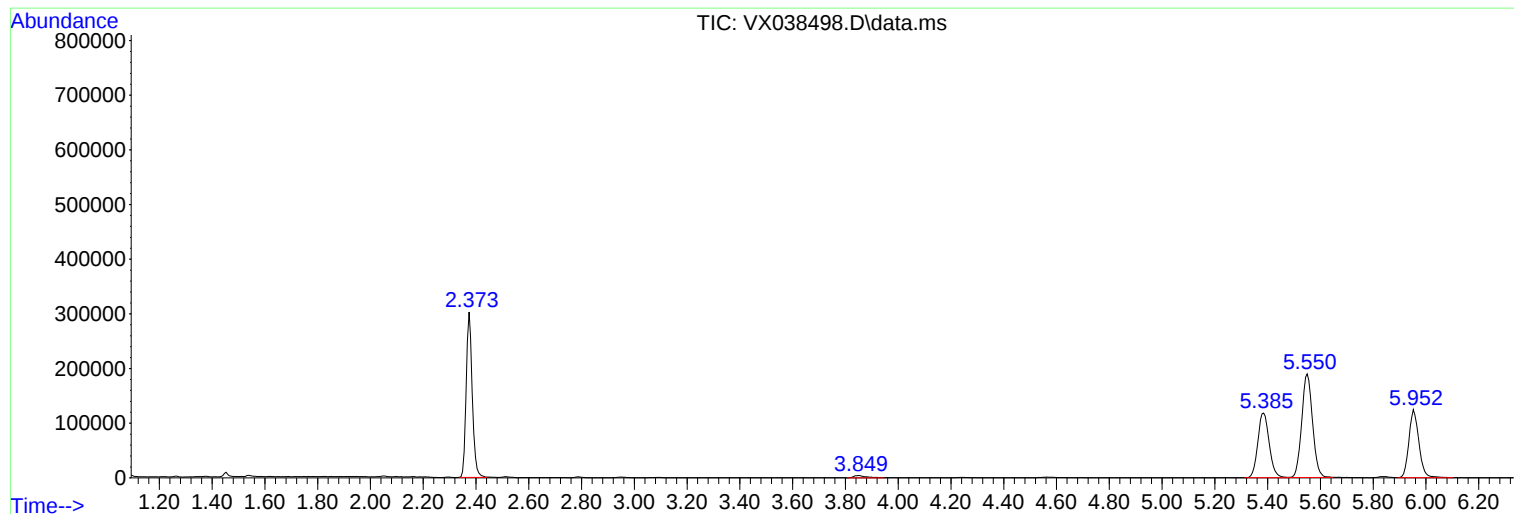

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038498.D
Acq On : 26 Oct 2023 05:11
Operator : JC/MD
Sample : 05030-01 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1723

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038498.D
Acq On : 26 Oct 2023 05:11
Operator : JC/MD
Sample : 05030-01 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1723

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------