


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102523\
Data File : VX038493.D
Acq On : 26 Oct 2023 01:23
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Title : SW846 8260
Last Update : Thu Oct 05 15:27:13 2023

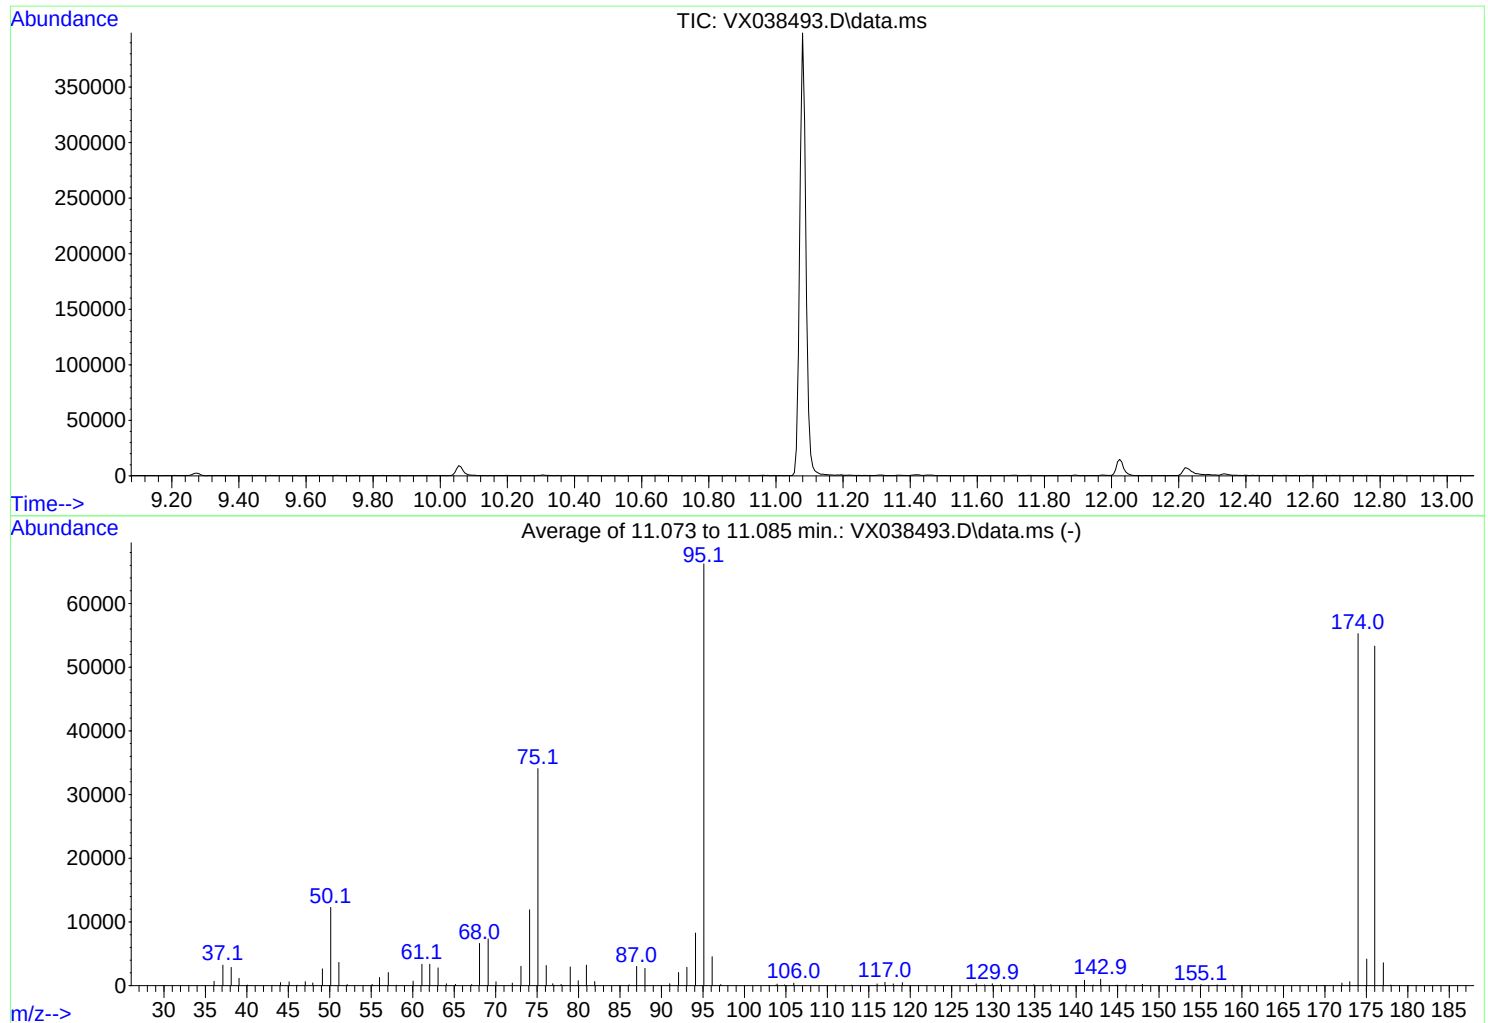

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	12282	PASS
75	95	30	60	51.5	34085	PASS
95	95	100	100	100.0	66227	PASS
96	95	5	9	6.9	4558	PASS
173	174	0.00	2	1.2	642	PASS
174	95	50	100	83.5	55267	PASS
175	174	5	9	7.5	4164	PASS
176	174	95	101	96.4	53299	PASS
177	176	5	9	6.8	3598	PASS