

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102618\
 Data File : VX005632.D
 Acq On : 27 Oct 2018 04:14
 Operator : JC/MD
 Sample : J5696-08
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DL-SW-02

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102418W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.629	64	78	87	rBV9	11631	35297	3.12%	0.543%
2	2.617	235	240	248	rVB	10313	20851	1.85%	0.321%
3	5.220	656	667	676	rBV4	8133	25252	2.24%	0.388%
4	5.494	702	712	728	rBV3	137446	400047	35.42%	6.151%
5	5.659	728	739	761	rBV	244066	701096	62.07%	10.780%
6	6.067	794	806	826	rBV	158198	419158	37.11%	6.445%
7	6.860	925	936	959	rBV	361562	863554	76.45%	13.278%
8	8.713	1233	1240	1256	rBV	684804	1129524	100.00%	17.368%
9	10.116	1463	1470	1484	rBV	694370	968750	85.77%	14.896%
10	10.359	1505	1510	1516	rVB	11185	16472	1.46%	0.253%
11	11.140	1632	1638	1653	rBV	581008	757729	67.08%	11.651%
12	11.810	1743	1748	1753	rBV	9929	13035	1.15%	0.200%
13	12.079	1786	1792	1799	rBV	789725	949352	84.05%	14.597%
14	12.603	1870	1878	1885	rBV5	7249	21183	1.88%	0.326%
15	12.670	1885	1889	1895	rVB	9083	12913	1.14%	0.199%
16	13.347	1989	2000	2005	rBV3	5974	12853	1.14%	0.198%
17	13.834	2076	2080	2086	rVB	19146	26368	2.33%	0.405%
18	14.700	2216	2222	2232	rVB	36767	52752	4.67%	0.811%
19	14.840	2232	2245	2250	rBV	24562	40357	3.57%	0.621%
20	15.548	2355	2361	2367	rBV3	10818	18348	1.62%	0.282%
21	15.688	2379	2384	2388	rBV3	10065	18648	1.65%	0.287%


Sum of corrected areas: 6503539

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102618\
Data File : VX005632.D
Acq On : 27 Oct 2018 04:14
Operator : JC/MD
Sample : J5696-08
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DL-SW-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

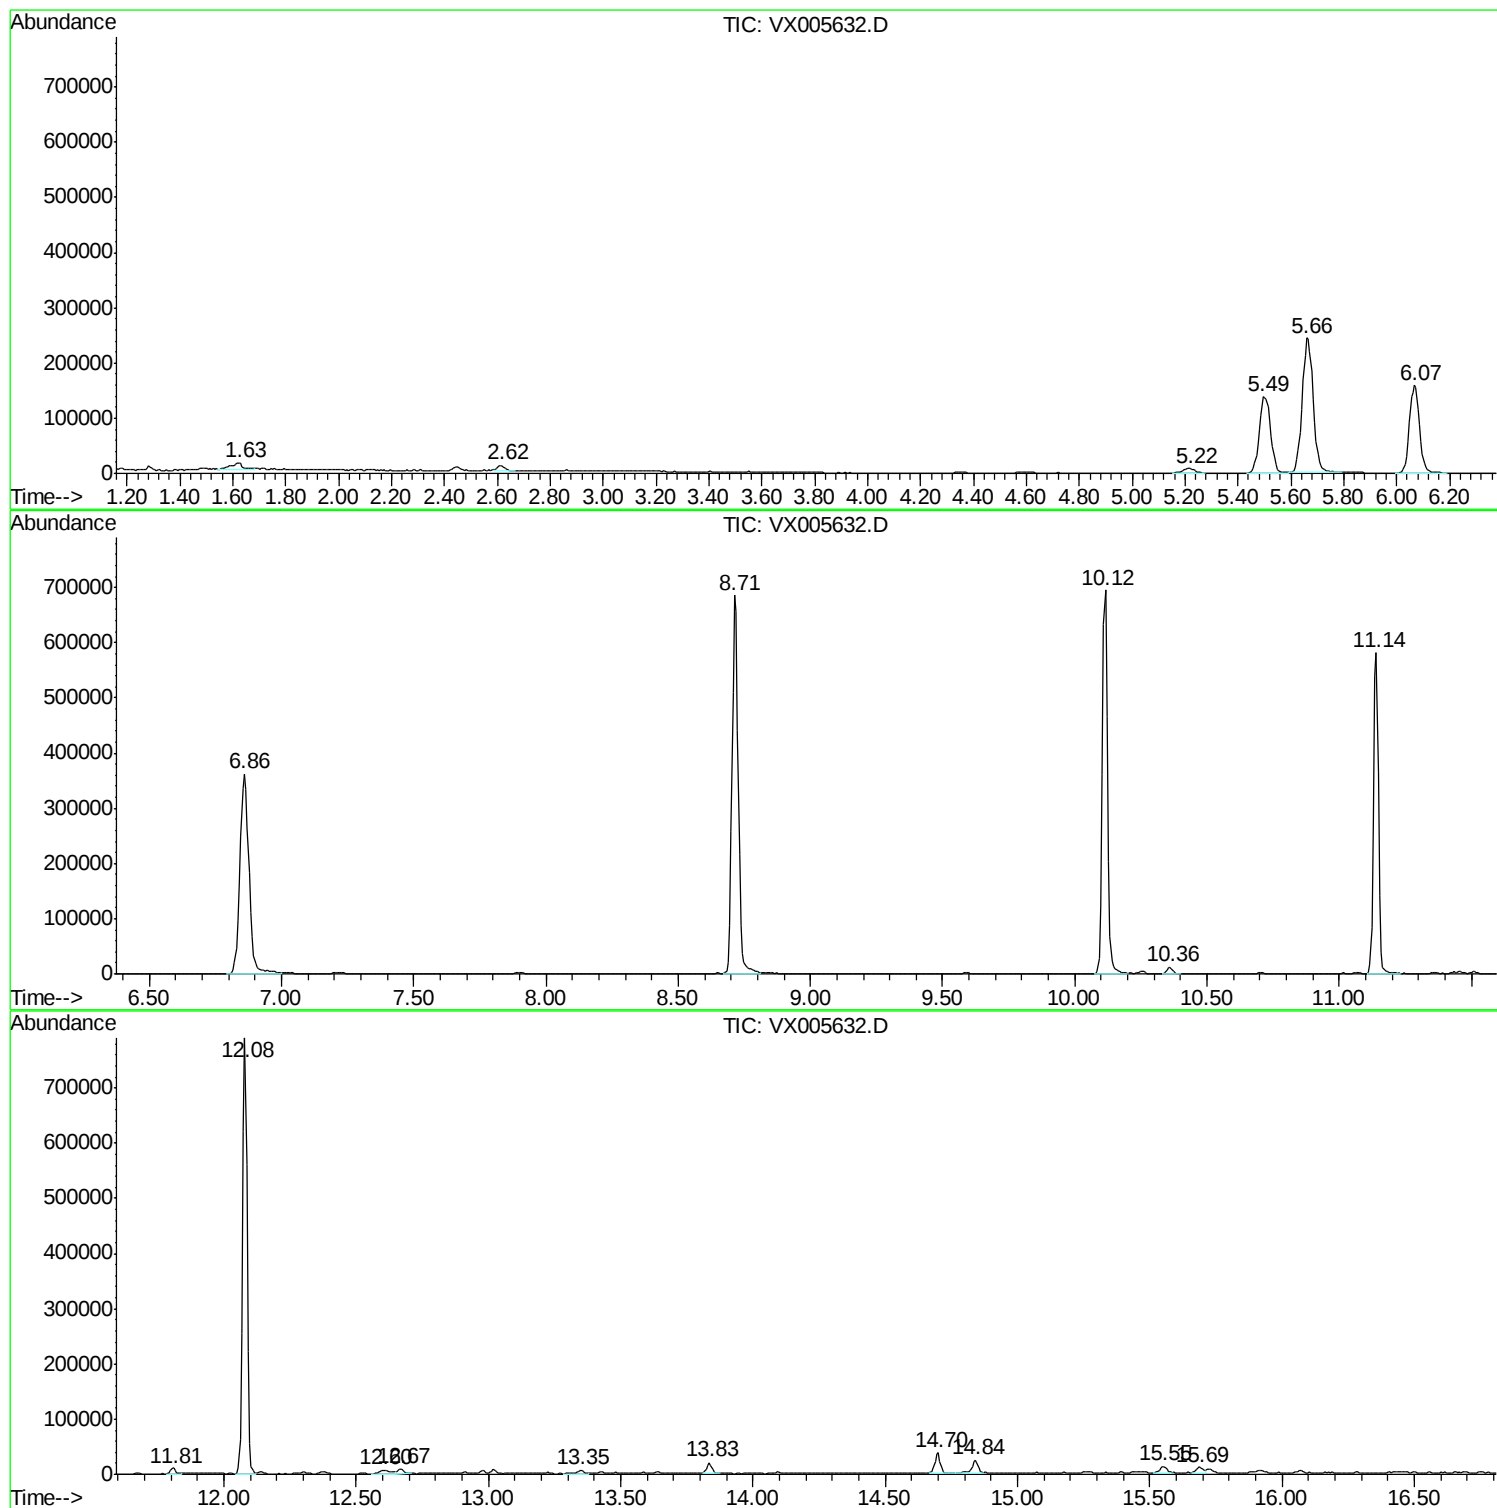

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX102618\
Data File : VX005632.D
Acq On : 27 Oct 2018 04:14
Operator : JC/MD
Sample : J5696-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DL-SW-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX102618\
Data File : VX005632.D
Acq On : 27 Oct 2018 04:14
Operator : JC/MD
Sample : J5696-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DL-SW-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc