


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX102618\
Data File : VX005625.D
Acq On : 27 Oct 2018 00:41
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102418W.M
Title : SW846 8260
Last Update : Thu Oct 25 02:52:45 2018

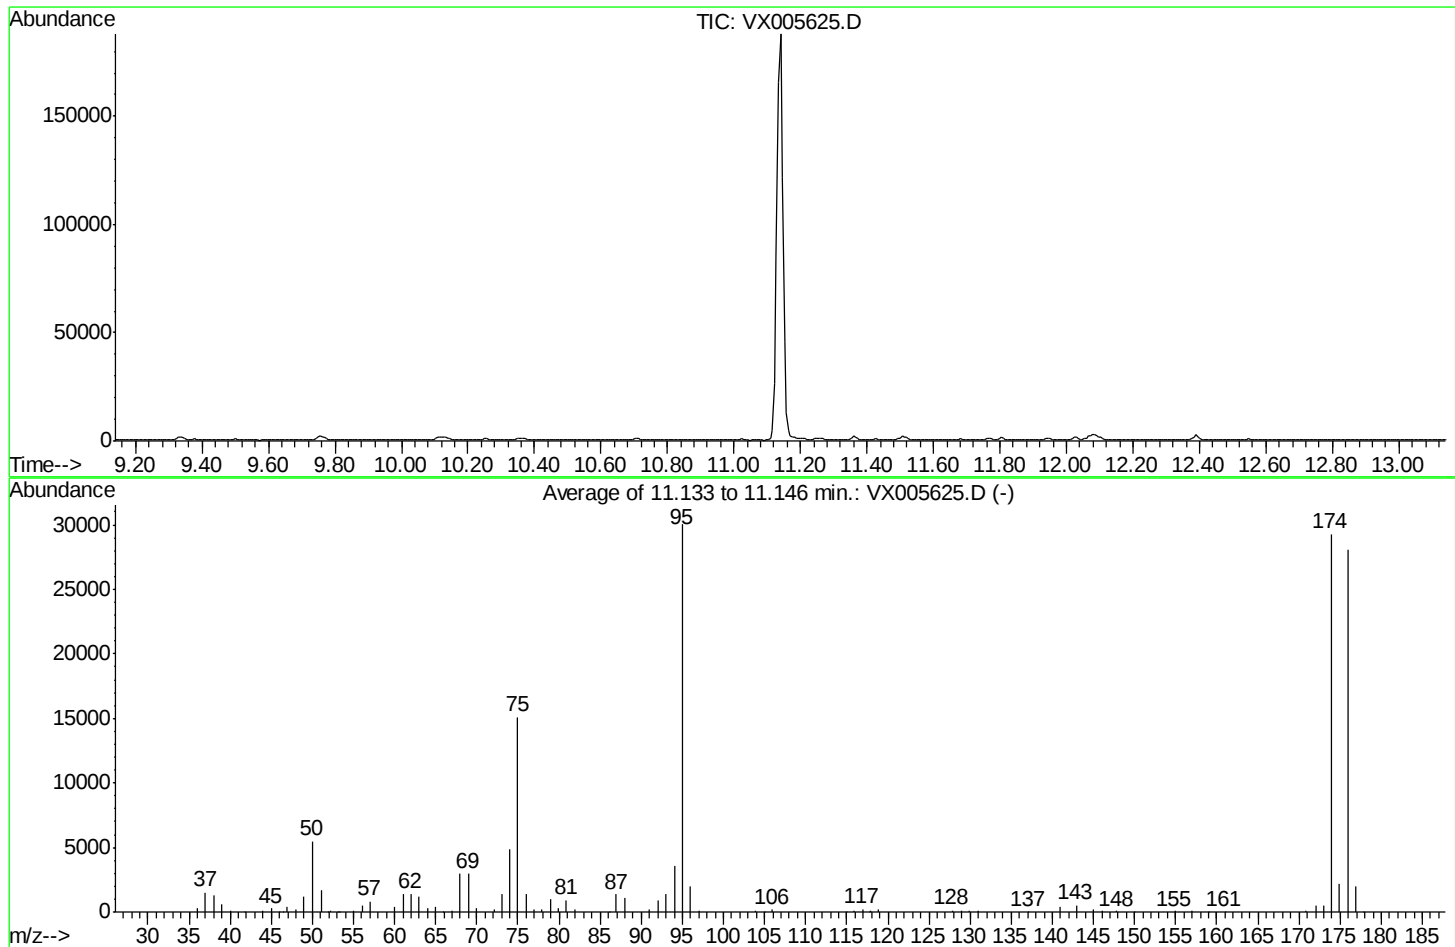

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	5504	PASS
75	95	30	60	50.2	15079	PASS
95	95	100	100	100.0	30037	PASS
96	95	5	9	6.5	1959	PASS
173	174	0.00	2	1.6	481	PASS
174	95	50	100	97.5	29298	PASS
175	174	5	9	7.5	2187	PASS
176	174	95	101	96.0	28114	PASS
177	176	5	9	7.1	1991	PASS