


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX102620\
Data File : VX019115.D
Acq On : 26 Oct 2020 09:23
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X102320W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Mon Oct 26 11:58:08 2020

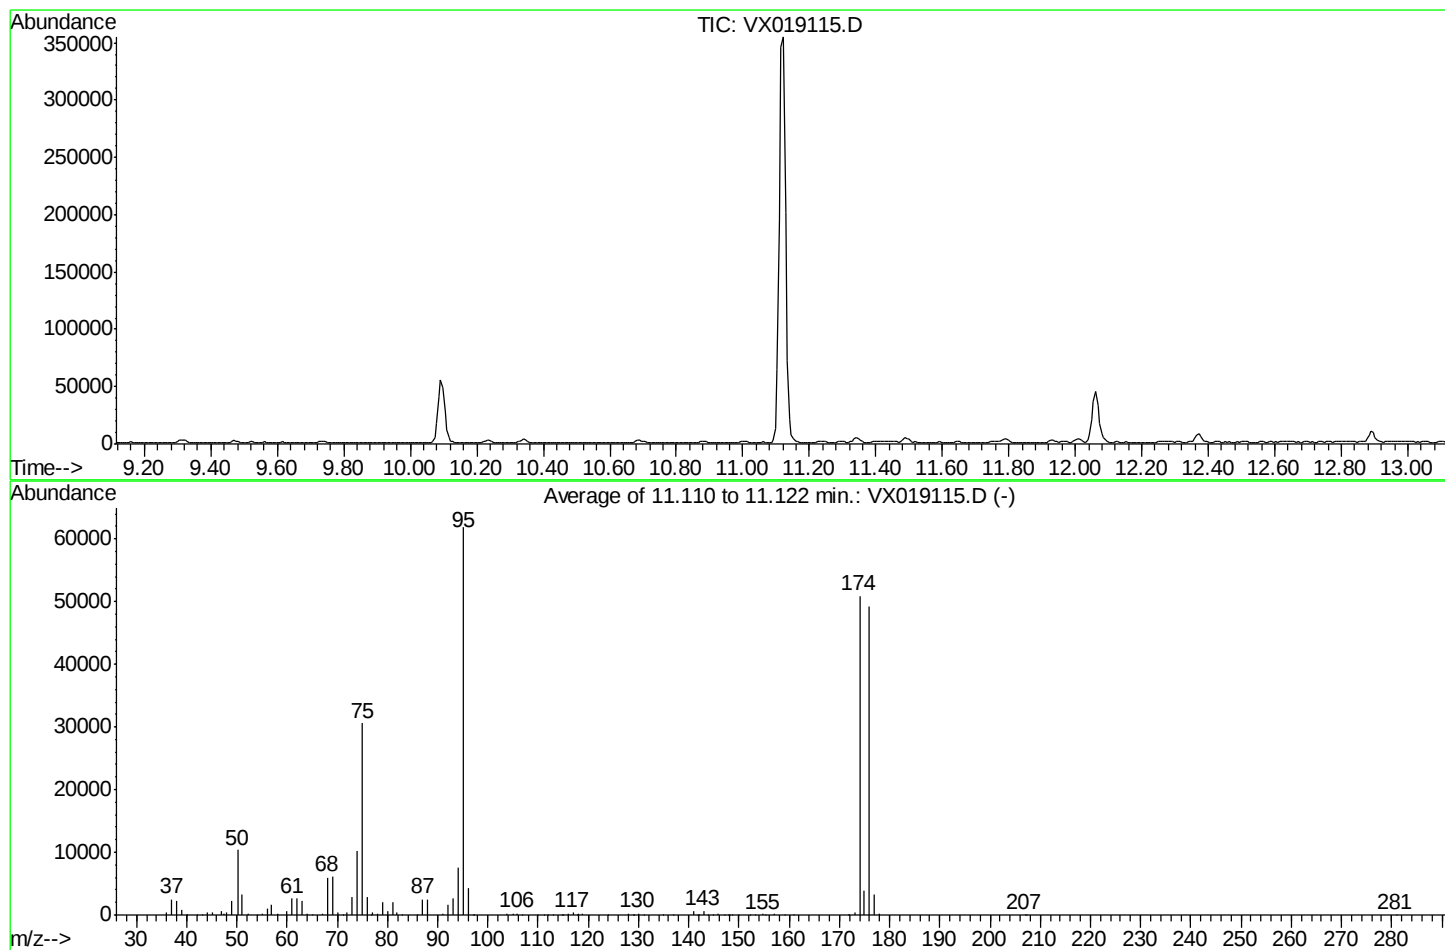

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	10343	PASS
75	95	30	60	49.4	30578	PASS
95	95	100	100	100.0	61842	PASS
96	95	5	9	7.1	4393	PASS
173	174	0.00	2	0.9	441	PASS
174	95	50	100	82.3	50912	PASS
175	174	5	9	7.6	3878	PASS
176	174	95	101	96.5	49154	PASS
177	176	5	9	6.5	3211	PASS